
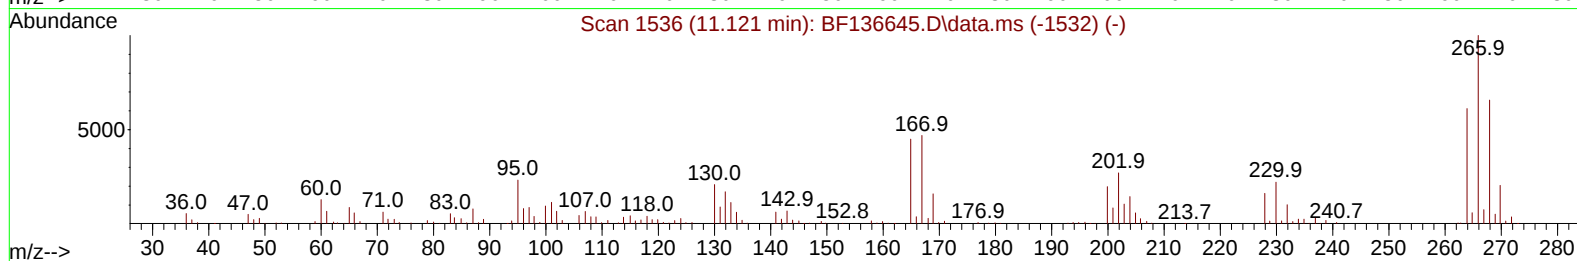
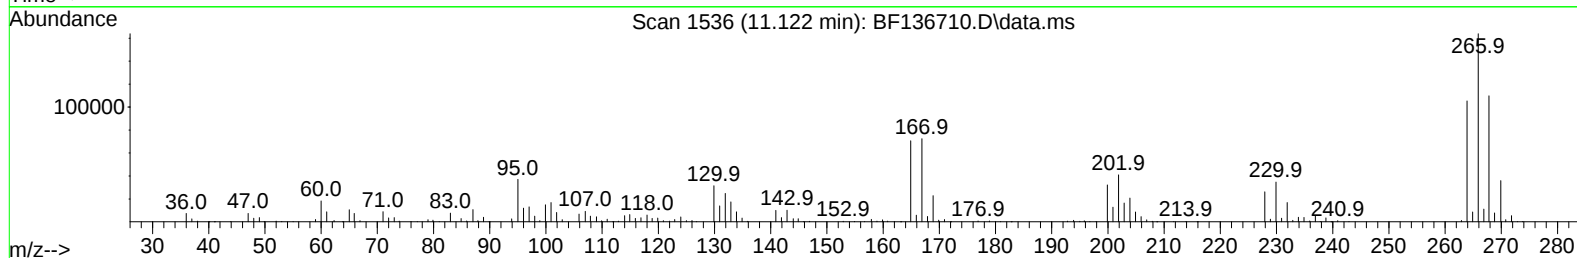


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122623\
 Data File : BF136710.D
 Acq On : 26 Dec 2023 10:13
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 11:14:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 21 01:54:25 2023
 Response via : Initial Calibration

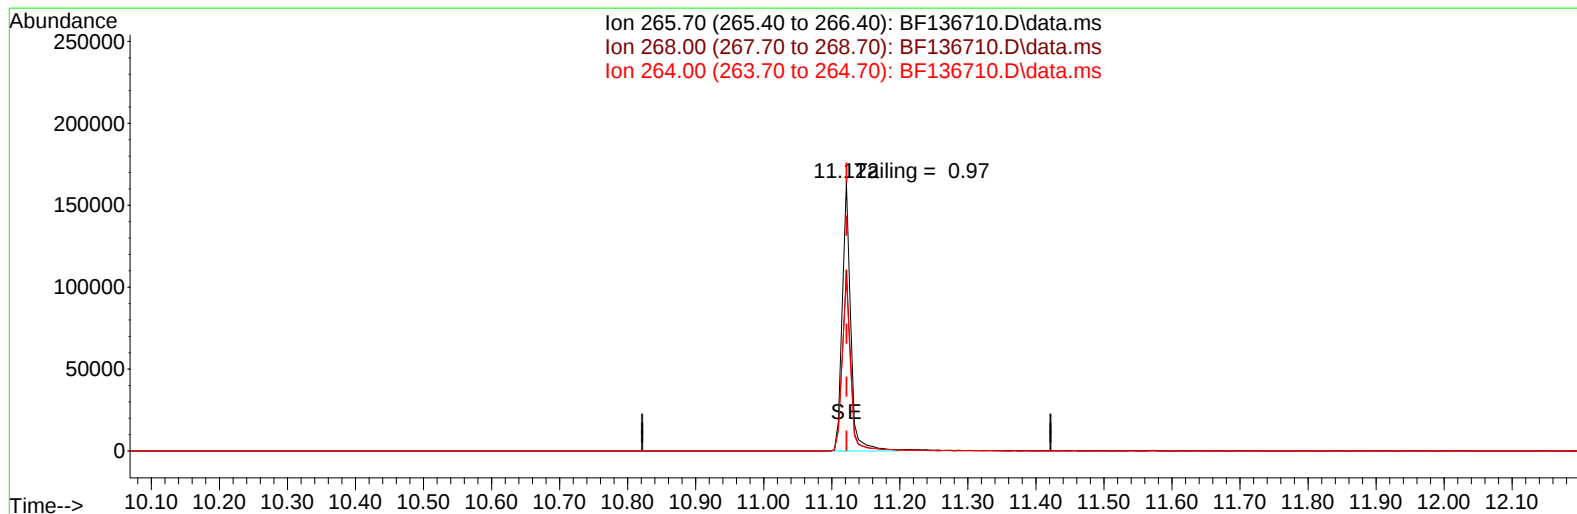

TIC: BF136710.D\data.ms

(70) Pentachlorophenol (C)




11.122min (+ 0.000) 39589.00 ng

response 142509

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	67.02
264.00	61.20	64.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122623\
Data File : BF136710.D
Acq On : 26 Dec 2023 10:13
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 11:14:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

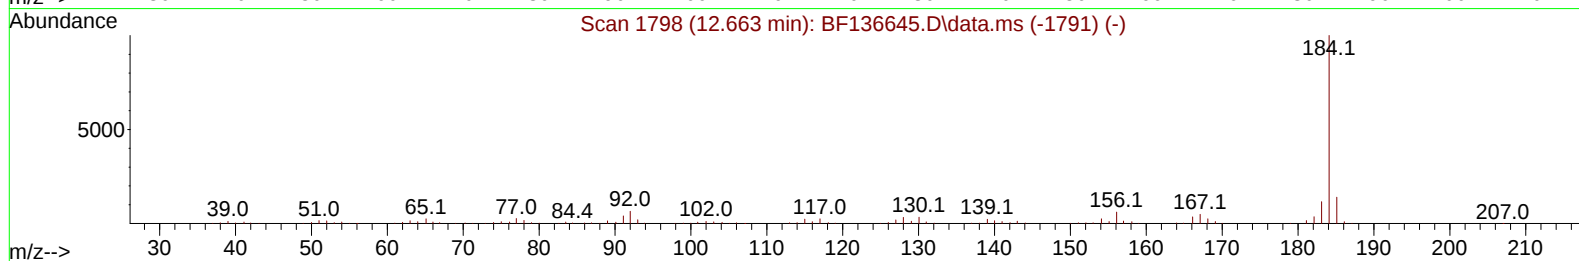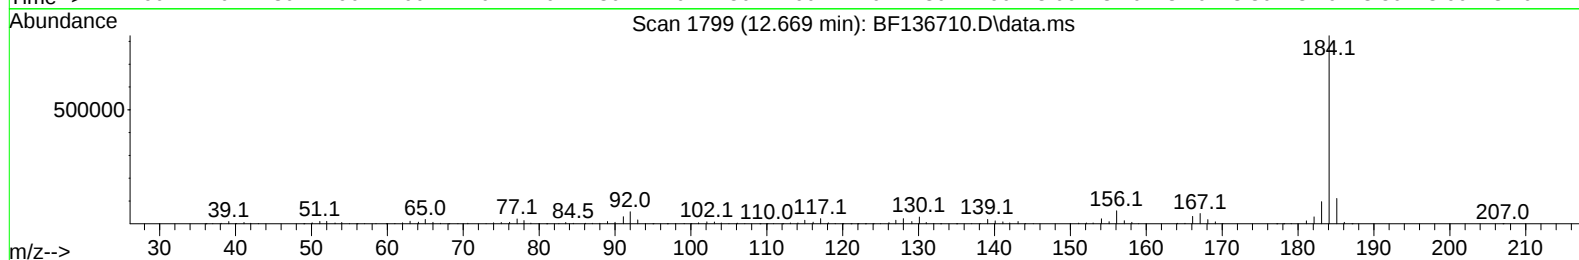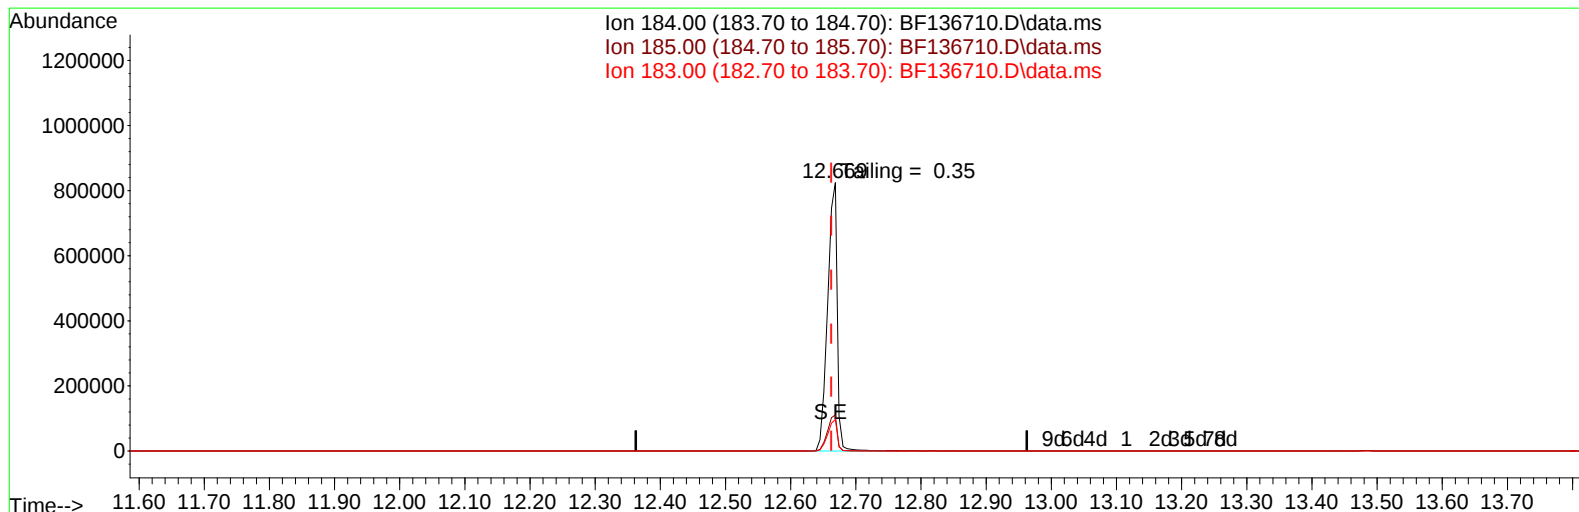

TIC: BF136710.D\data.ms

(77) Benzidine

12.669min (+ 0.006) 224880.85 ng m

response 848739

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.43
183.00	11.60	11.75
0.00	0.00	0.00