

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122623\
 Data File : BF136712.D
 Acq On : 26 Dec 2023 11:15
 Operator : CG\JU
 Sample : PB157949BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB157949BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136712.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.057	501	505	514	rBV2	55159	85800	2.52%	0.432%
2	5.440	565	570	573	rBV	2618967	2816660	82.72%	14.174%
3	6.439	734	740	743	rBV	2412793	2818177	82.76%	14.182%
4	6.786	795	799	802	rBV	636434	511725	15.03%	2.575%
5	7.351	889	895	898	rBV	1793508	1879300	55.19%	9.457%
6	8.063	1011	1016	1019	rBV	793711	674792	19.82%	3.396%
7	9.145	1193	1200	1203	rBV	3642277	3405176	100.00%	17.136%
8	9.816	1310	1314	1318	rBV	817693	743556	21.84%	3.742%
9	10.616	1445	1450	1453	rBV	1987157	1937212	56.89%	9.748%
10	11.310	1564	1568	1572	rBV	955364	771877	22.67%	3.884%
11	12.910	1835	1840	1843	rBV	2982743	3234810	95.00%	16.278%
12	13.963	2015	2019	2023	rBV	602741	542890	15.94%	2.732%
13	15.445	2266	2271	2275	rBV	365356	449933	13.21%	2.264%




Sum of corrected areas: 19871908

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122623\
Data File : BF136712.D
Acq On : 26 Dec 2023 11:15
Operator : CG\JU
Sample : PB157949BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157949BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

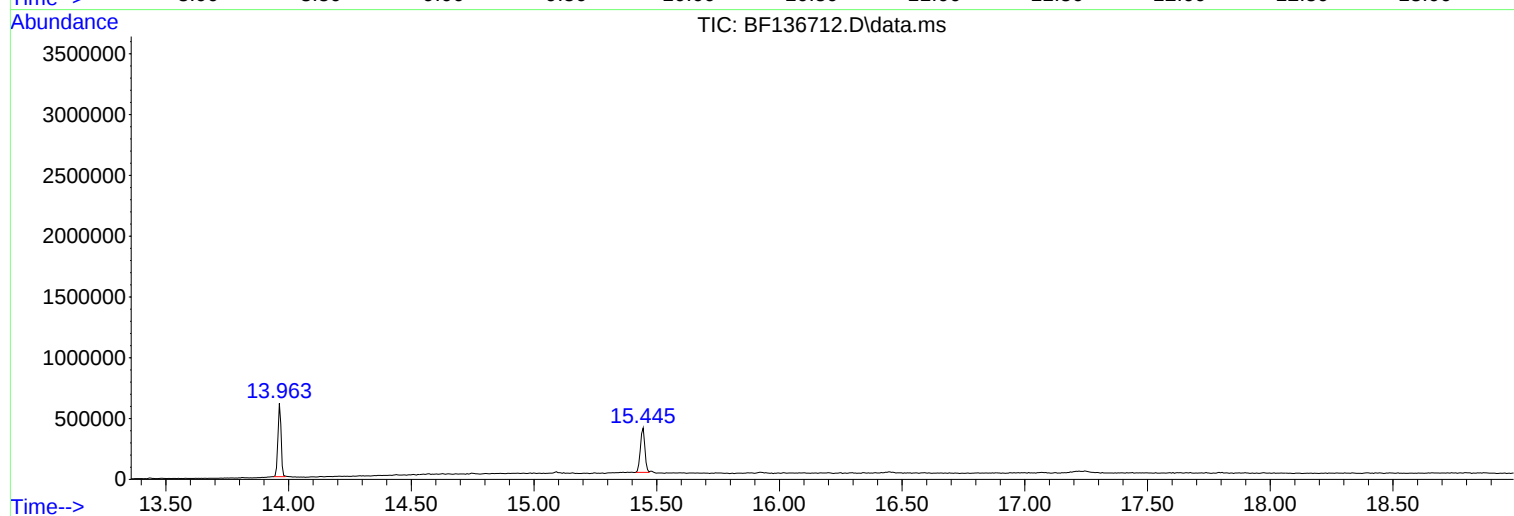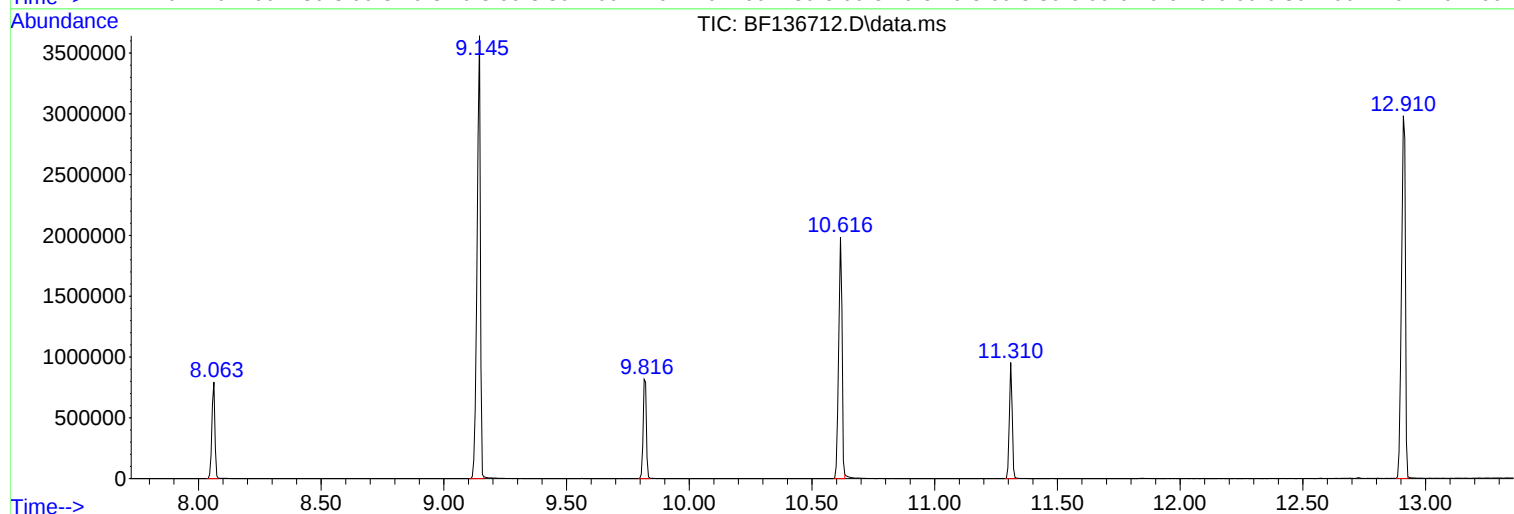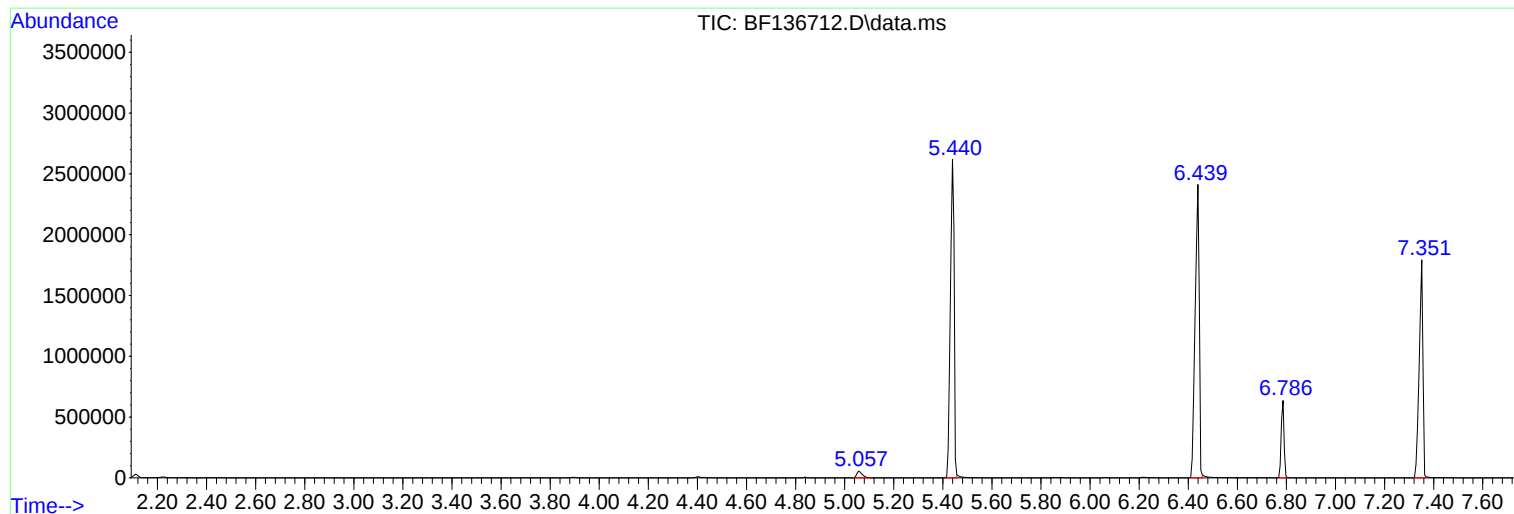

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122623\
Data File : BF136712.D
Acq On : 26 Dec 2023 11:15
Operator : CG\JU
Sample : PB157949BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157949BL









Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
5.057	3.35 ng	85800	1,4-Dichlorobenzene-d4			6.786

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56	
2	Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	40	
3	2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	33	
4	3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33	
5	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	28	

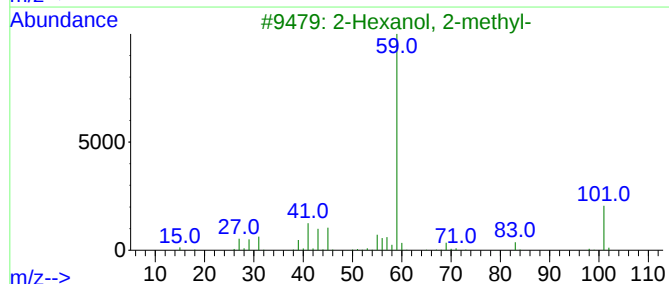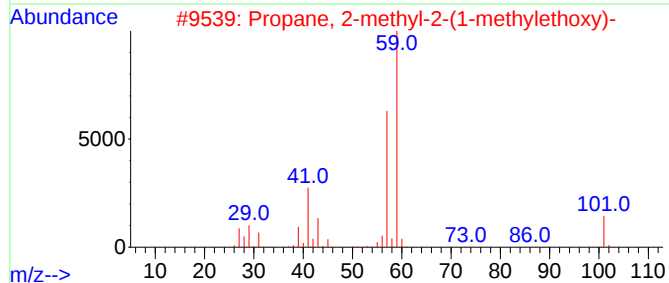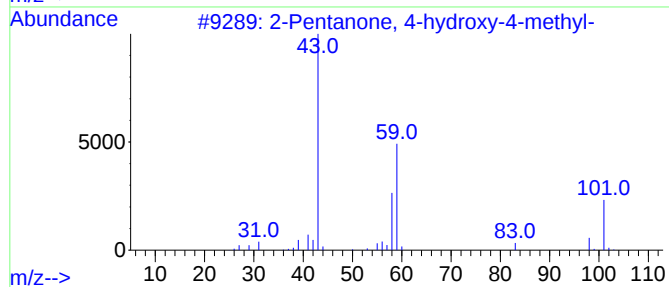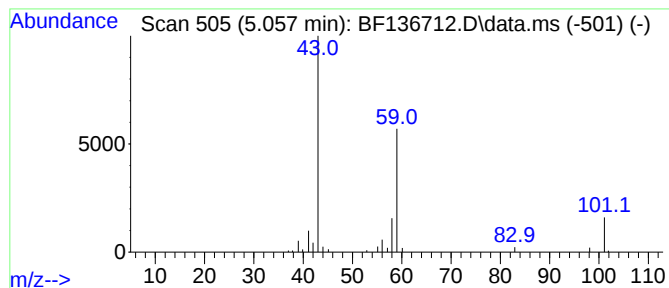

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122623\
Data File : BF136712.D
Acq On : 26 Dec 2023 11:15
Operator : CG\JU
Sample : PB157949BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157949BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.057	3.4	ng	85800	1	6.786	511725	20.0