
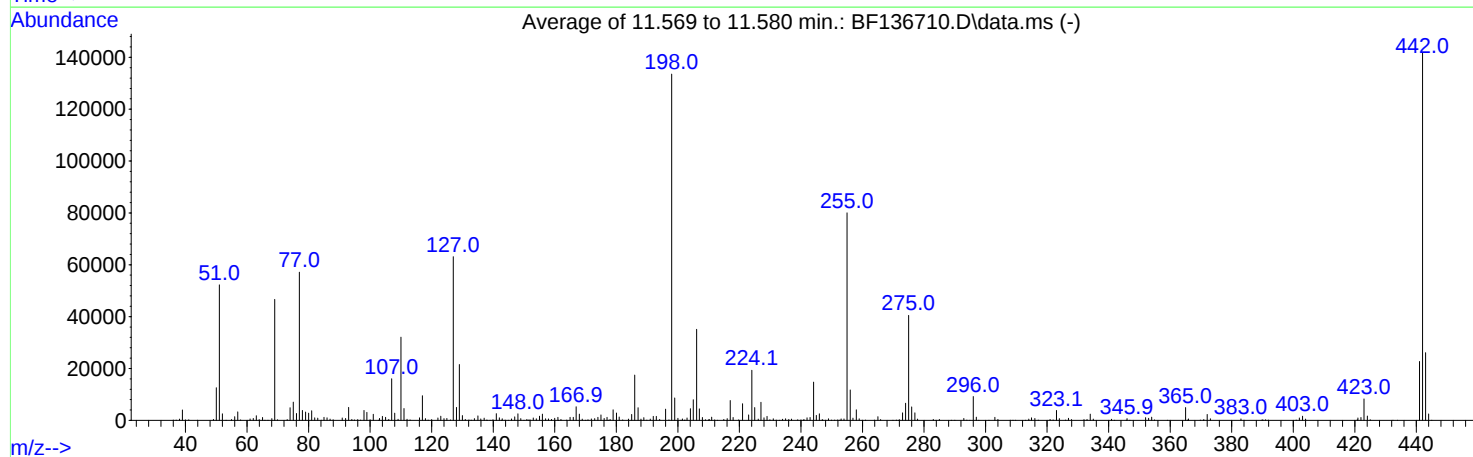


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122623\
Data File : BF136710.D
Acq On : 26 Dec 2023 10:13
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 21 01:54:25 2023

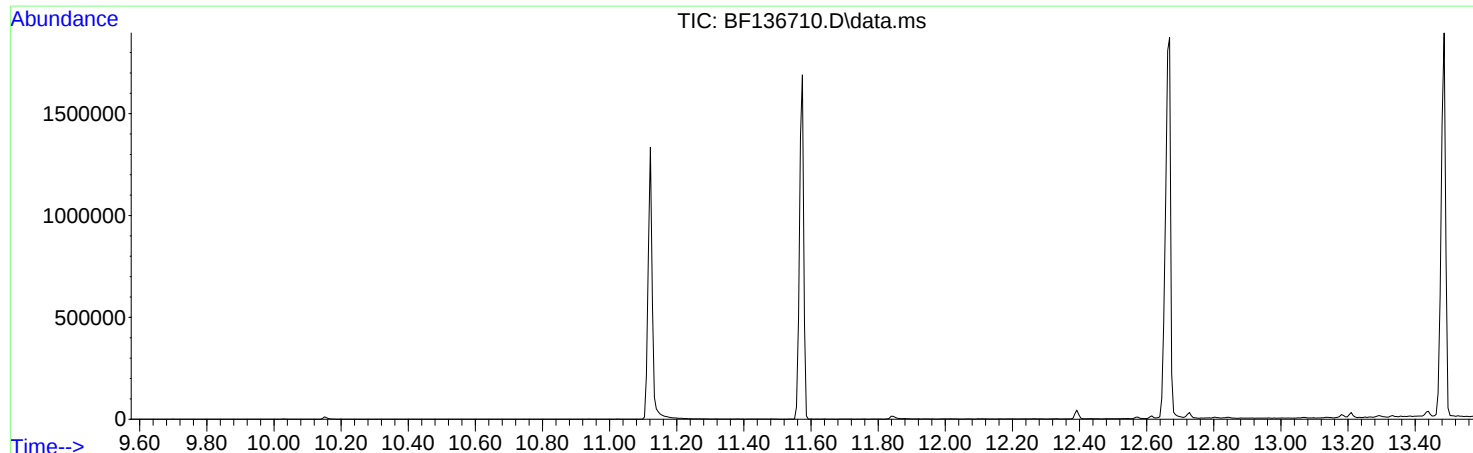




AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	52247	PASS
68	69	0.00	2	1.5	711	PASS
69	198	0.00	100	34.9	46632	PASS
70	69	0.00	2	0.6	264	PASS
127	198	10	80	47.3	63104	PASS
197	198	0.00	2	0.1	185	PASS
198	198	100	100	100.0	133552	PASS
199	198	5	9	6.5	8655	PASS
275	198	10	60	30.3	40501	PASS
365	198	1	100	3.7	4912	PASS
441	198	0.01	100	17.0	22741	PASS
442	442	50	100	100.0	141864	PASS
443	442	15	24	18.4	26125	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122623\
Data File : BF136710.D
Acq On : 26 Dec 2023 10:13
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 26 11:14:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

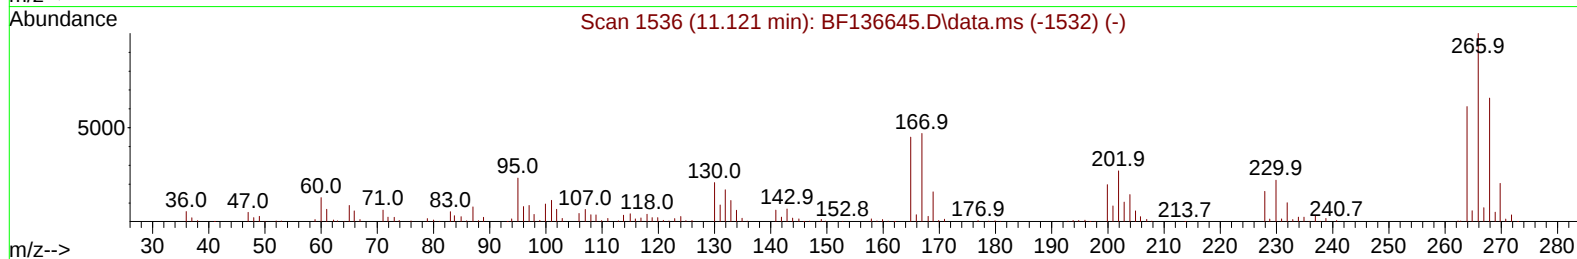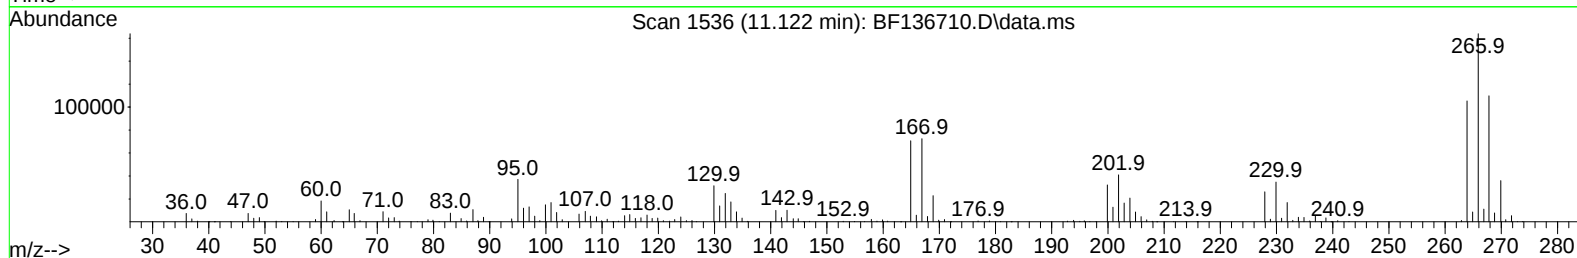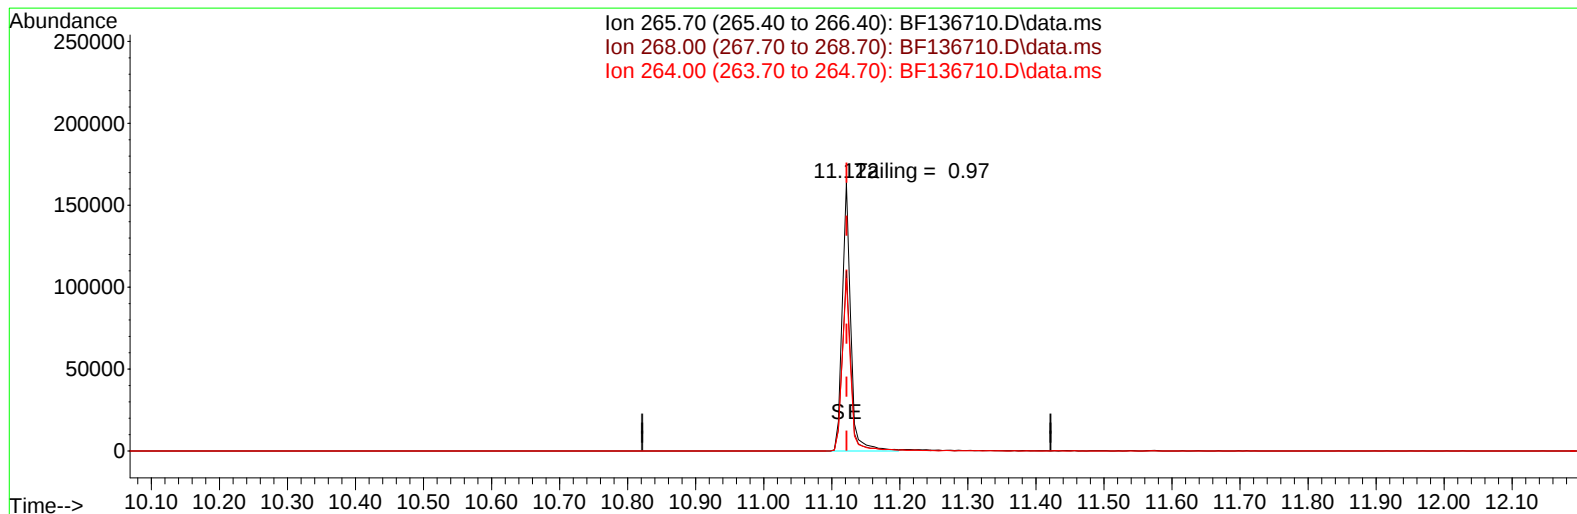

TIC: BF136710.D\data.ms

(70) Pentachlorophenol (C)

11.122min (+ 0.000) 39589.00 ng




response 142509

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	67.02
264.00	61.20	64.31
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122623\  
Data File : BF136710.D  
Acq On    : 26 Dec 2023  10:13  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 26 11:14:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

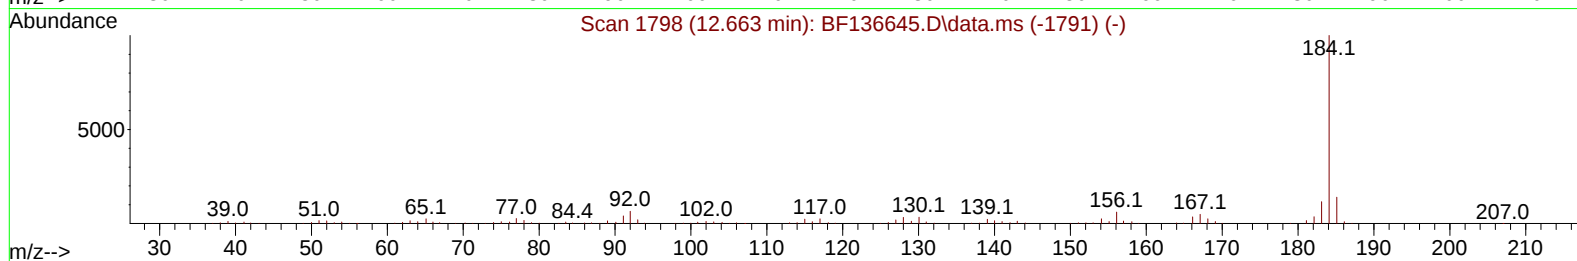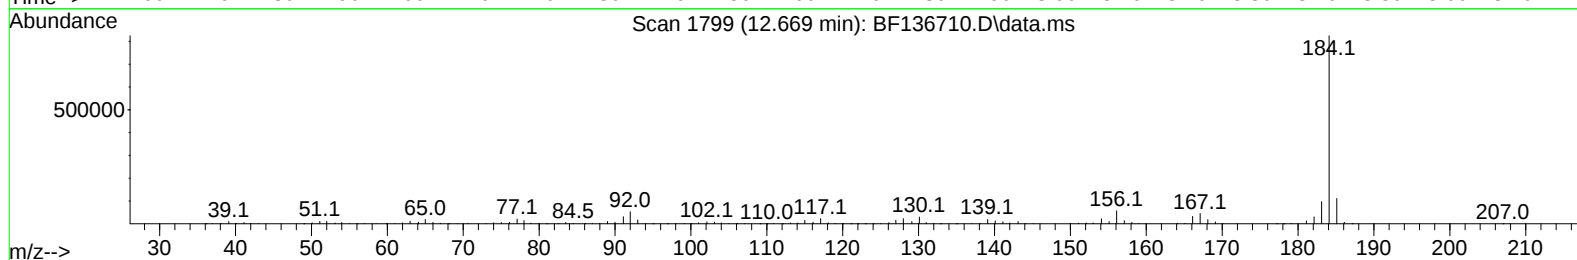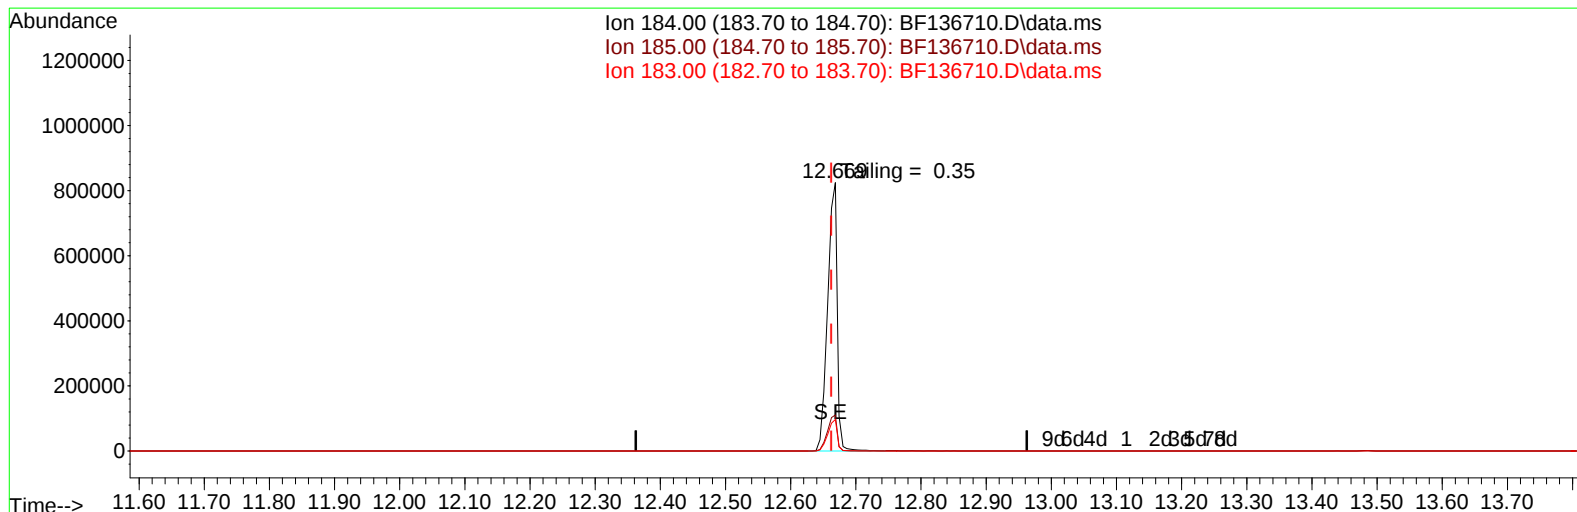

TIC: BF136710.D\data.ms

(77) Benzidine

12.669min (+ 0.006) 224880.85 ng m

response **848739**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.00	13.43
--------	-------	-------

183.00	11.60	11.75
--------	-------	-------

0.00 0.00 0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/26/2023	BNA_F	<u>BF136710.D</u>
Compound Name	Response	Retention Time
DDT	353918	13.486
DDD	6836	13.21
DDE	722	12.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7558	361476	2.09

Instrument :
BNA_F
ClientSampleId :
DFTPP