
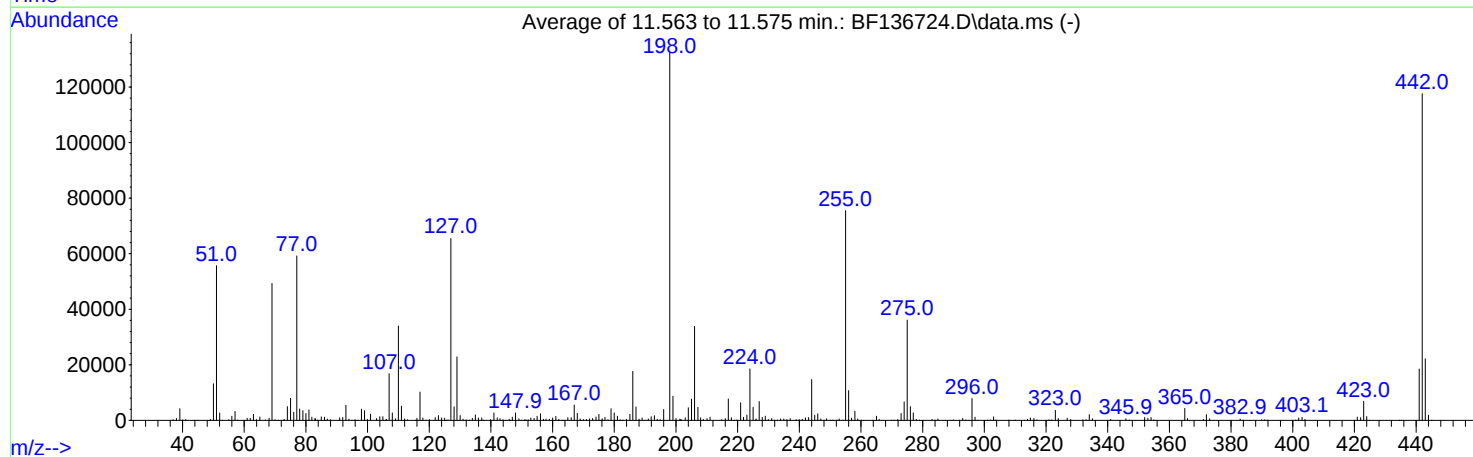


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122623\
 Data File : BF136724.D
 Acq On : 26 Dec 2023 17:50
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 21 01:54:25 2023

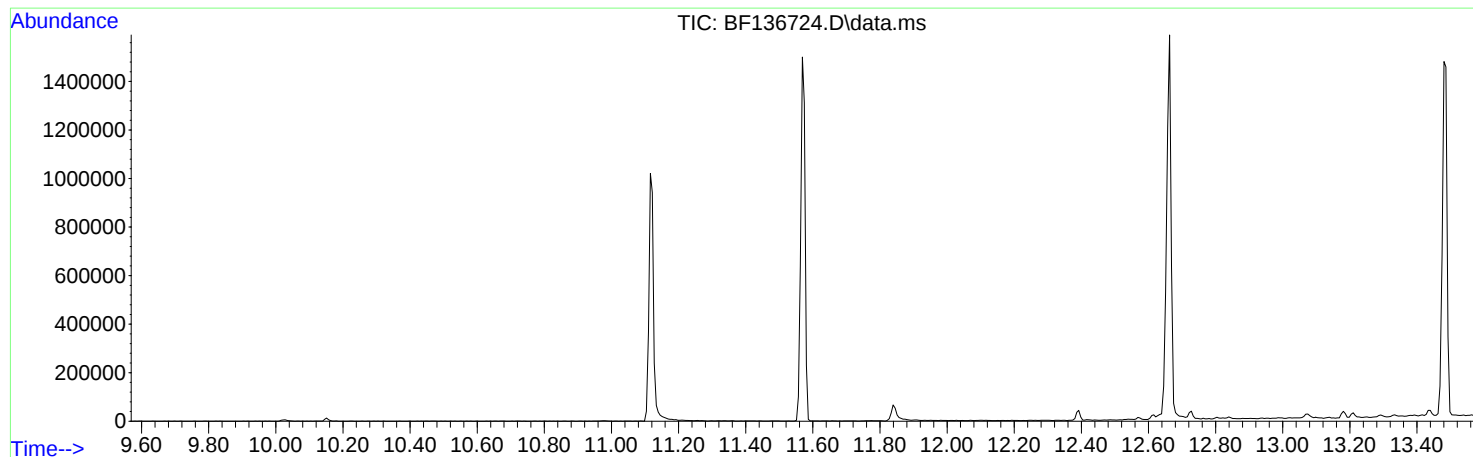




AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.1	55709	PASS
68	69	0.00	2	1.7	839	PASS
69	198	0.00	100	37.2	49323	PASS
70	69	0.00	2	0.5	229	PASS
127	198	10	80	49.5	65520	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	132440	PASS
199	198	5	9	6.6	8731	PASS
275	198	10	60	27.3	36116	PASS
365	198	1	100	3.3	4309	PASS
441	198	0.01	100	13.9	18466	PASS
442	442	50	100	100.0	117579	PASS
443	442	15	24	18.9	22168	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122623\
 Data File : BF136724.D
 Acq On : 26 Dec 2023 17:50
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 27 03:51:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 21 01:54:25 2023
 Response via : Initial Calibration

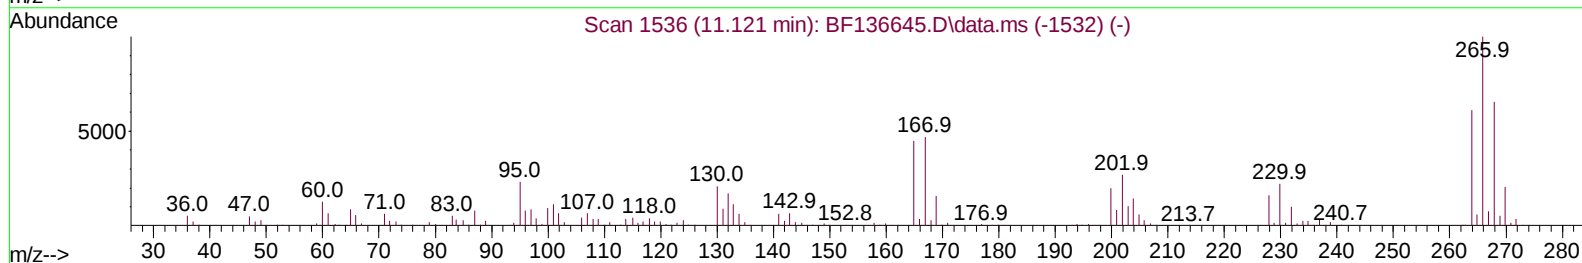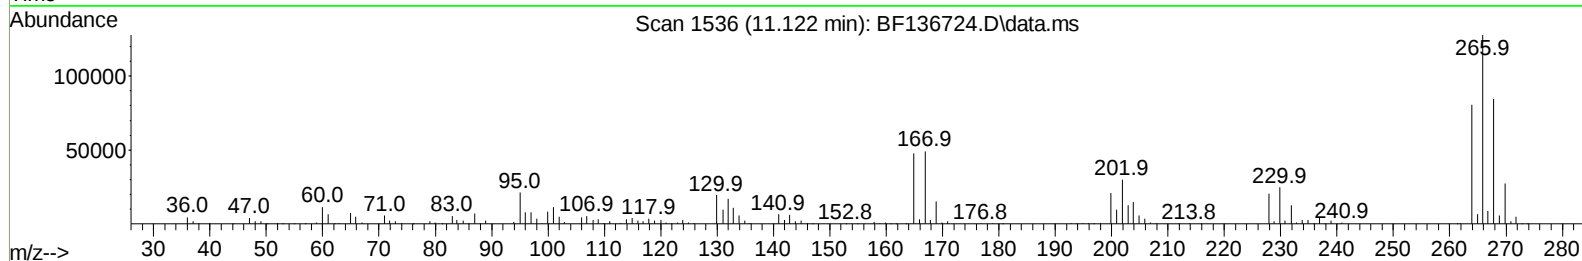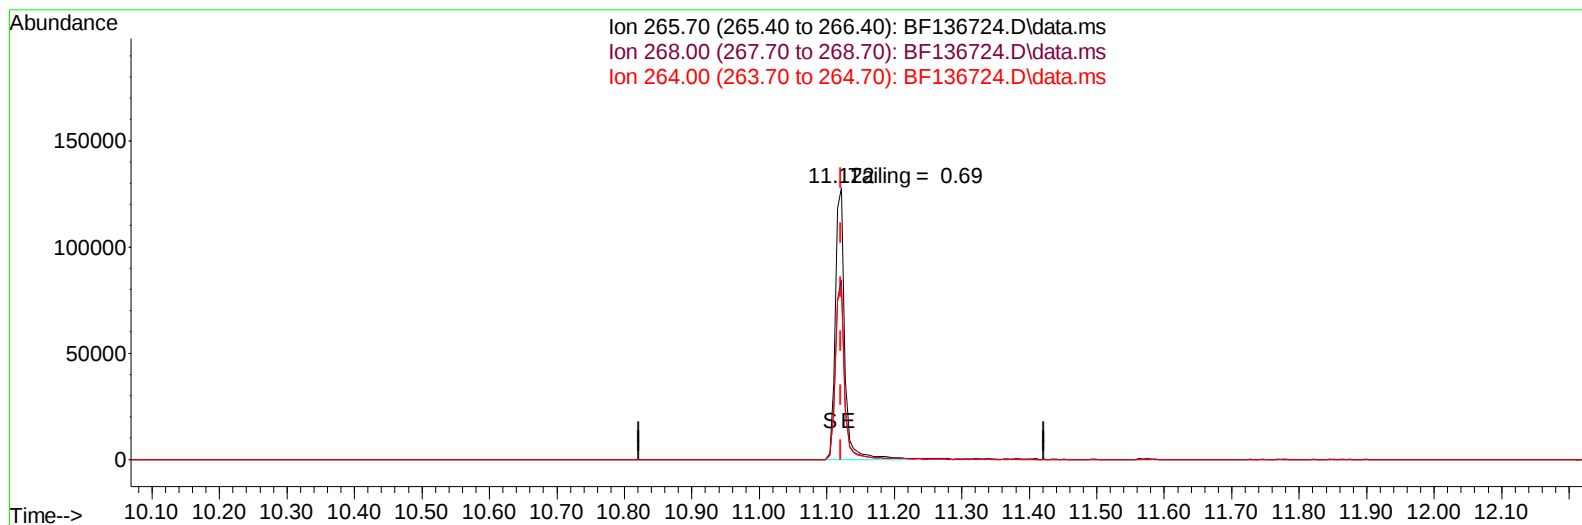

TIC: BF136724.D\data.ms




(70) Pentachlorophenol (C)**11.122min (+ 0.000) 42468.38 ng****response 125925**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	66.11
264.00	61.20	63.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122623\
Data File : BF136724.D
Acq On : 26 Dec 2023 17:50
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 27 03:51:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

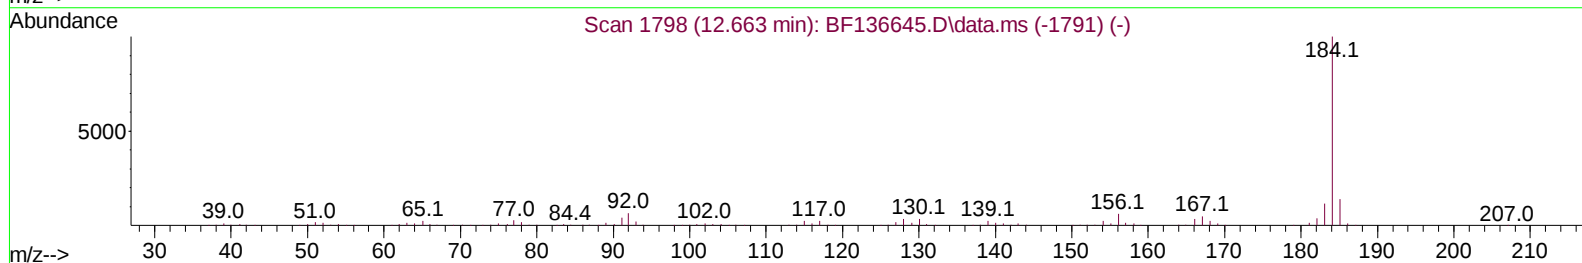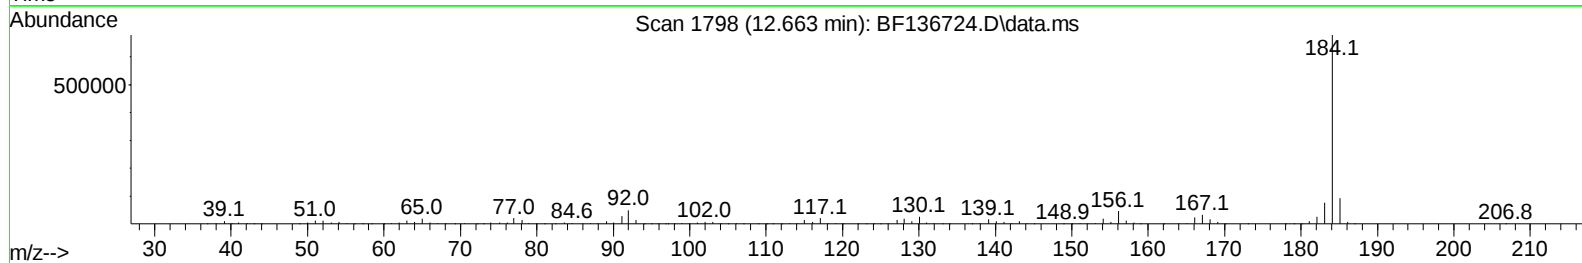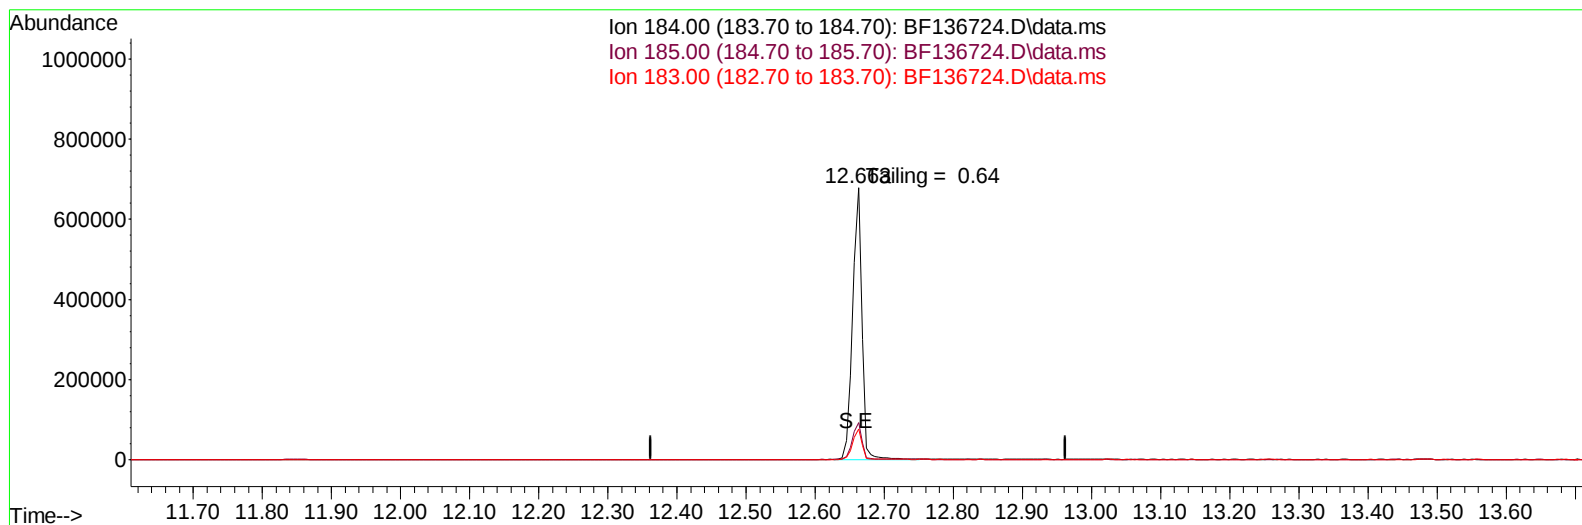

TIC: BF136724.D\data.ms

(77) Benzidine

12.663min (-12.663) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	14.00	0.00#
183.00	11.60	0.00#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/26/2023	BNA_F	<u>BF136724.D</u>
Compound Name	Response	Retention Time
DDT	297959	13.486
DDD	8378	13.18
DDE	845	12.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9223	307182	3.00

Instrument :
BNA_F
ClientSampleId :
DFTPP