

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF122718\
 Data File : BF111777.D
 Acq On : 27 Dec 2018 21:55
 Operator : JU/SJ
 Sample : J6188-06MSD
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BU-03-122118MSD

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.863	127	132	140	rVB	276717	352421	7.43%	0.239%
2	2.975	145	151	158	rVB	288026	381078	8.04%	0.258%
3	3.510	233	242	251	rBV	328464	641442	13.53%	0.435%
4	3.581	251	254	269	rVB	490370	822091	17.33%	0.557%
5	4.675	436	440	445	rVB	126682	137091	2.89%	0.093%
6	4.734	445	450	454	rBV	209862	219810	4.63%	0.149%
7	5.093	507	511	514	rBV	128959	126086	2.66%	0.085%
8	5.145	514	520	527	rVB	883916	1327993	28.00%	0.900%
9	5.557	585	590	593	rBV	3151494	3073214	64.80%	2.082%
10	6.457	739	743	747	rBV	1105120	972597	20.51%	0.659%
11	6.557	755	760	769	rBV2	2794548	3928394	82.83%	2.661%
12	6.640	769	774	777	rVB	1234964	970405	20.46%	0.657%
13	6.687	777	782	788	rBV2	3307108	4742611	100.00%	3.213%
14	6.851	806	810	813	rBV	1941937	1535548	32.38%	1.040%
15	6.910	816	820	821	rBV	941925	937615	19.77%	0.635%
16	6.928	821	823	826	rVB	1928468	1425771	30.06%	0.966%
17	7.069	844	847	852	rVB2	3026356	4313962	90.96%	2.922%
18	7.175	859	865	870	rBV2	2252845	2762054	58.24%	1.871%
19	7.316	883	889	897	rBV3	3065443	4141047	87.32%	2.805%
20	7.422	903	907	910	rBV	1178823	981442	20.69%	0.665%
21	7.469	910	915	917	rVV	2275709	2744827	57.88%	1.859%
22	7.487	917	918	921	rVB	1488164	697825	14.71%	0.473%
23	7.586	930	935	939	rBV	1963281	1759289	37.10%	1.192%
24	7.728	953	959	962	rBV	1580263	1558509	32.86%	1.056%
25	7.804	967	972	975	rBV	953350	864217	18.22%	0.585%
26	7.845	975	979	983	rBV	1682700	1522885	32.11%	1.032%
27	7.934	983	994	1000	rBV2	1388547	1688626	35.61%	1.144%
28	8.051	1009	1014	1018	rBV	1513357	1292751	27.26%	0.876%
29	8.134	1023	1028	1031	rBV	1664529	1585719	33.44%	1.074%
30	8.192	1033	1038	1039	rBV	1053026	1014372	21.39%	0.687%
31	8.210	1039	1041	1045	rVV	2088251	1936732	40.84%	1.312%
32	8.257	1045	1049	1051	rVV	107359	138751	2.93%	0.094%
33	8.286	1051	1054	1057	rVV	178996	213953	4.51%	0.145%
34	8.328	1057	1061	1065	rVB	1630689	1475752	31.12%	1.000%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF122718\
 Data File : BF111777.D
 Acq On : 27 Dec 2018 21:55
 Operator : JU/SJ
 Sample : J6188-06MSD
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BU-03-122118MSD

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	8.610	1105	1109	1112	rBV	435873	482073	10.16%	0.327%
36	8.745	1127	1132	1135	rBV	1504164	1201257	25.33%	0.814%
37	8.845	1143	1149	1153	rBV	1943991	1840572	38.81%	1.247%
38	8.904	1154	1159	1162	rVV	2623664	2161130	45.57%	1.464%
39	8.957	1162	1168	1171	rVV	543062	491095	10.35%	0.333%
40	9.004	1171	1176	1179	rVV	2377467	2048858	43.20%	1.388%
41	9.069	1179	1187	1190	rVB2	1925063	2134376	45.00%	1.446%
42	9.186	1202	1207	1211	rBV2	1644767	1545820	32.59%	1.047%
43	9.228	1211	1214	1216	rVV	1376017	1151536	24.28%	0.780%
44	9.263	1216	1220	1223	rVB	4440931	3861454	81.42%	2.616%
45	9.363	1229	1237	1239	rBV	2578752	2255493	47.56%	1.528%
46	9.392	1239	1242	1245	rVV	2109172	1770265	37.33%	1.199%
47	9.480	1248	1257	1260	rBV	1161354	1073358	22.63%	0.727%
48	9.616	1274	1280	1282	rBV	753604	642686	13.55%	0.435%
49	9.657	1282	1287	1290	rVV	1731136	1584028	33.40%	1.073%
50	9.692	1290	1293	1295	rVV	786250	717333	15.13%	0.486%
51	9.722	1295	1298	1301	rVV	1119150	960422	20.25%	0.651%
52	9.775	1301	1307	1309	rVV	660678	588606	12.41%	0.399%
53	9.810	1309	1313	1316	rVB	2071798	1883240	39.71%	1.276%
54	9.886	1323	1326	1330	rVB	556772	482186	10.17%	0.327%
55	9.945	1330	1336	1339	rBV2	1065783	981430	20.69%	0.665%
56	9.980	1339	1342	1350	rVB	2551586	2223709	46.89%	1.506%
57	10.069	1352	1357	1358	rBV	1208686	1099585	23.19%	0.745%
58	10.086	1358	1360	1363	rVV	1103871	876738	18.49%	0.594%
59	10.122	1363	1366	1368	rVV	1055916	930497	19.62%	0.630%
60	10.151	1368	1371	1374	rVB	2172241	1778104	37.49%	1.205%
61	10.227	1379	1384	1388	rBV	1321424	1123488	23.69%	0.761%
62	10.275	1388	1392	1395	rVV	1224451	1107981	23.36%	0.751%
63	10.357	1400	1406	1409	rBV	1833647	1649777	34.79%	1.118%
64	10.386	1409	1411	1413	rVB	125088	92213	1.94%	0.062%
65	10.492	1421	1429	1433	rBV3	2739581	4449795	93.83%	3.014%
66	10.533	1433	1436	1439	rVV	154738	132149	2.79%	0.090%
67	10.598	1442	1447	1450	rVV	2241262	1930022	40.70%	1.307%
68	10.645	1450	1455	1458	rVB	1738829	1544987	32.58%	1.047%
69	10.739	1466	1471	1474	rBV	2426249	2254817	47.54%	1.528%
70	10.975	1506	1511	1514	rVB	1505064	1374027	28.97%	0.931%
71	11.045	1519	1523	1527	rBV	1634996	1386110	29.23%	0.939%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF122718\
Data File : BF111777.D
Acq On : 27 Dec 2018 21:55
Operator : JU/SJ
Sample : J6188-06MSD
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BU-03-122118MSD

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	11.127	1531	1537	1548	rVB2	1499436	1393745	29.39%	0.944%
73	11.239	1552	1556	1566	rBV	1423188	1263850	26.65%	0.856%
74	11.433	1584	1589	1590	rBV	975386	905981	19.10%	0.614%
75	11.457	1590	1593	1596	rVB	2575204	2077392	43.80%	1.407%
76	11.510	1598	1602	1605	rBV	2463704	2131285	44.94%	1.444%
77	11.663	1624	1628	1631	rVB	2023535	1739820	36.68%	1.179%
78	11.986	1679	1683	1686	rBV	2251731	1771859	37.36%	1.200%
79	12.645	1791	1795	1798	rBV	2422754	2084597	43.95%	1.412%
80	12.757	1810	1814	1818	rBV	372839	326149	6.88%	0.221%
81	12.874	1829	1834	1838	rBV	2383543	2154490	45.43%	1.460%
82	13.016	1853	1858	1861	rBV	4208947	3748632	79.04%	2.539%
83	13.174	1881	1885	1890	rBV	246797	254465	5.37%	0.172%
84	13.486	1934	1938	1941	rBV	1943762	1636772	34.51%	1.109%
85	13.516	1941	1943	1945	rVV	211813	182257	3.84%	0.123%
86	13.551	1945	1949	1952	rVB	2176736	1995537	42.08%	1.352%
87	14.015	2025	2028	2030	rBV	441756	367339	7.75%	0.249%
88	14.045	2030	2033	2034	rVV	2373983	2088799	44.04%	1.415%
89	14.063	2034	2036	2040	rVV2	2074567	2512439	52.98%	1.702%
90	14.098	2040	2042	2045	rVB	2173502	1724278	36.36%	1.168%
91	14.268	2068	2071	2075	rBV	626157	564460	11.90%	0.382%
92	14.474	2102	2106	2109	rVB2	352613	391798	8.26%	0.265%
93	14.657	2132	2137	2141	rBV	2002161	1840003	38.80%	1.247%
94	14.845	2167	2169	2177	rVB2	67622	74962	1.58%	0.051%
95	15.121	2211	2216	2218	rBV	1295414	1444195	30.45%	0.978%
96	15.151	2218	2221	2225	rVB	1405584	1418446	29.91%	0.961%
97	15.498	2275	2280	2285	rVB	1133951	1353277	28.53%	0.917%
98	15.557	2286	2290	2298	rVB	475534	672116	14.17%	0.455%
99	17.074	2539	2548	2556	rVB3	966846	2286540	48.21%	1.549%
100	17.521	2617	2624	2633	rVB	525981	1109501	23.39%	0.752%


Sum of corrected areas: 147613081

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF122718\
Data File : BF111777.D
Acq On : 27 Dec 2018 21:55
Operator : JU/SJ
Sample : J6188-06MSD
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BU-03-122118MSD

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

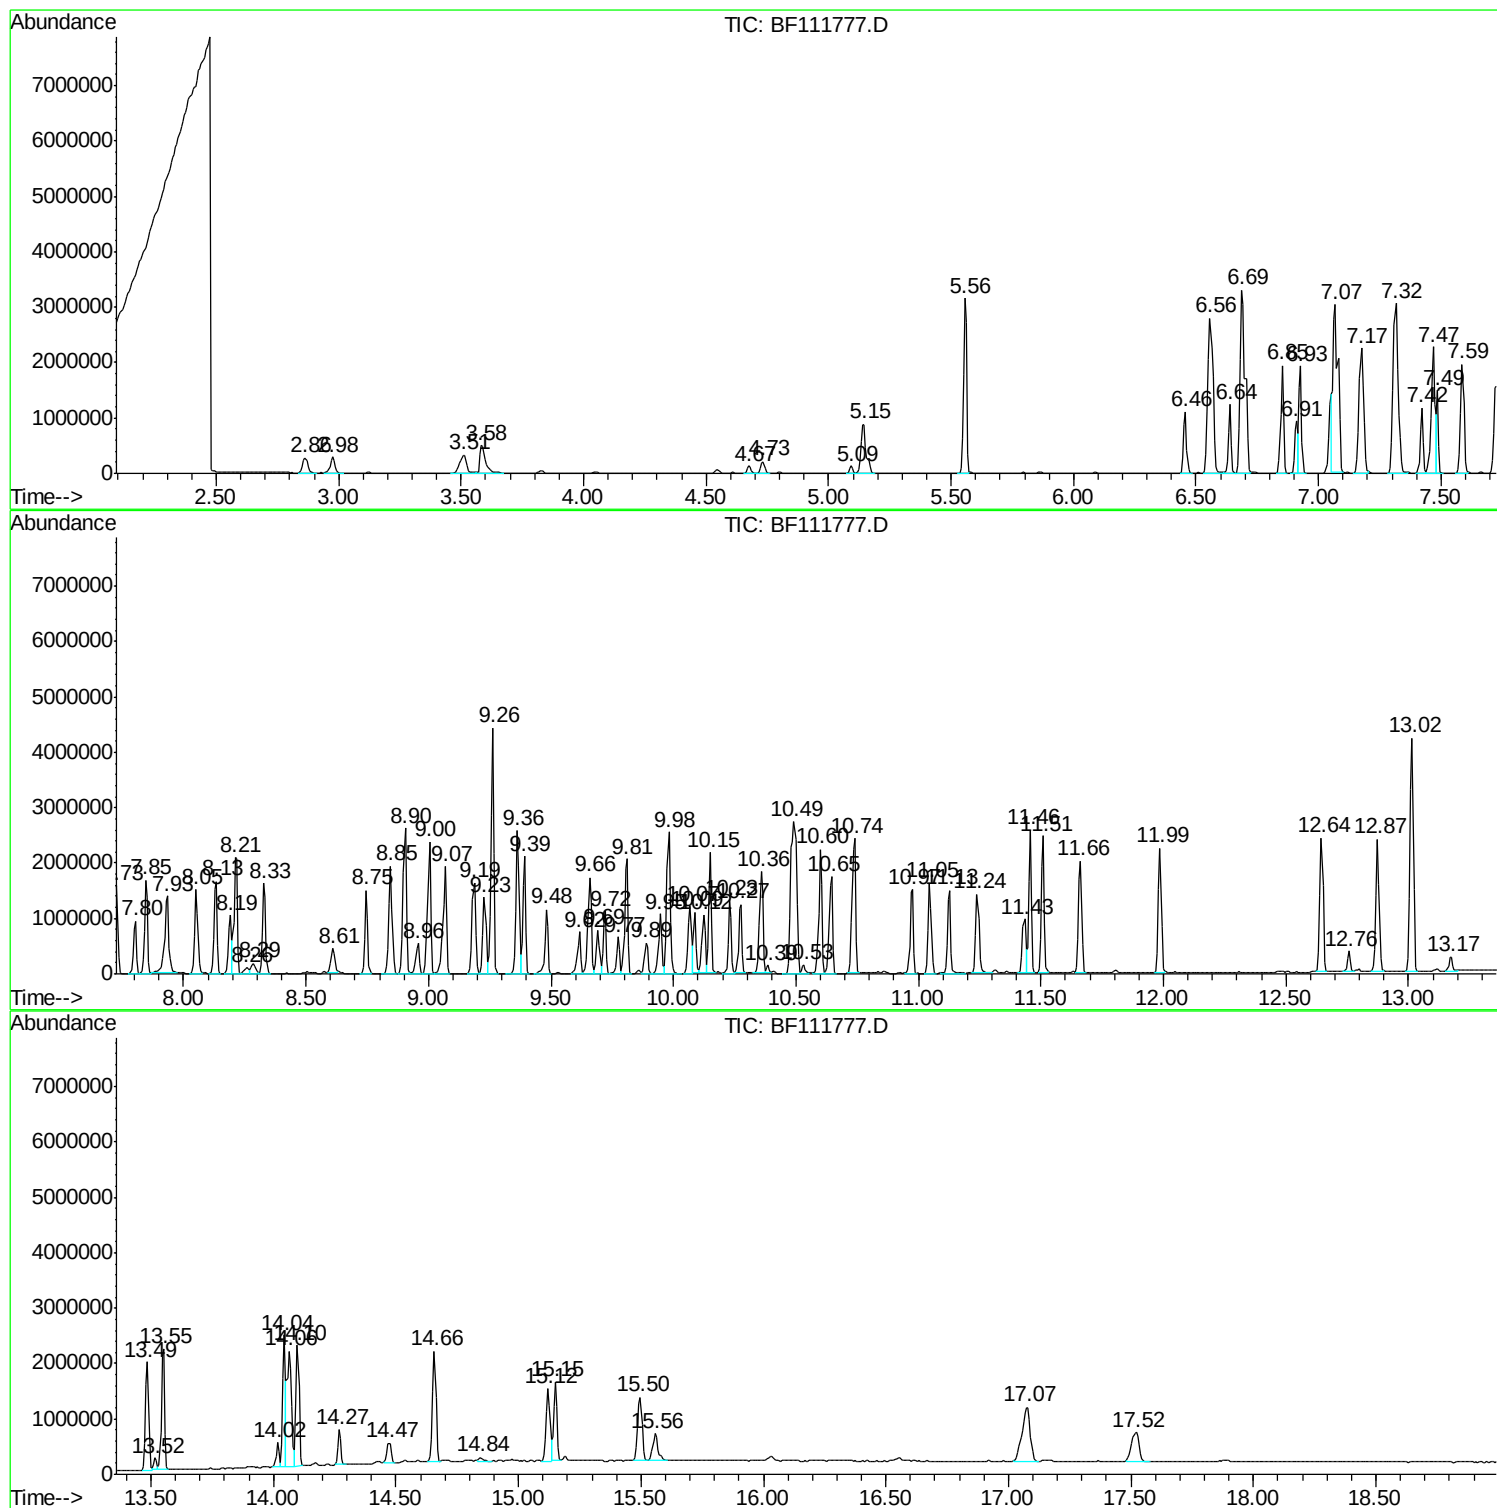

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF122718\
Data_File : BF111777.D
Acq_On : 27 Dec 2018 21:555
Operator : JU/SJJ
Sample : J6188-06MSDD
Misc :
ALS_Vial : 25 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
BU-03-122118MSD

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
