


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF122718\
 Data File : BF111753.D
 Acq On : 27 Dec 2018 10:52
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 19 17:39:39 2018

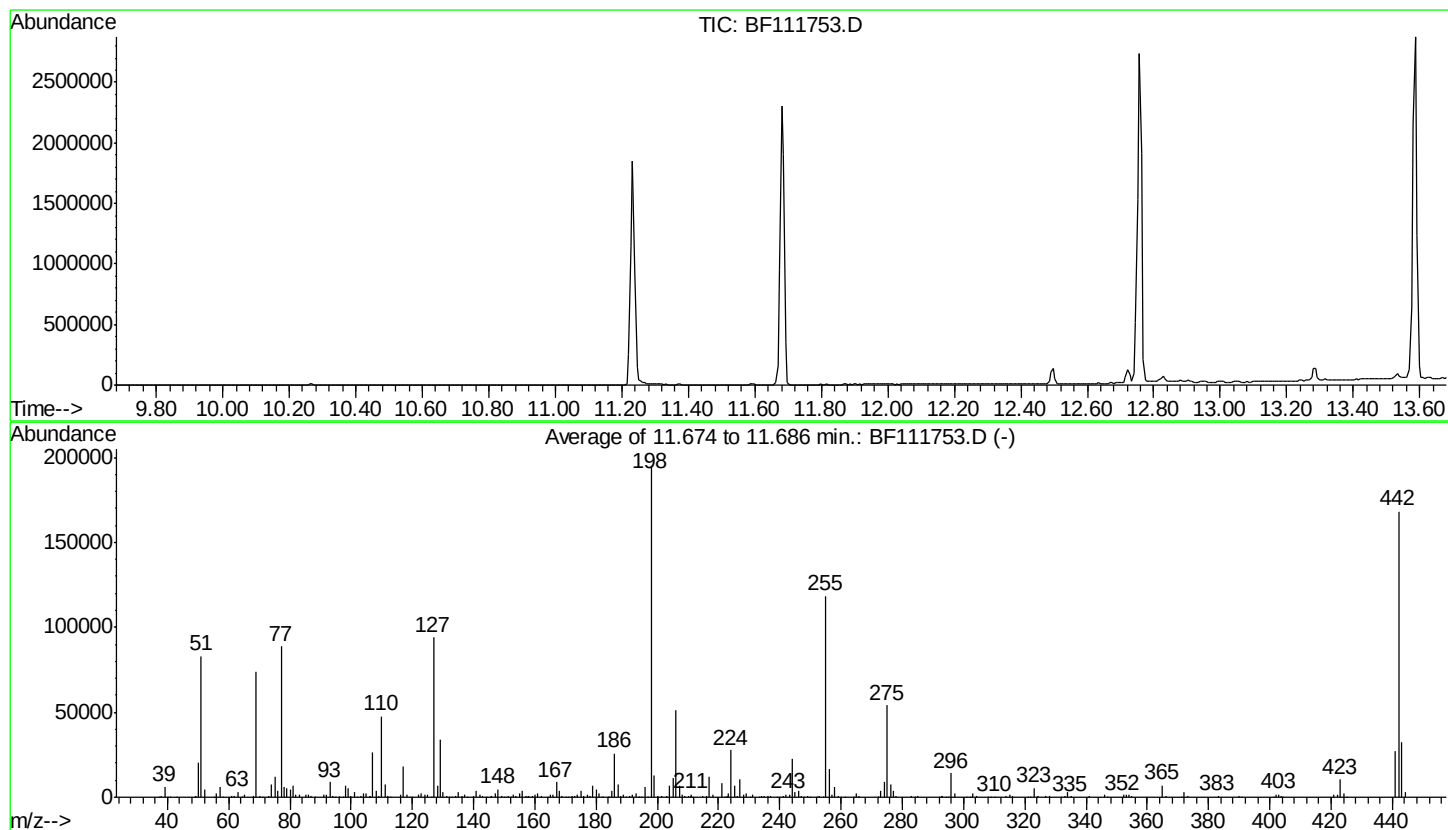

AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.5	82976	PASS
68	69	0.00	2	1.5	1132	PASS
69	198	0.00	100	37.8	73821	PASS
70	69	0.00	2	0.7	499	PASS
127	198	10	80	48.1	93925	PASS
197	198	0.00	2	0.1	256	PASS
198	198	100	100	100.0	195136	PASS
199	198	5	9	6.6	12795	PASS
275	198	10	60	27.7	54013	PASS
365	198	1	100	3.7	7153	PASS
441	198	0.01	100	13.8	26838	PASS
442	198	50	100	86.1	168010	PASS
443	442	15	24	19.3	32416	PASS