
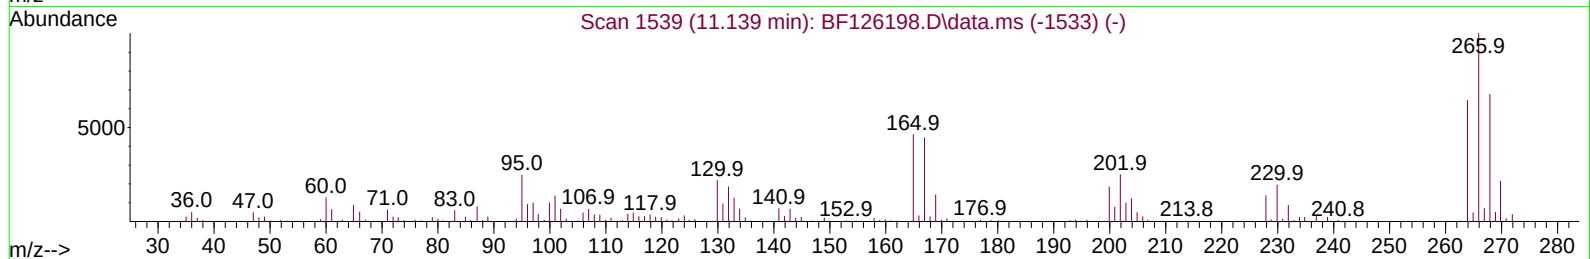
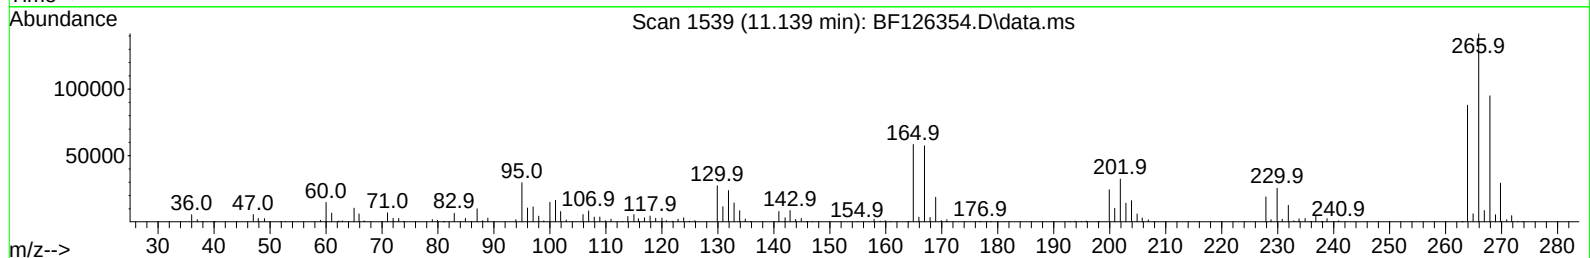


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122721\
 Data File : BF126354.D
 Acq On : 27 Dec 2021 14:16
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 27 15:53:11 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 22 13:00:11 2021
 Response via : Initial Calibration

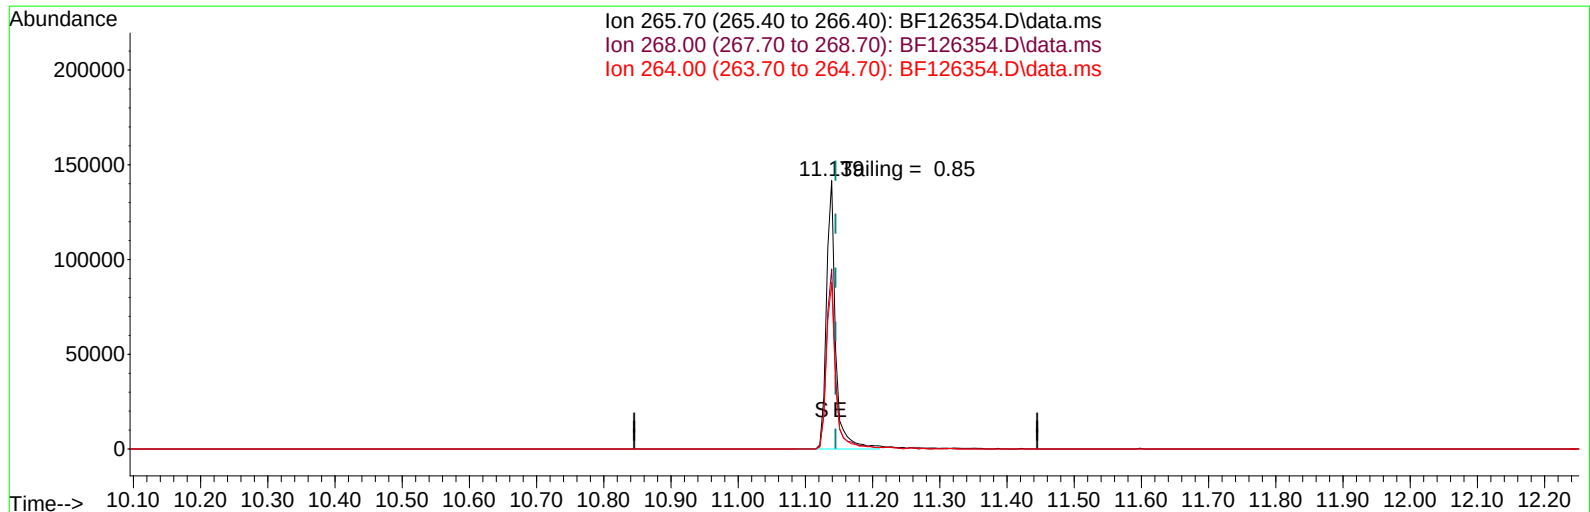

TIC: BF126354.D\data.ms

(70) Pentachlorophenol (C)




11.139min (-0.006) 52051.80 ng

response 136213

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	67.09
264.00	69.90	62.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122721\
 Data File : BF126354.D
 Acq On : 27 Dec 2021 14:16
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 27 15:53:11 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 22 13:00:11 2021
 Response via : Initial Calibration

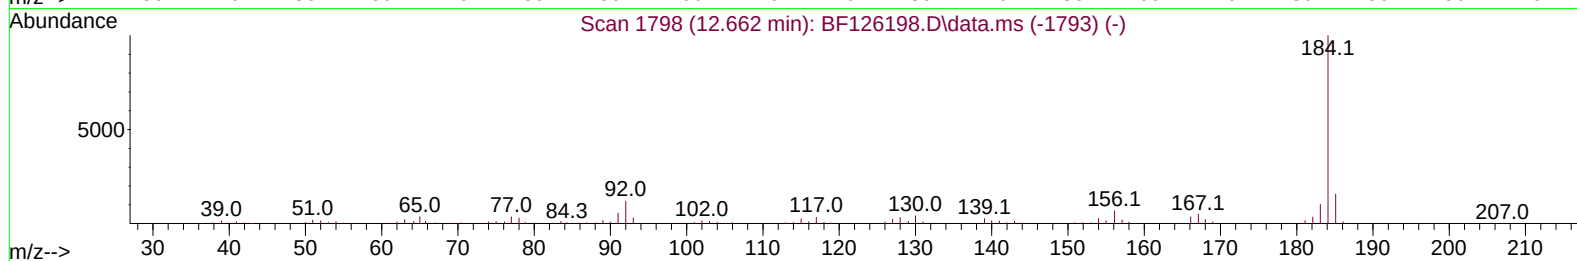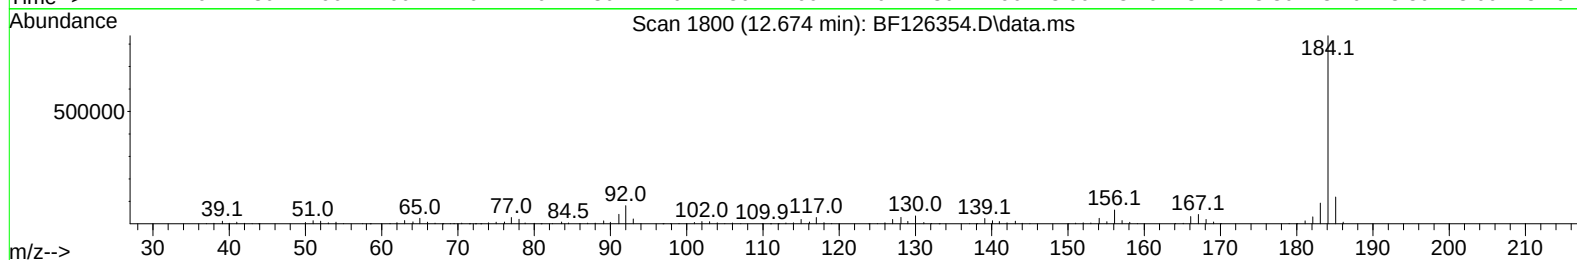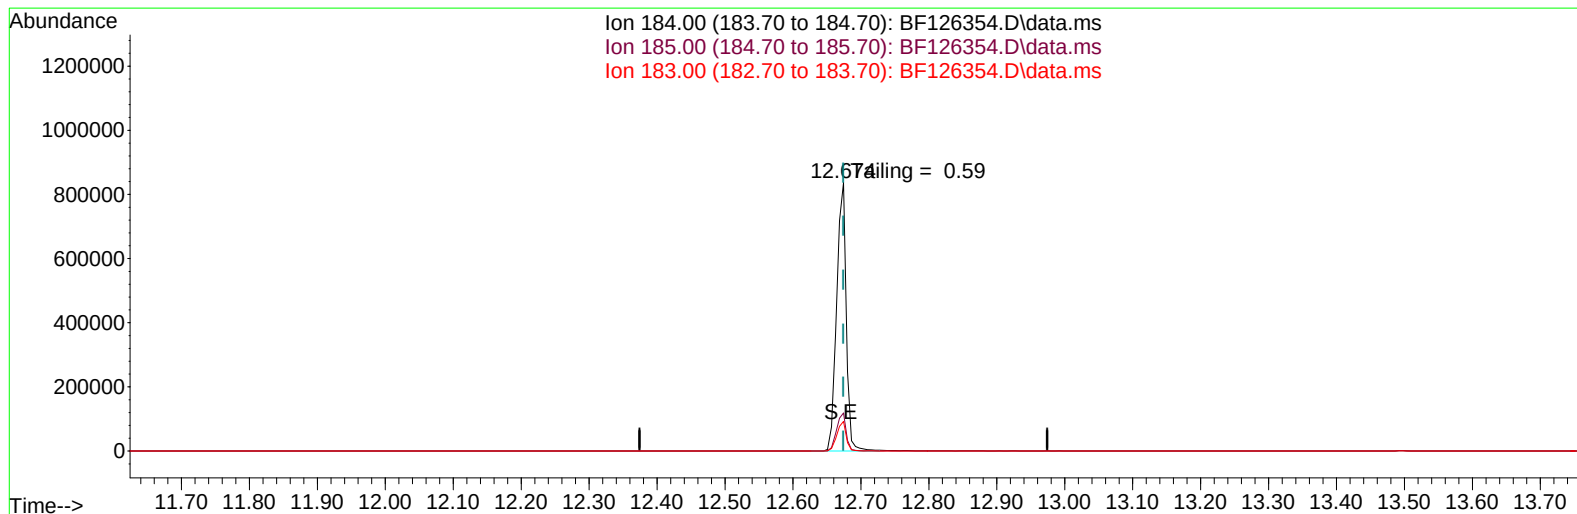

TIC: BF126354.D\data.ms

(77) Benzidine

12.674min (0.000) 0.00 ng

response 821669

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.22
183.00	10.10	11.03
0.00	0.00	0.00