

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122721\
 Data File : BF126363.D
 Acq On : 27 Dec 2021 19:07
 Operator : JU/CG
 Sample : M5188-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SASP2-119-1-COMP

Quant Time: Dec 28 05:59:47 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 22 13:00:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.810	152	110327	20.000	ng	0.00
21) Naphthalene-d8	8.092	136	446370	20.000	ng	#-0.01
39) Acenaphthene-d10	9.845	164	191449	20.000	ng	-0.01
64) Phenanthrene-d10	11.327	188	266954	20.000	ng	#-0.01
76) Chrysene-d12	13.968	240	202461	20.000	ng	-0.01
86) Perylene-d12	15.415	264	205155	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.428	112	826215	110.284	ng	0.00
7) Phenol-d6	6.440	99	925010	97.241	ng	0.00
23) Nitrobenzene-d5	7.369	82	691507	83.902	ng	-0.01
42) 2,4,6-Tribromophenol	10.633	330	193615	125.841	ng	-0.01
45) 2-Fluorobiphenyl	9.169	172	996083	91.252	ng	-0.01
79) Terphenyl-d14	12.922	244	721131	61.909	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122721\
Data File : BF126363.D
Acq On : 27 Dec 2021 19:07
Operator : JU/CG
Sample : M5188-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SASP2-119-1-COMP

Quant Time: Dec 28 05:59:47 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 22 13:00:11 2021
Response via : Initial Calibration




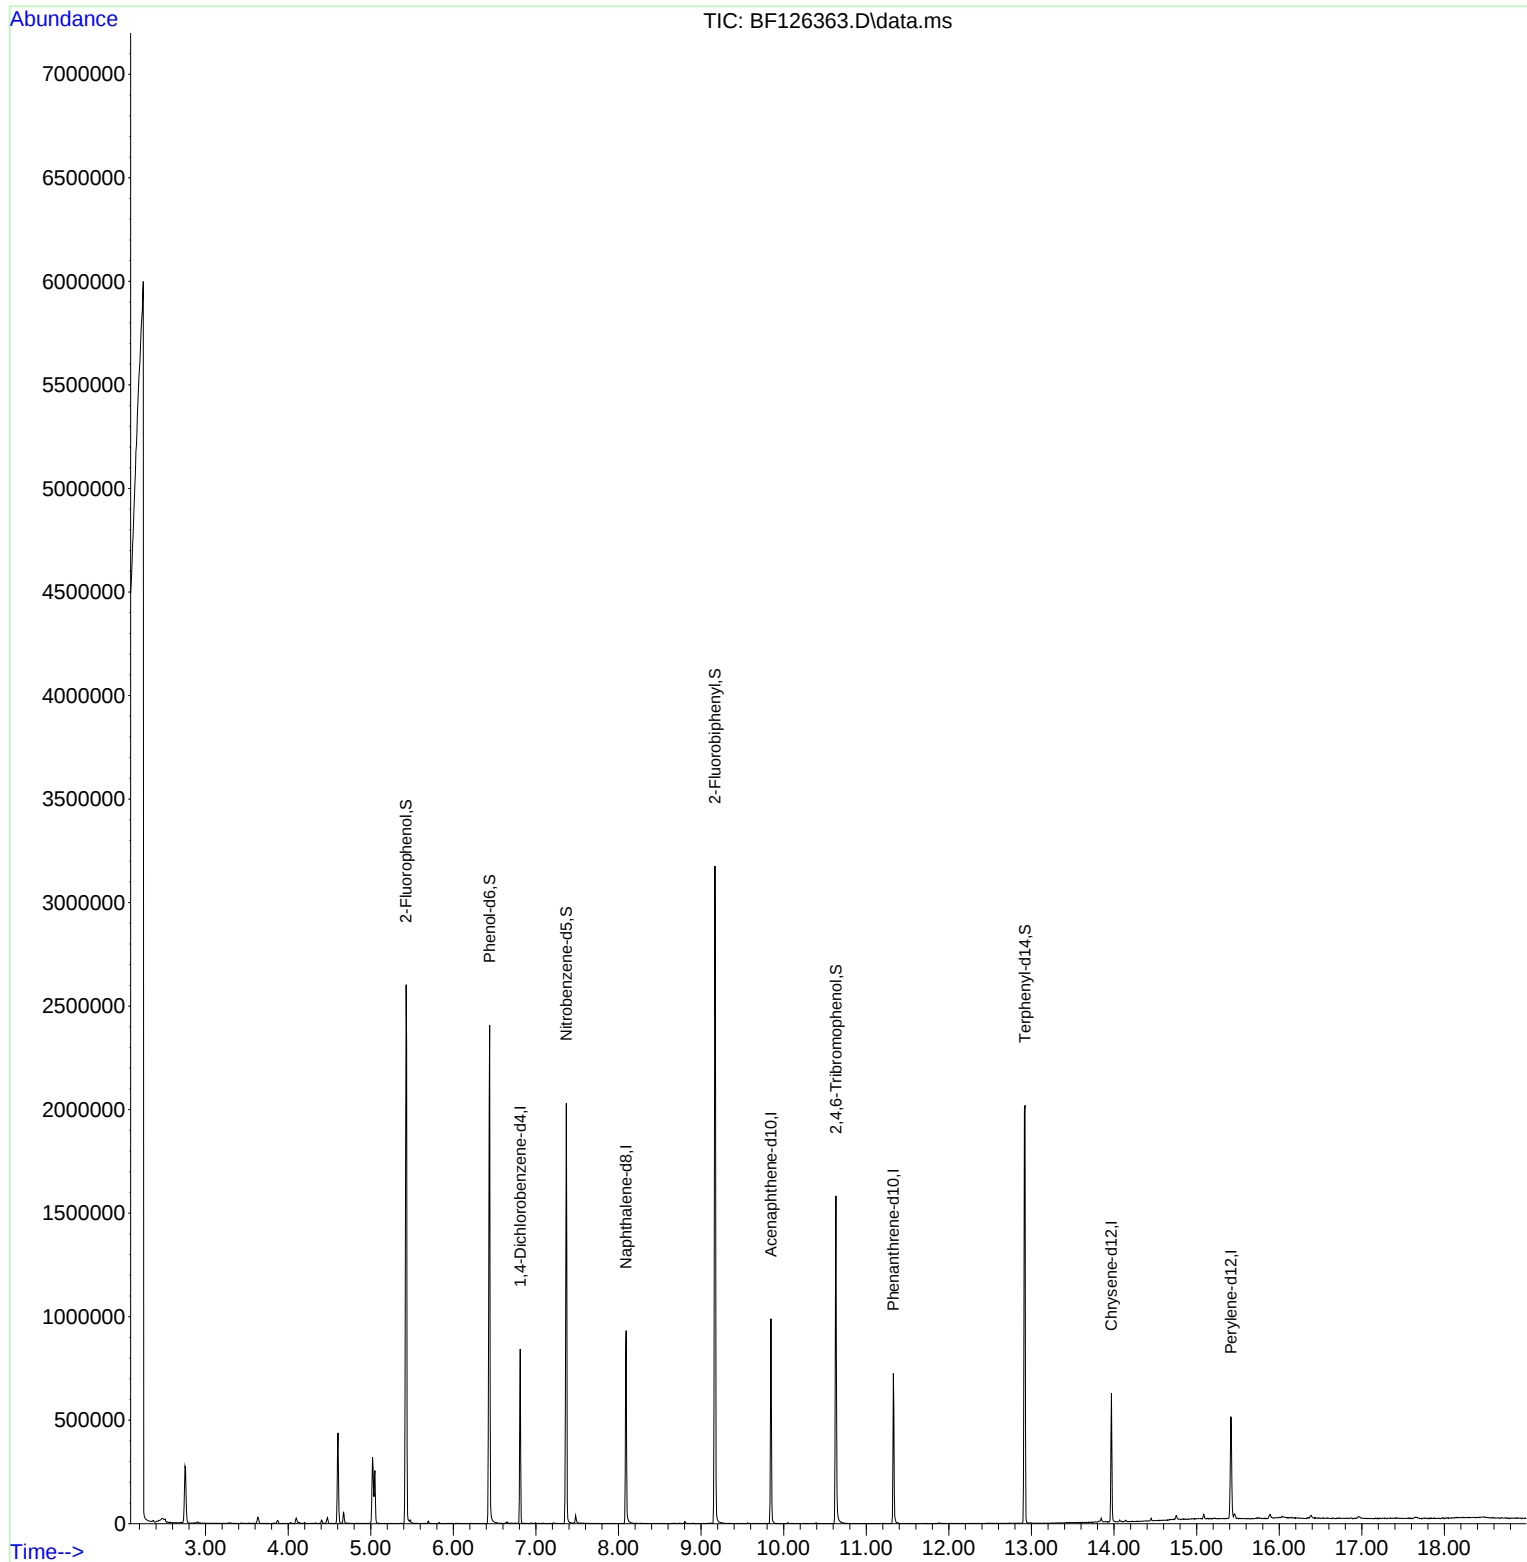




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.810 min Scan# 804
Delta R.T. -0.006 min
Lab File: BF126363.D
Acq: 27 Dec 2021 19:07




Instrument :
BNA_F
ClientSampleId :
SASP2-119-1-COMP


Tgt Ion:152 Resp: 110327
Ion Ratio Lower Upper
152 100
150 160.7 117.6 176.4
115 66.5 47.1 70.7

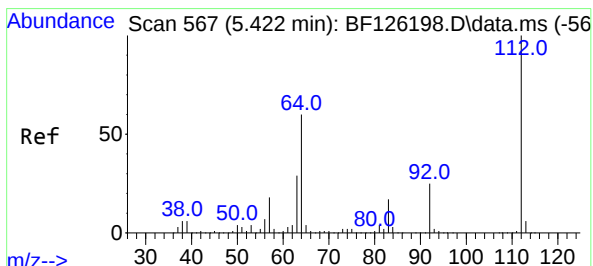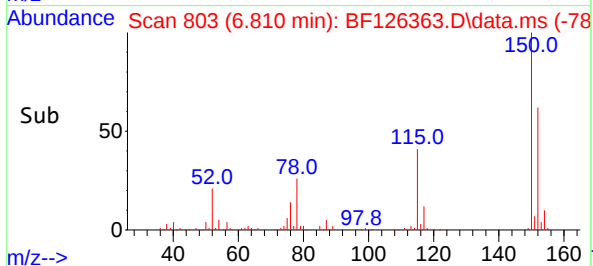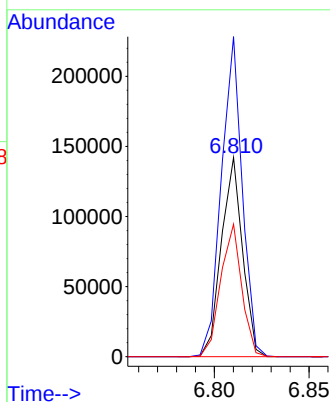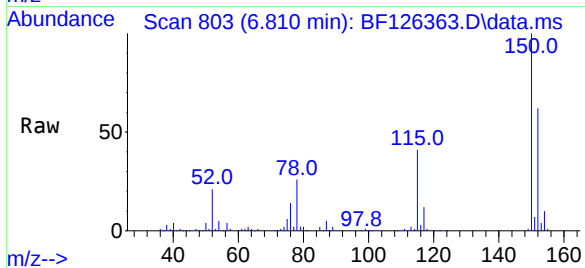

#5
2-Fluorophenol
Concen: 110.284 ng
RT: 5.428 min Scan# 568
Delta R.T. 0.000 min
Lab File: BF126363.D
Acq: 27 Dec 2021 19:07

Tgt Ion:112 Resp: 826215
Ion Ratio Lower Upper
112 100
64 61.9 44.2 66.2
63 29.0 26.2 39.2


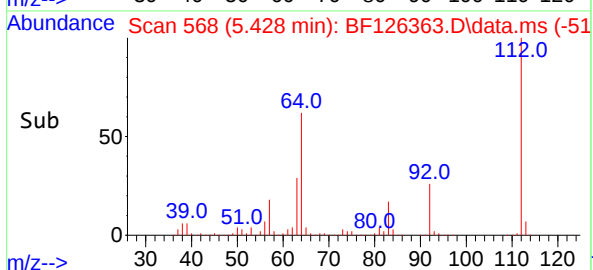
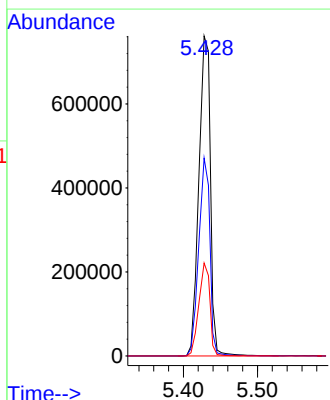
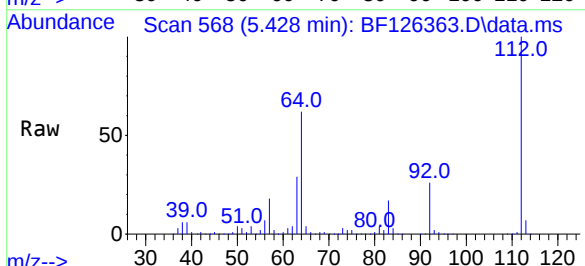


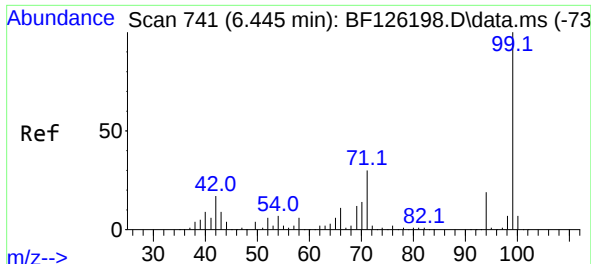

#7
Phenol-d6
Concen: 97.241 ng
RT: 6.440 min Scan# 741
Delta R.T. -0.006 min
Lab File: BF126363.D
Acq: 27 Dec 2021 19:07




Instrument :
BNA_F
ClientSampleId :
SASP2-119-1-COMP


Tgt Ion: 99 Resp: 925010
Ion Ratio Lower Upper
99 100
42 16.8 23.5 35.3#
71 30.3 25.6 38.4

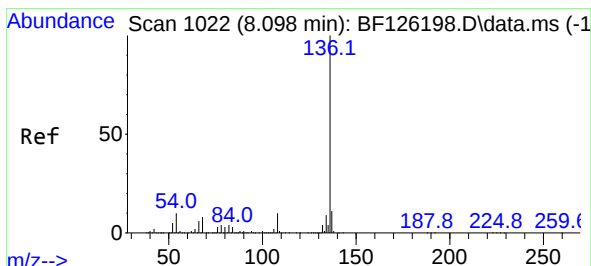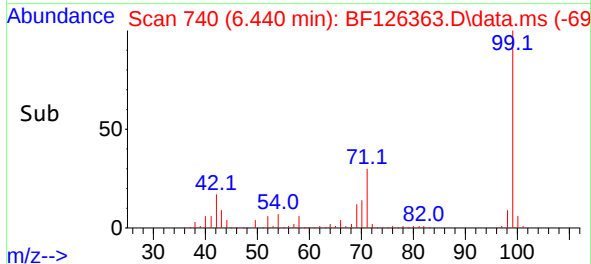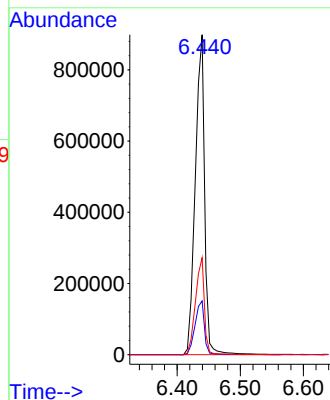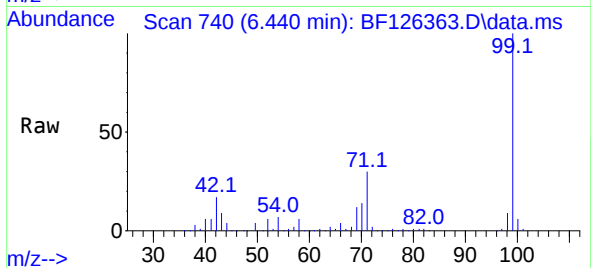

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.092 min Scan# 1021
Delta R.T. -0.012 min
Lab File: BF126363.D
Acq: 27 Dec 2021 19:07

Tgt Ion: 136 Resp: 446370
Ion Ratio Lower Upper
136 100
137 10.5 9.8 14.6
54 8.2 6.4 9.6
68 5.9 3.3 4.9#


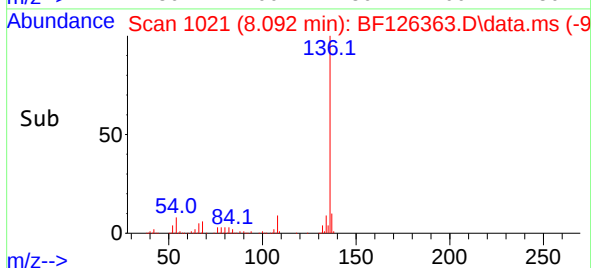
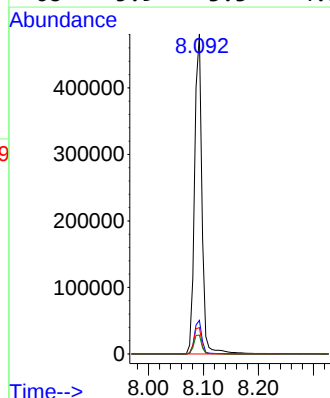
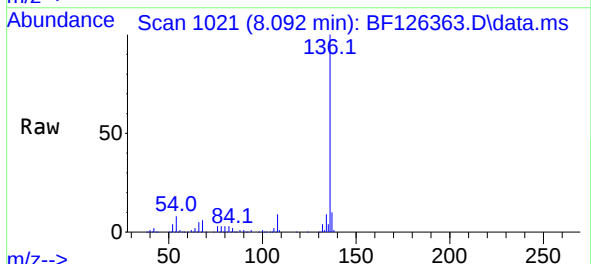


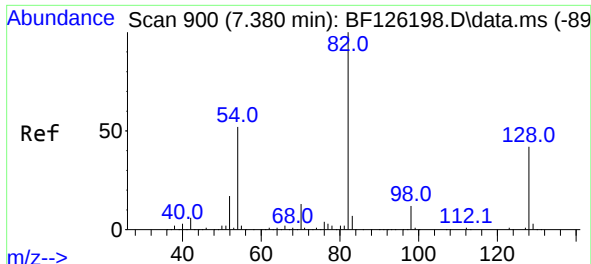

#23
Nitrobenzene-d5
Concen: 83.902 ng
RT: 7.369 min Scan# 89
Delta R.T. -0.012 min
Lab File: BF126363.D
Acq: 27 Dec 2021 19:07




Instrument :
BNA_F
ClientSampleId :
SASP2-119-1-COMP


Tgt Ion: 82 Resp: 691507
Ion Ratio Lower Upper
82 100
128 43.2 40.6 60.8
54 52.0 49.6 74.4

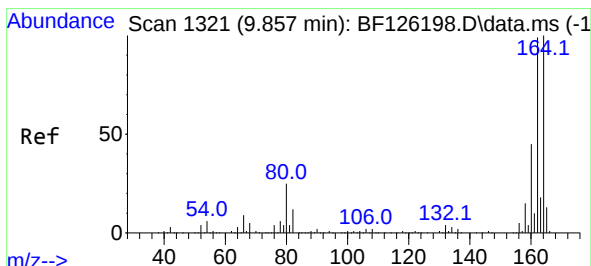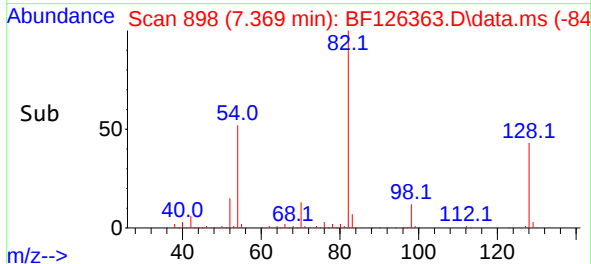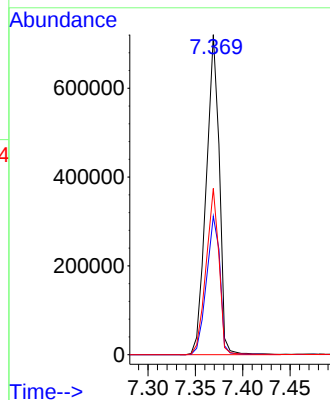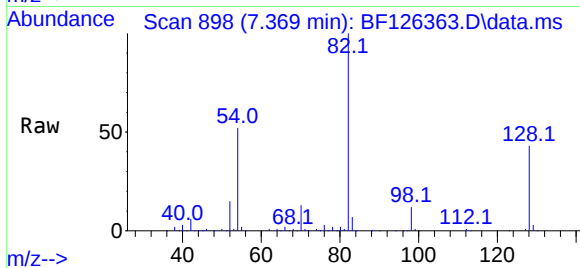

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.845 min Scan# 1319
Delta R.T. -0.012 min
Lab File: BF126363.D
Acq: 27 Dec 2021 19:07


Tgt Ion:164 Resp: 191449
Ion Ratio Lower Upper
164 100
162 99.8 81.3 121.9
160 45.3 38.0 57.0

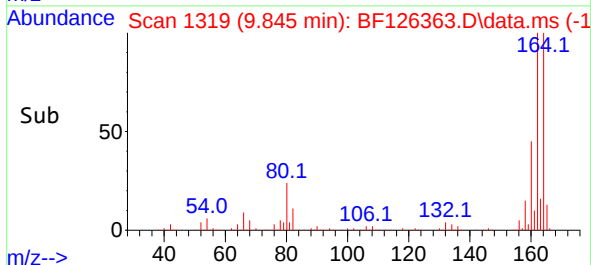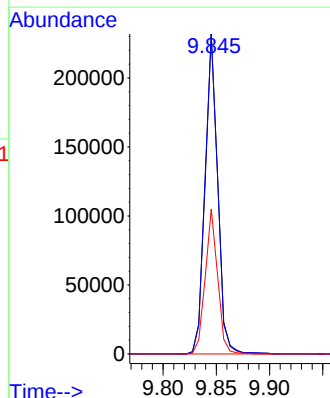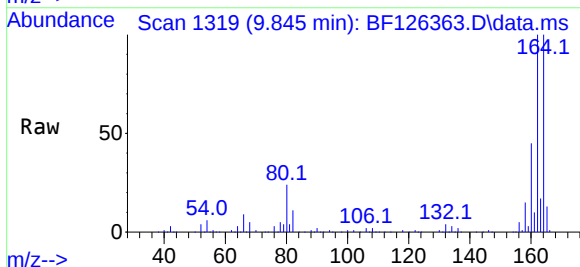



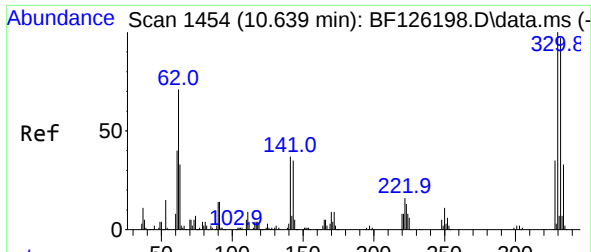


#42
2,4,6-Tribromophenol
Concen: 125.841 ng
RT: 10.633 min Scan# 1454
Delta R.T. -0.012 min
Lab File: BF126363.D
Acq: 27 Dec 2021 19:07

Instrument :
BNA_F
ClientSampleId :
SASP2-119-1-COMP



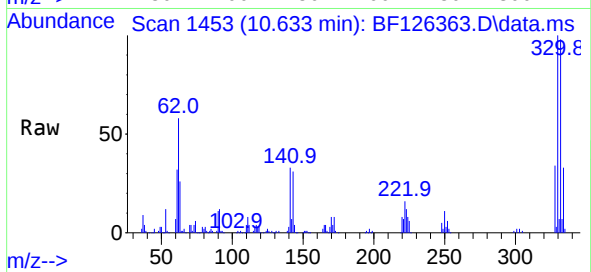



Tgt Ion:330 Resp: 193615
Ion Ratio Lower Upper
330 100
332 95.0 76.2 114.4
141 32.7 44.6 66.8#

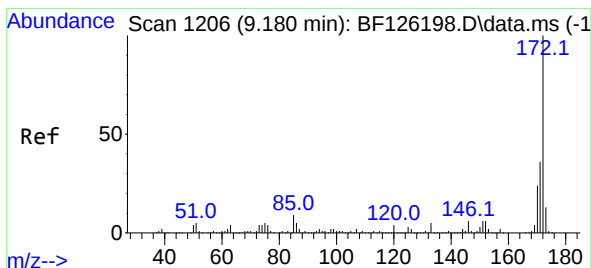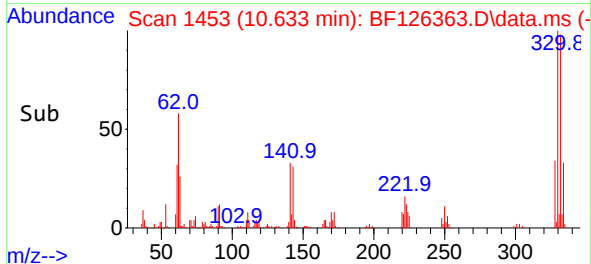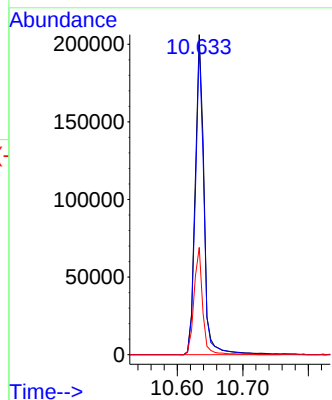

#45
2-Fluorobiphenyl
Concen: 91.252 ng
RT: 9.169 min Scan# 1204
Delta R.T. -0.012 min
Lab File: BF126363.D
Acq: 27 Dec 2021 19:07


Tgt Ion:172 Resp: 996083
Ion Ratio Lower Upper
172 100
171 34.3 26.5 39.7
170 23.5 18.8 28.2

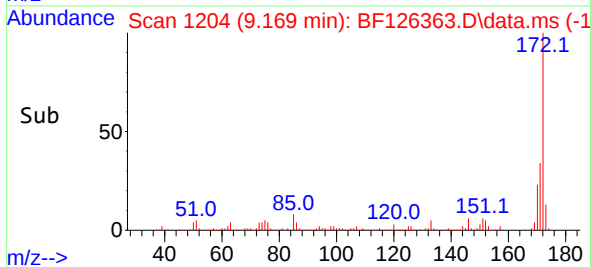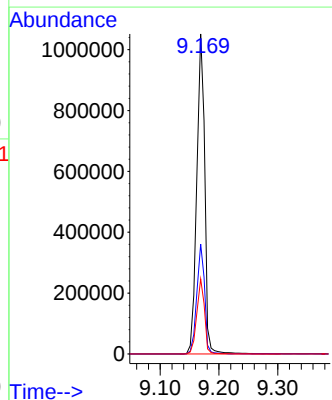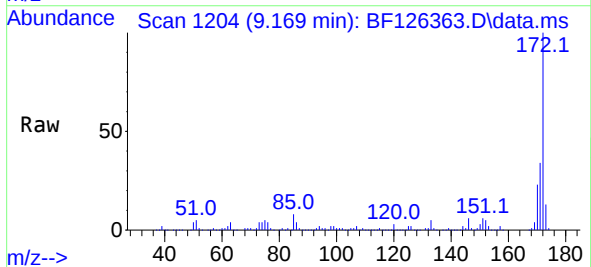



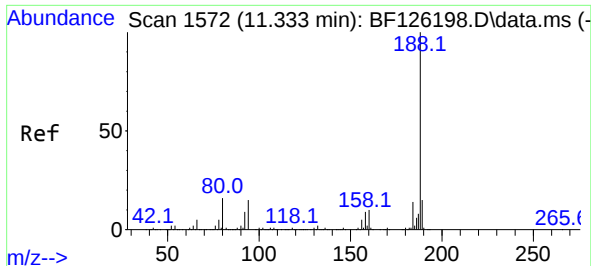


#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.327 min Scan# 11
Delta R.T. -0.012 min
Lab File: BF126363.D
Acq: 27 Dec 2021 19:07

Instrument :
BNA_F
ClientSampleId :
SASP2-119-1-COMP



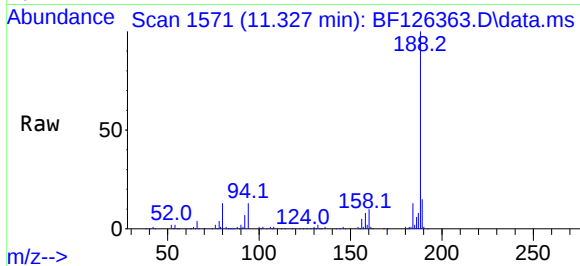



Tgt Ion:188 Resp: 266954
Ion Ratio Lower Upper
188 100
94 12.7 6.7 10.1#
80 13.3 7.5 11.3#

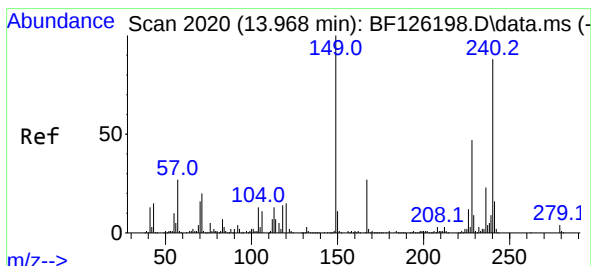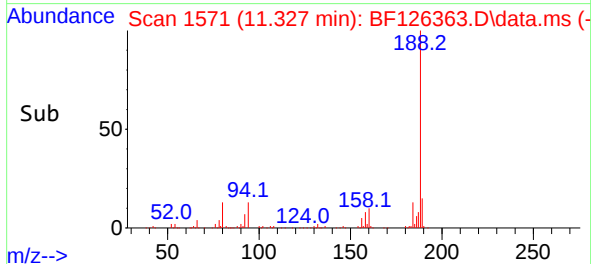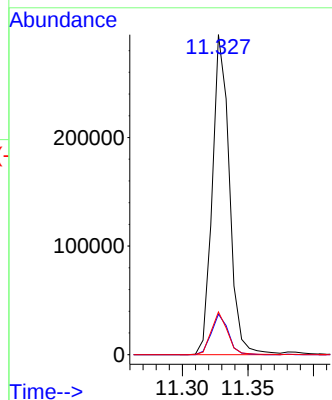

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.968 min Scan# 2020
Delta R.T. -0.012 min
Lab File: BF126363.D
Acq: 27 Dec 2021 19:07


Tgt Ion:240 Resp: 202461
Ion Ratio Lower Upper
240 100
120 14.2 10.8 16.2
236 23.7 21.6 32.4

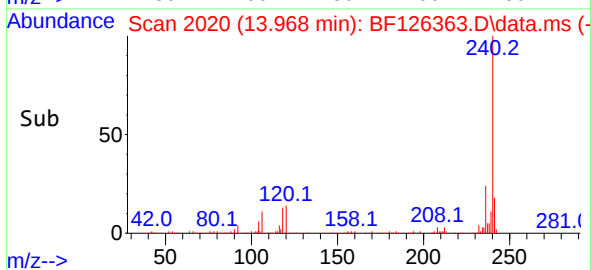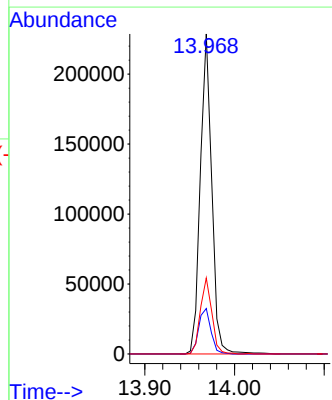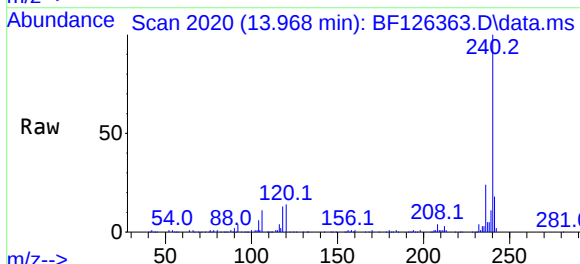



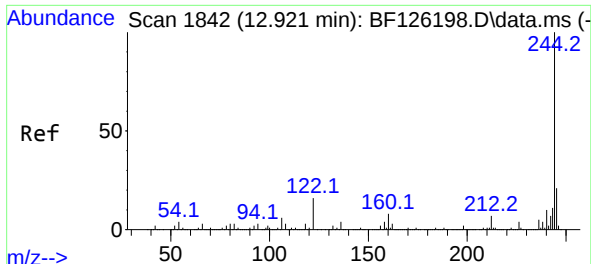


#79
 Terphenyl-d14
 Concen: 61.909 ng
 RT: 12.922 min Scan# 1842
 Delta R.T. -0.006 min
 Lab File: BF126363.D
 Acq: 27 Dec 2021 19:07


Instrument :
 BNA_F
 ClientSampleId :
 SASP2-119-1-COMP

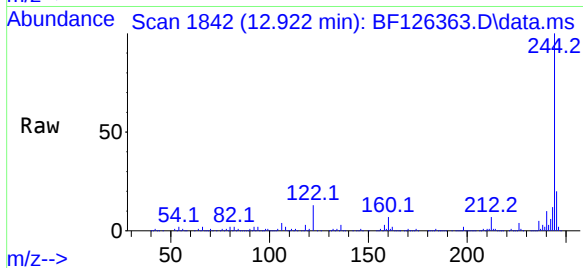

Tgt Ion:244 Resp: 721131
 Ion Ratio Lower Upper
 244 100
 212 6.5 5.9 8.9
 122 12.6 9.0 13.4

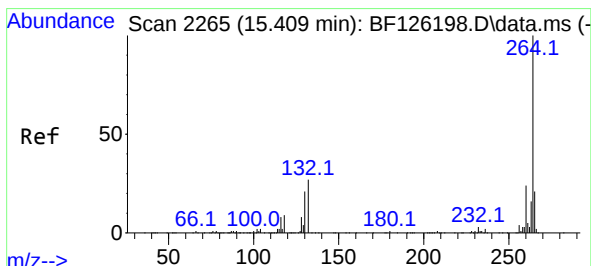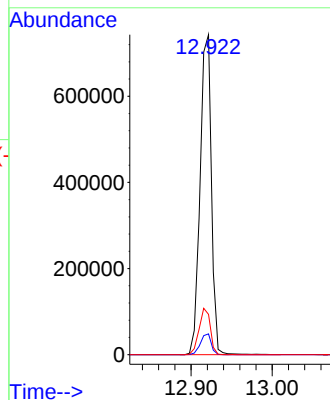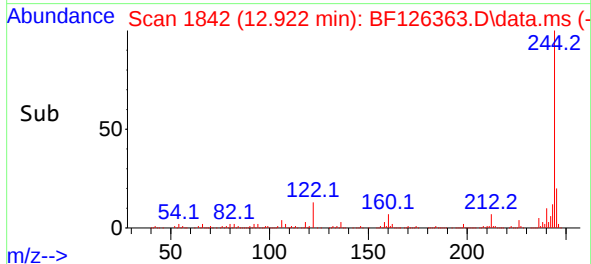

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.415 min Scan# 2266
 Delta R.T. -0.012 min
 Lab File: BF126363.D
 Acq: 27 Dec 2021 19:07

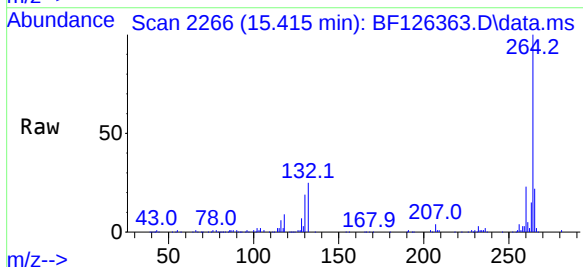

Tgt Ion:264 Resp: 205155
 Ion Ratio Lower Upper
 264 100
 260 22.6 19.6 29.4
 265 22.4 17.2 25.8

