

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122721\
 Data File : BF126365.D
 Acq On : 27 Dec 2021 20:10
 Operator : JU/CG
 Sample : M5065-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 UV-1WC

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126365.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.763	109	115	121	rVB	311546	415241	14.86%	2.194%
2	4.604	424	428	433	rBV	454907	472253	16.90%	2.496%
3	5.022	495	499	502	rBV	283749	366058	13.10%	1.934%
4	5.051	502	504	511	rVB	299659	260018	9.31%	1.374%
5	5.428	564	568	572	rBV	2465553	2601903	93.11%	13.749%
6	6.439	735	740	743	rBV	2277077	2313473	82.79%	12.225%
7	6.810	799	803	806	rBV	875717	691649	24.75%	3.655%
8	7.369	893	898	901	rBV	1948544	1882323	67.36%	9.947%
9	8.092	1016	1021	1026	rBV	979957	894383	32.01%	4.726%
10	9.169	1199	1204	1207	rBV	3156487	2794299	100.00%	14.766%
11	9.845	1315	1319	1327	rBV	1046115	863103	30.89%	4.561%
12	10.633	1449	1453	1471	rBV	1591891	1452934	52.00%	7.678%
13	11.327	1568	1571	1579	rBV	752490	710272	25.42%	3.753%
14	12.921	1837	1842	1845	rBV	2059071	2024984	72.47%	10.701%
15	13.968	2016	2020	2028	rBV	642567	578996	20.72%	3.060%
16	15.415	2261	2266	2271	rBV	490832	601762	21.54%	3.180%




Sum of corrected areas: 18923651

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122721\
Data File : BF126365.D
Acq On : 27 Dec 2021 20:10
Operator : JU/CG
Sample : M5065-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
UV-1WC

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

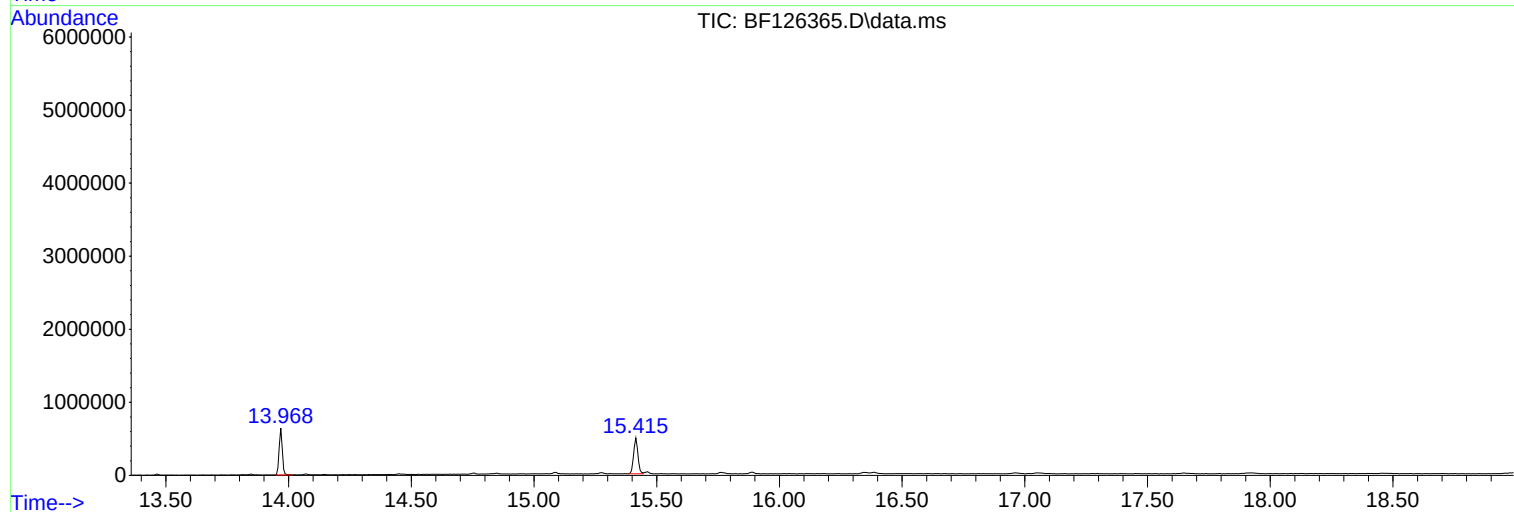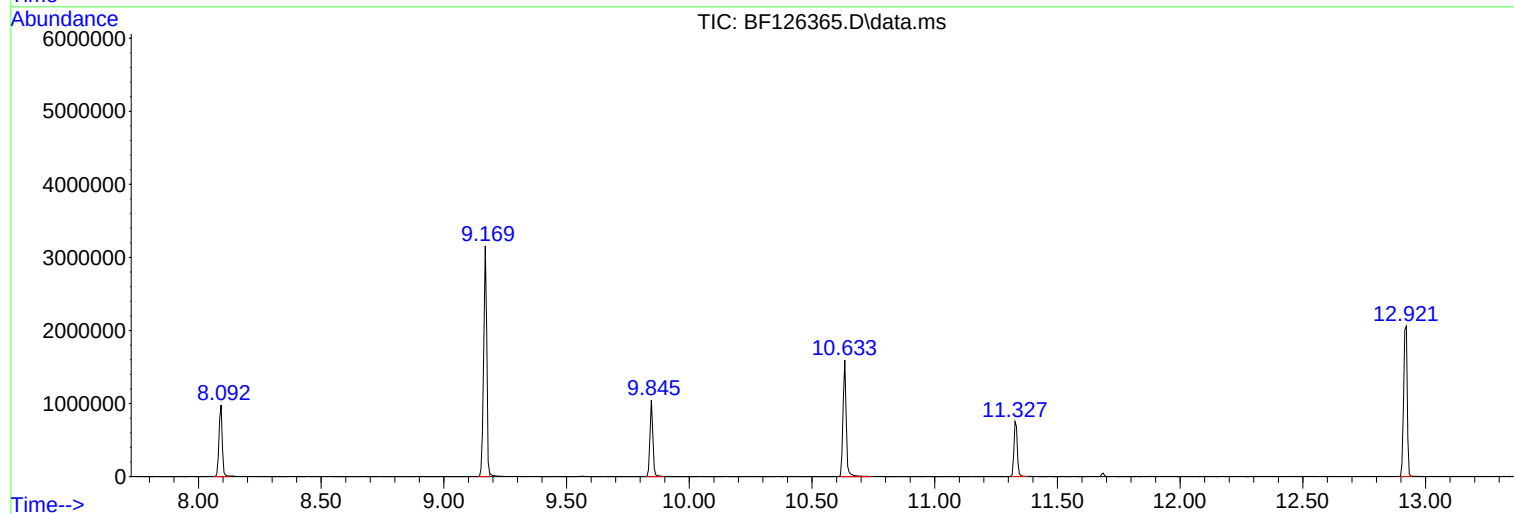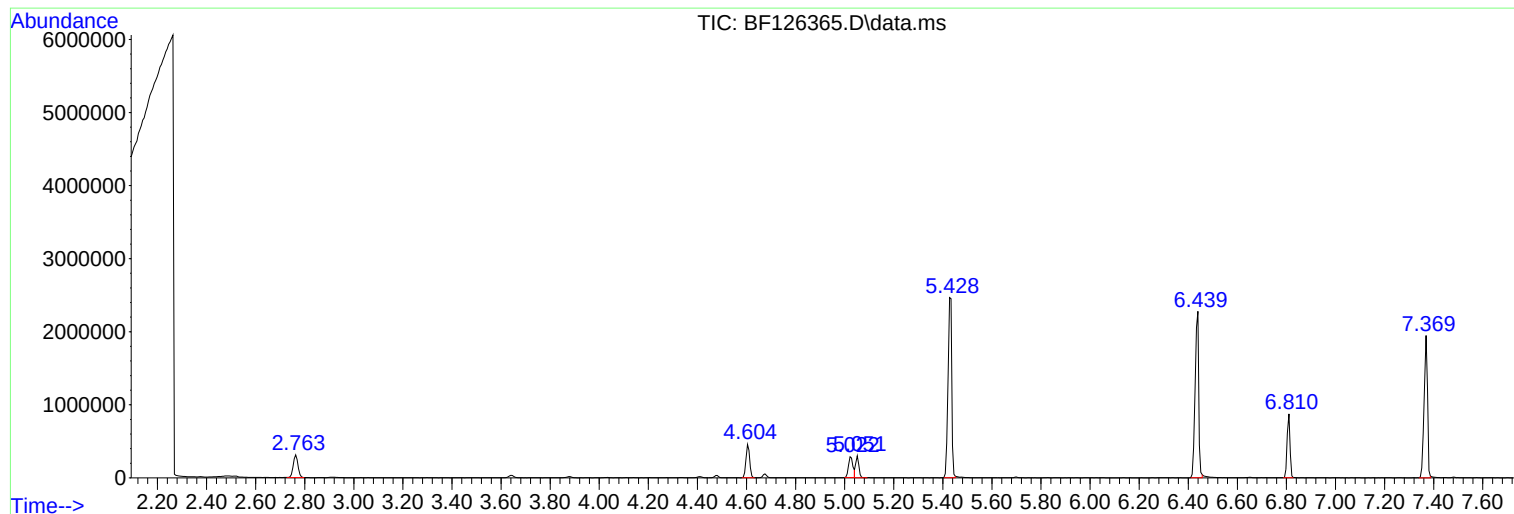

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122721\
Data File : BF126365.D
Acq On : 27 Dec 2021 20:10
Operator : JU/CG
Sample : M5065-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
UV-1WC

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122721\
Data File : BF126365.D
Acq On : 27 Dec 2021 20:10
Operator : JU/CG
Sample : M5065-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
UV-1WC

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------