
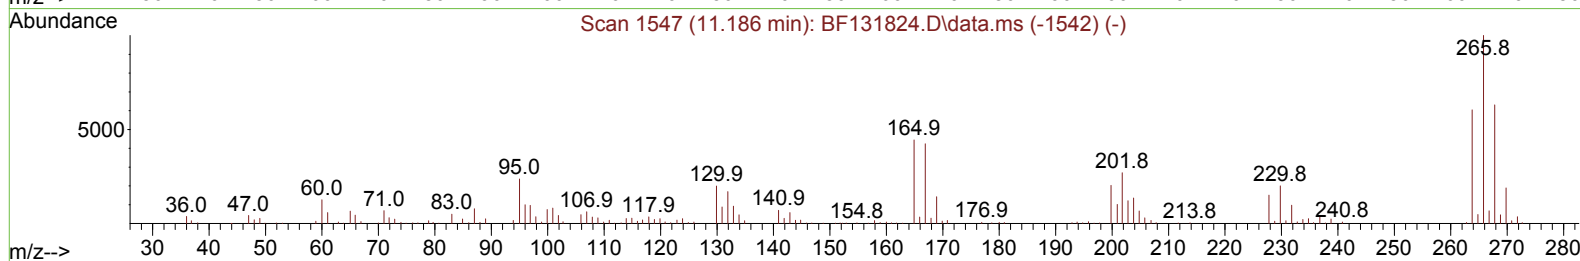
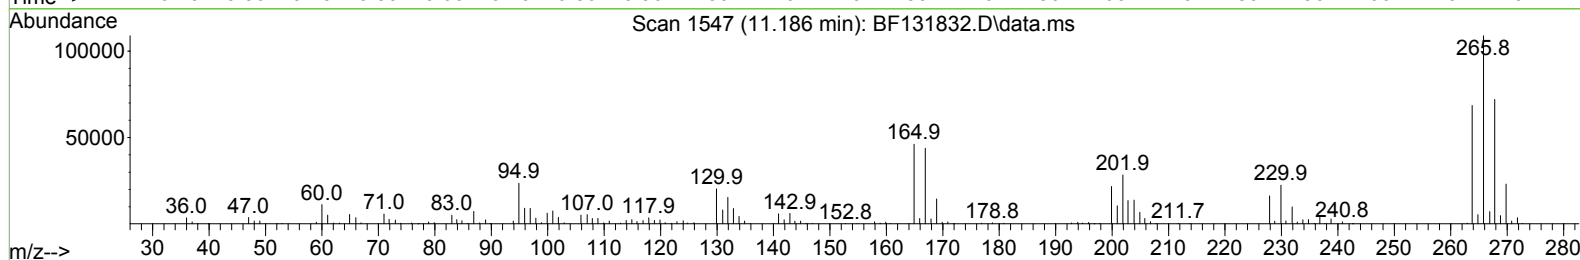


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122722\
Data File : BF131832.D
Acq On : 27 Dec 2022 11:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 06:12:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 26 05:13:34 2022
Response via : Initial Calibration

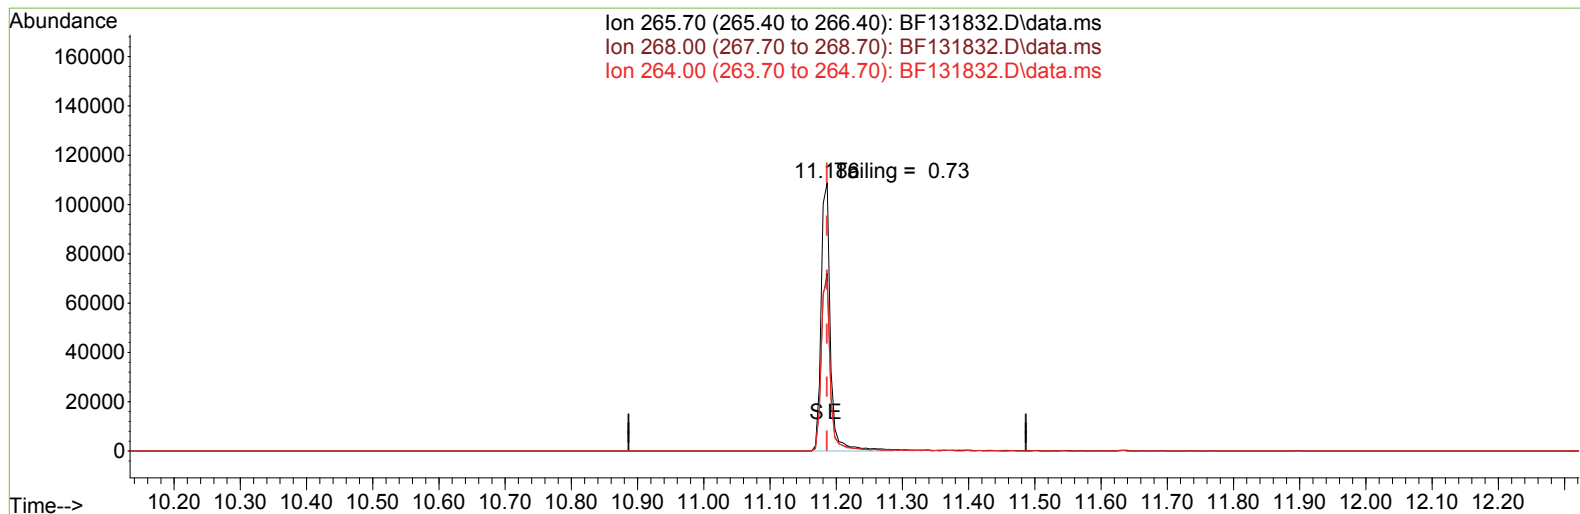

TIC: BF131832.D\data.ms

(70) Pentachlorophenol (C)

11.186min (+ 0.000) 30046.79 ng

response 107331

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	66.15
264.00	60.40	62.91
0.00	0.00	0.00

