
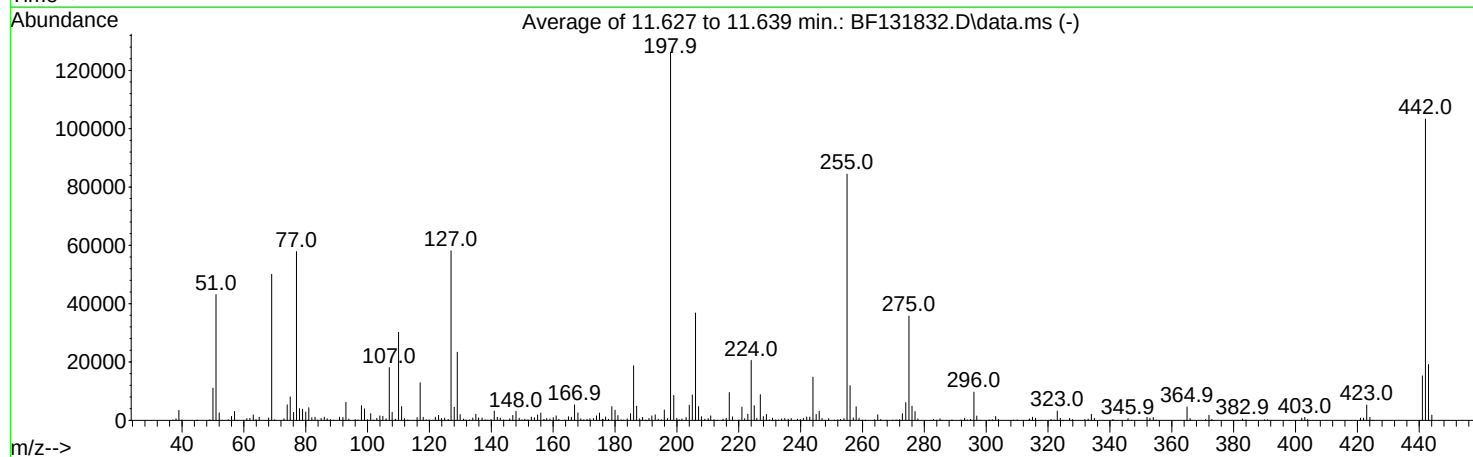


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122722\
 Data File : BF131832.D
 Acq On : 27 Dec 2022 11:45
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 26 05:13:34 2022

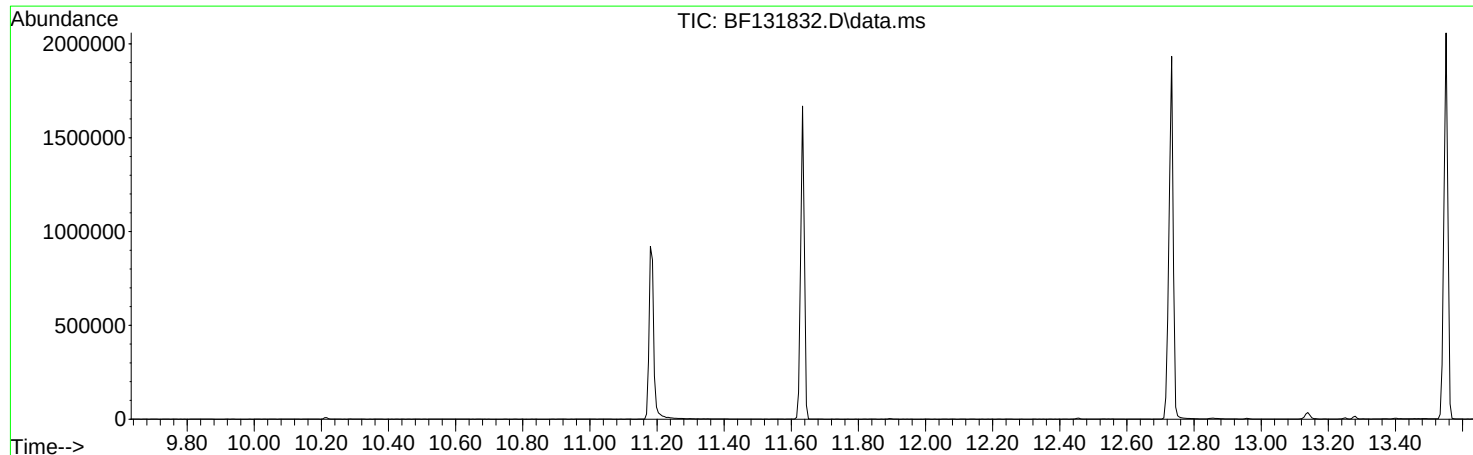




AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	43131	PASS
68	69	0.00	2	1.6	807	PASS
69	198	0.00	100	39.7	50072	PASS
70	69	0.00	2	0.4	197	PASS
127	198	10	80	46.1	58112	PASS
197	198	0.00	2	0.5	607	PASS
198	198	100	100	100.0	126155	PASS
199	198	5	9	6.8	8566	PASS
275	198	10	60	28.3	35741	PASS
365	198	1	100	3.6	4580	PASS
441	198	0.01	100	12.1	15251	PASS
442	442	50	100	100.0	103299	PASS
443	442	15	24	18.5	19132	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122722\
Data File : BF131832.D
Acq On : 27 Dec 2022 11:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 28 06:12:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 26 05:13:34 2022
Response via : Initial Calibration

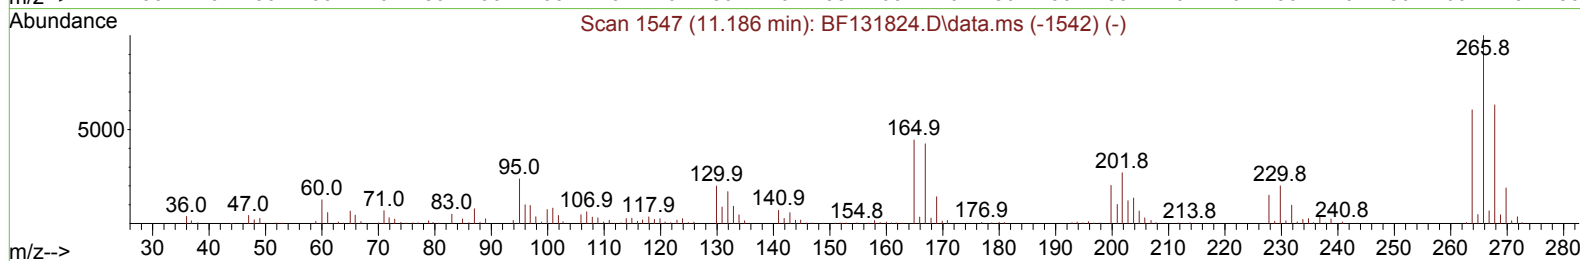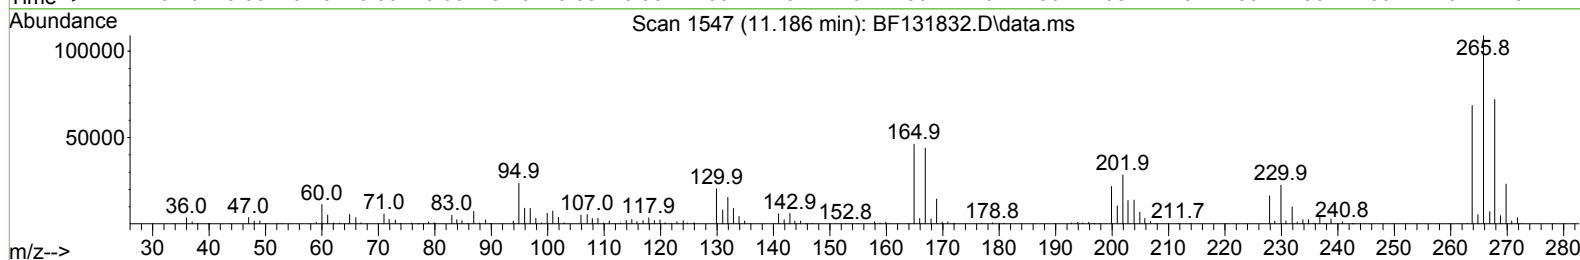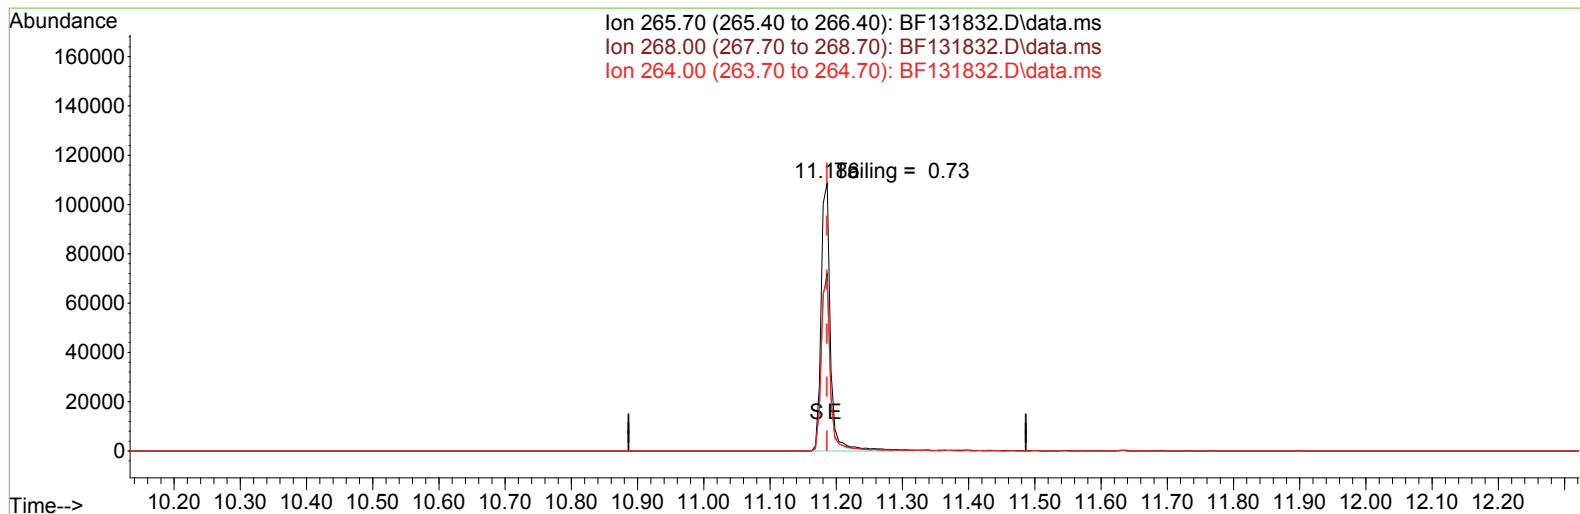

TIC: BF131832.D\data.ms

(70) Pentachlorophenol (C)

11.186min (+ 0.000) 30046.79 ng

response 107331

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	66.15
264.00	60.40	62.91
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/27/2022	BNA_F	<u>BF131832.D</u>
Compound Name	Response	Retention Time
DDT	329056	13.551
DDD	4295	13.28
DDE	156	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4451	333507	1.33

Instrument :
BNA_F
ClientSampleId :
DFTPP