
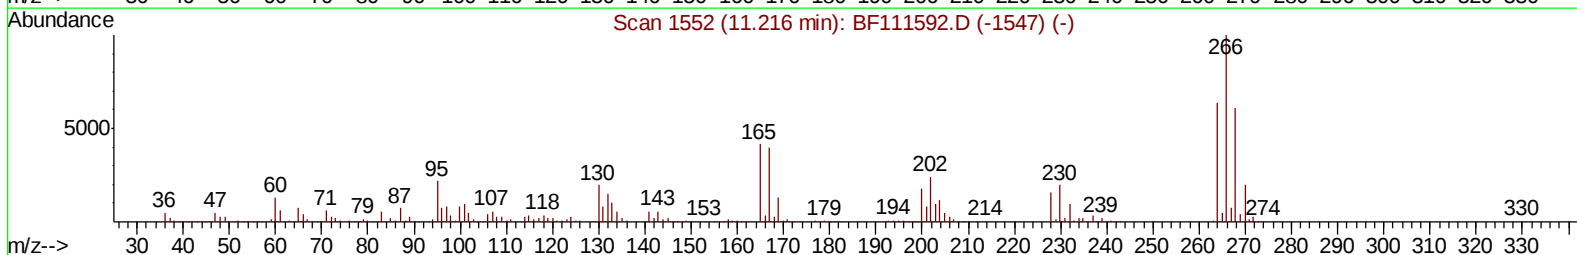
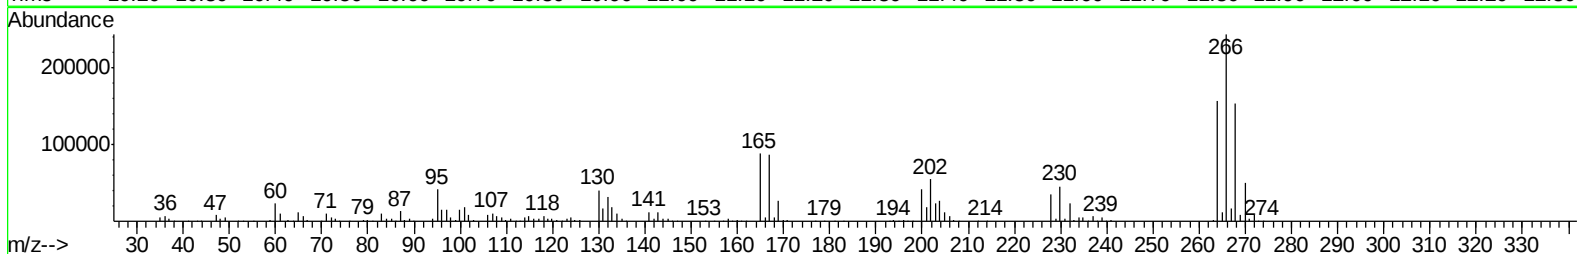


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122818\
 Data File : BF111785.D
 Acq On : 28 Dec 2018 13:30
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 14:02:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 19 17:39:39 2018
 Response via : Initial Calibration

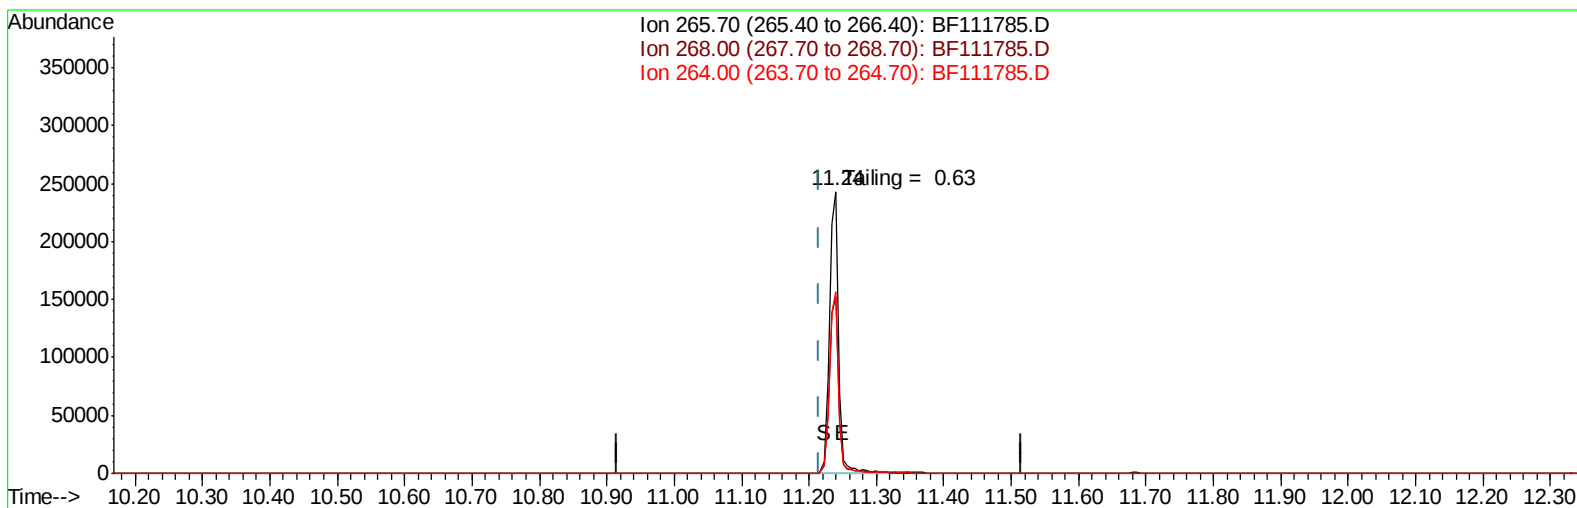

TIC: BF111785.D

(70) Pentachlorophenol (C)




11.239min (+0.023) 174234.22ng

response 233869

Ion	Exp%	Act%
265.70	100	100
268.00	59.90	62.91
264.00	61.40	64.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122818\
Data File : BF111785.D
Acq On : 28 Dec 2018 13:30
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 14:02:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 17:39:39 2018
Response via : Initial Calibration

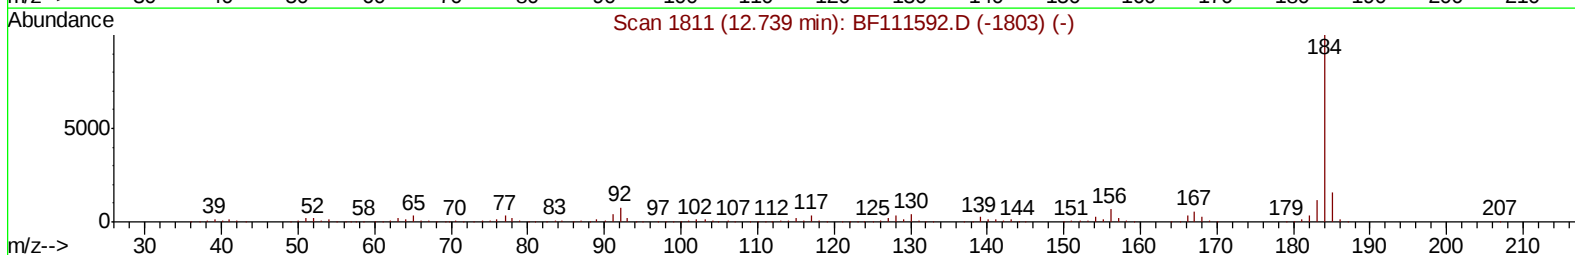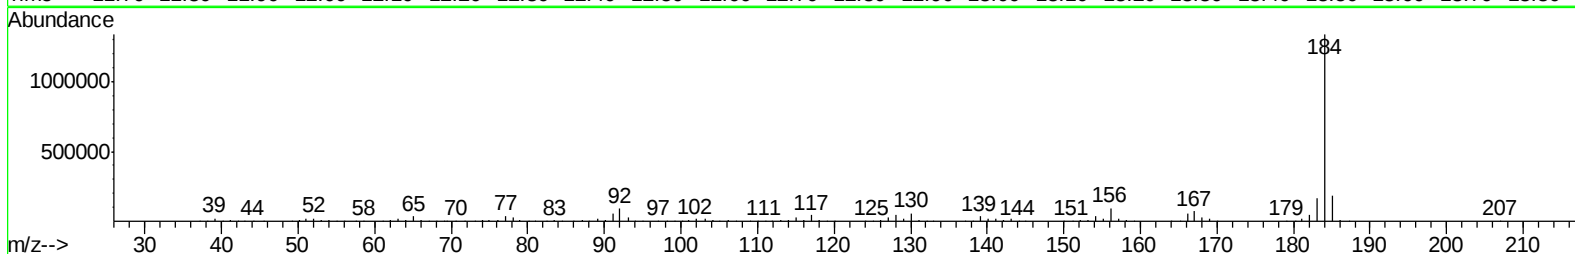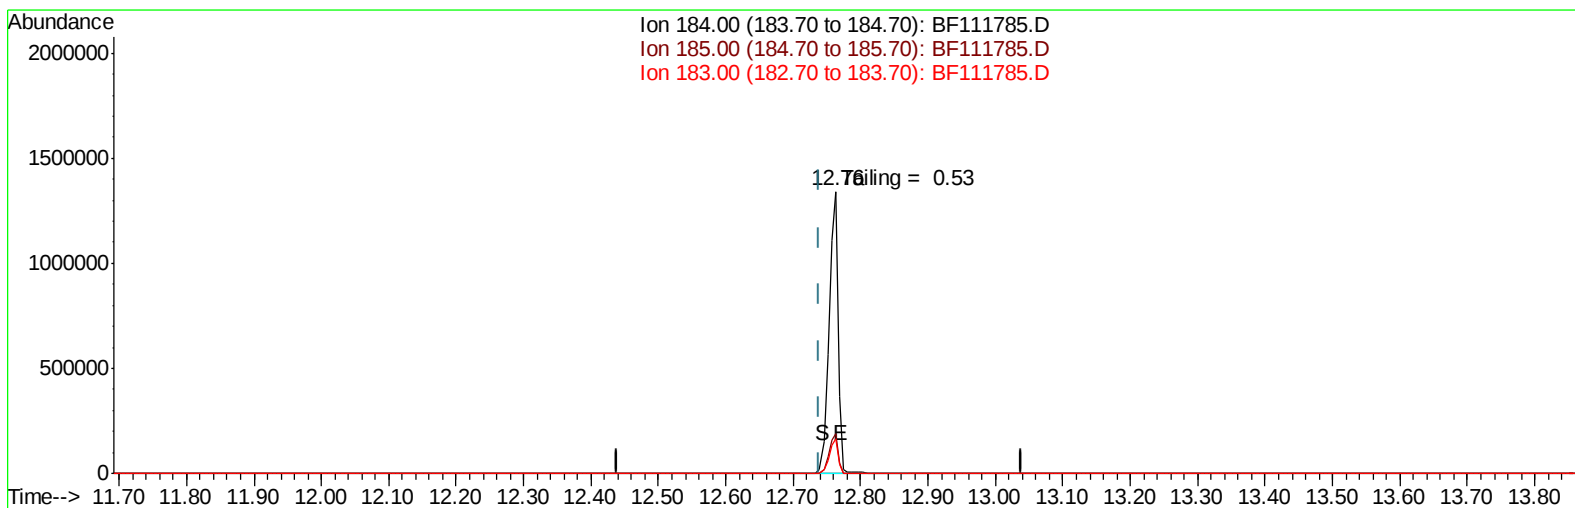

TIC: BF111785.D

(77) Benzidine

12.763min (+0.023) 130372.54ng

response 1275524

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	13.92
183.00	11.60	12.21
0.00	0.00	0.00