


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122818\
 Data File : BF111785.D
 Acq On : 28 Dec 2018 13:30
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 19 17:39:39 2018

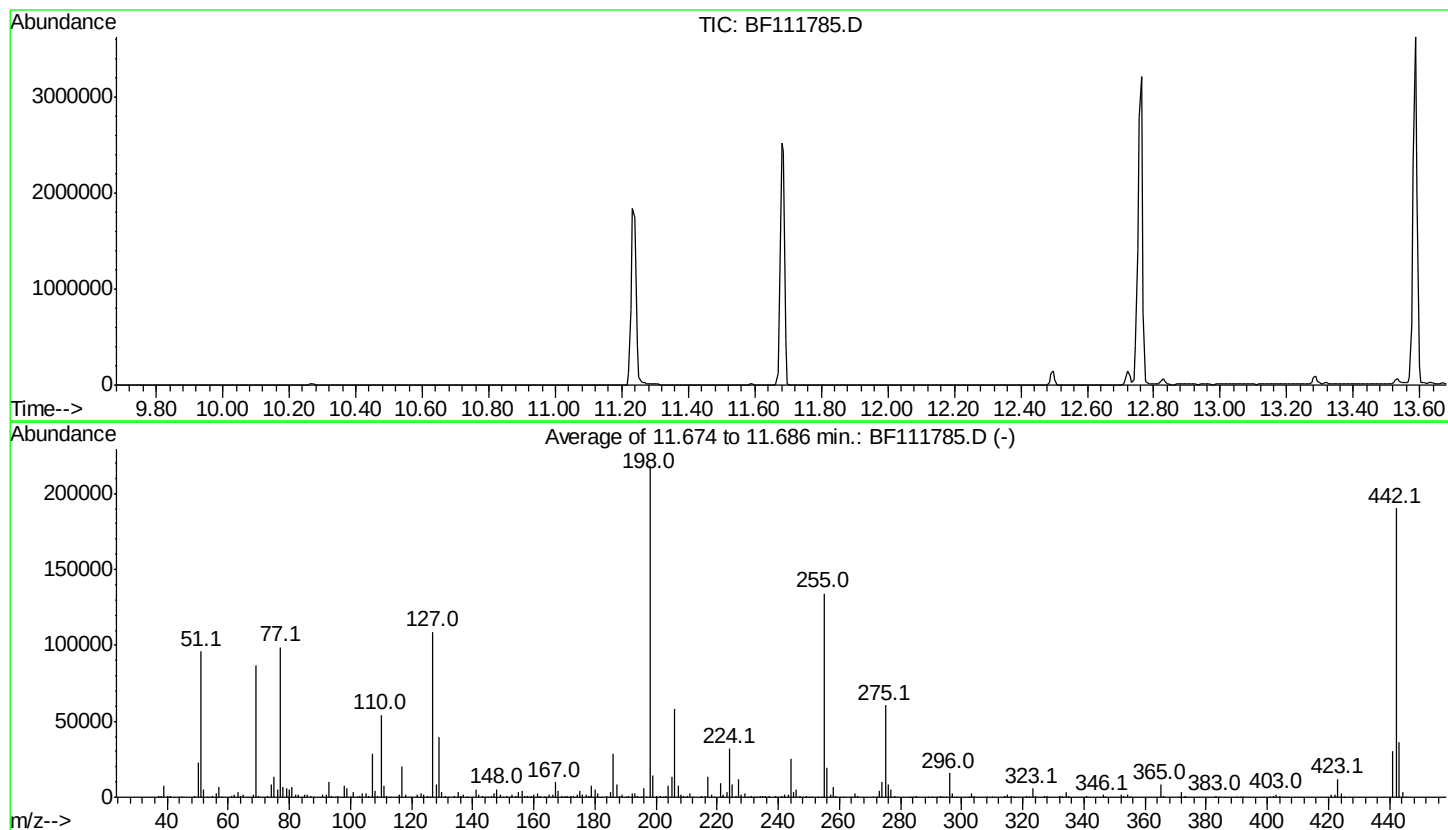

AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.9	95928	PASS
68	69	0.00	2	1.8	1576	PASS
69	198	0.00	100	39.8	86914	PASS
70	69	0.00	2	0.6	509	PASS
127	198	10	80	49.9	108960	PASS
197	198	0.00	2	0.1	220	PASS
198	198	100	100	100.0	218354	PASS
199	198	5	9	6.8	14759	PASS
275	198	10	60	27.7	60432	PASS
365	198	1	100	3.7	8156	PASS
441	198	0.01	100	13.7	29977	PASS
442	198	50	100	87.1	190117	PASS
443	442	15	24	19.1	36343	PASS