

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF122819\
 Data File : BF118363.D
 Acq On : 28 Dec 2019 14:09
 Operator : JU
 Sample : PB125767BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB125767BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF122419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.481	572	577	591	rBV	2371074	2490699	42.78%	7.414%
2	6.486	744	748	767	rBV	2602555	2650208	45.52%	7.889%
3	6.622	767	771	775	rBV	3133454	2844782	48.86%	8.468%
4	6.851	806	810	818	rVB	969611	804198	13.81%	2.394%
5	7.010	832	837	840	rBV	3663640	3221608	55.33%	9.589%
6	7.422	901	907	919	rBV	2090130	2404687	41.30%	7.158%
7	8.139	1024	1029	1045	rBV	997642	1030592	17.70%	3.068%
8	9.216	1207	1212	1228	rBV	4862878	5276426	90.63%	15.706%
9	9.904	1323	1329	1343	rVB	1173570	1258243	21.61%	3.745%
10	10.698	1459	1464	1478	rBV	2167175	2370675	40.72%	7.056%
11	11.398	1579	1583	1591	rBV	1262907	1326956	22.79%	3.950%
12	12.986	1848	1853	1856	rBV	5860156	5822261	100.00%	17.330%
13	14.051	2030	2034	2044	rBV	974569	1008157	17.32%	3.001%
14	15.151	2217	2221	2228	rBV	55647	67524	1.16%	0.201%
15	15.545	2282	2288	2302	rBV	512017	882491	15.16%	2.627%
16	15.986	2358	2363	2368	rVB2	46782	73085	1.26%	0.218%
17	16.492	2444	2449	2455	rBV2	32636	63031	1.08%	0.188%


Sum of corrected areas: 33595623

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF122819\
Data File : BF118363.D
Acq On : 28 Dec 2019 14:09
Operator : JU
Sample : PB125767BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB125767BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF122419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

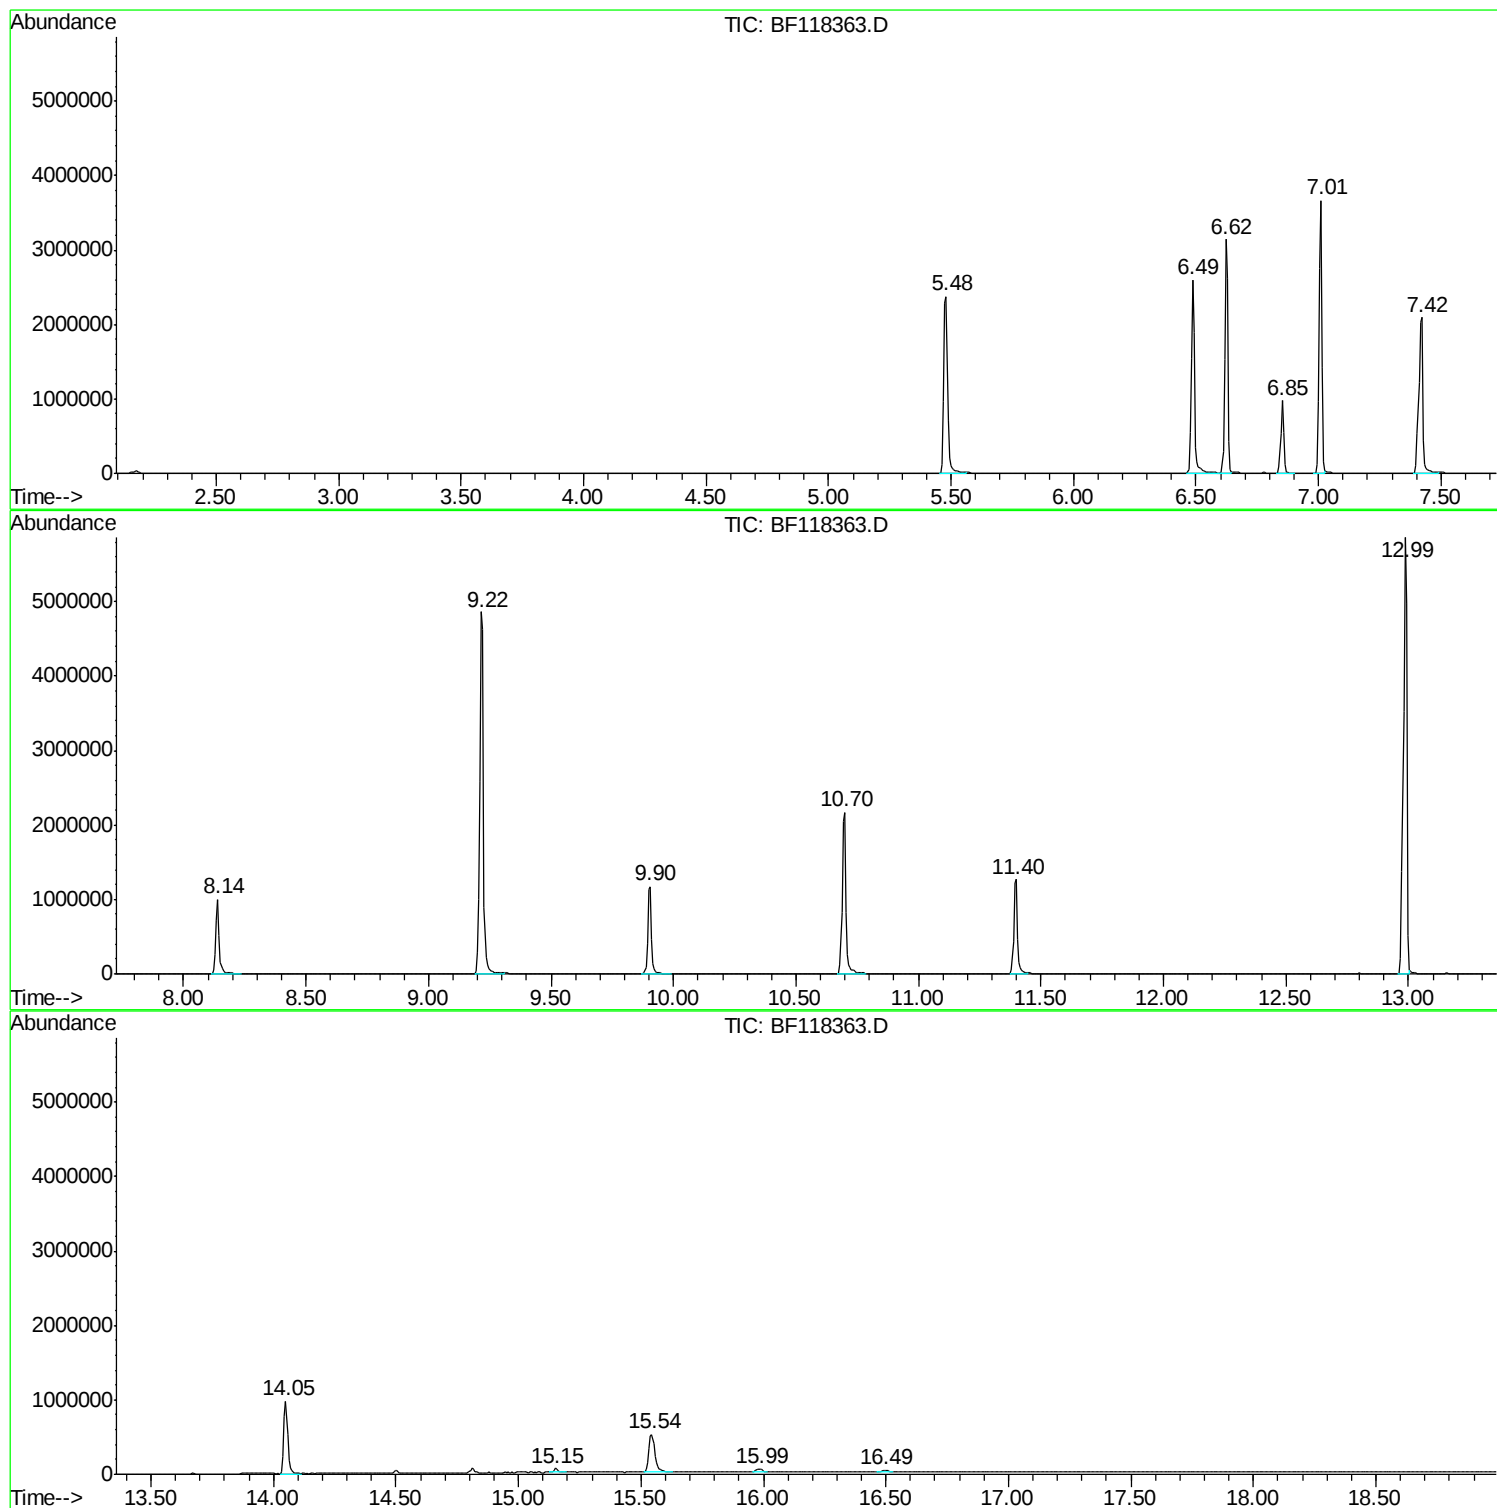

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF122819\
Data File : BF118363.D
Acq On : 28 Dec 2019 14:09
Operator : JU
Sample : PB125767BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB125767BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF122419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.62 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.62	70.75 ng	2844780	1,4-Dichlorobenzene-d4	6.85

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		5-Aminoindole	132	C8H8N2	005192-03-0	16
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	16
5		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9

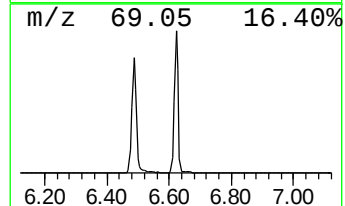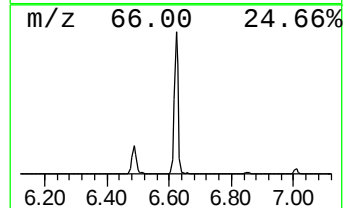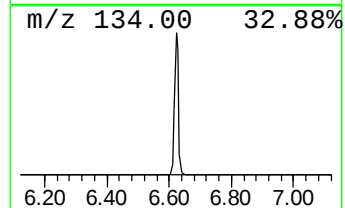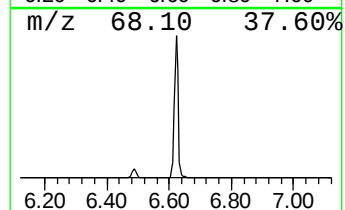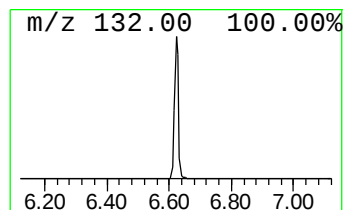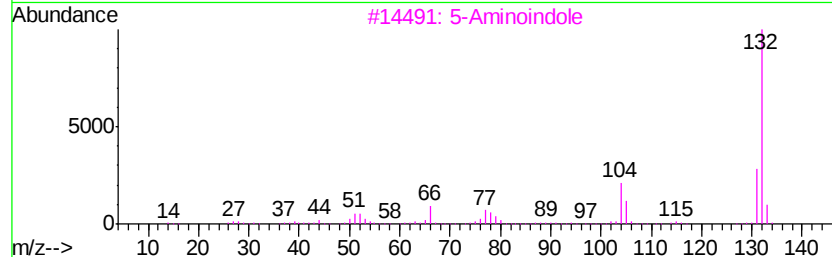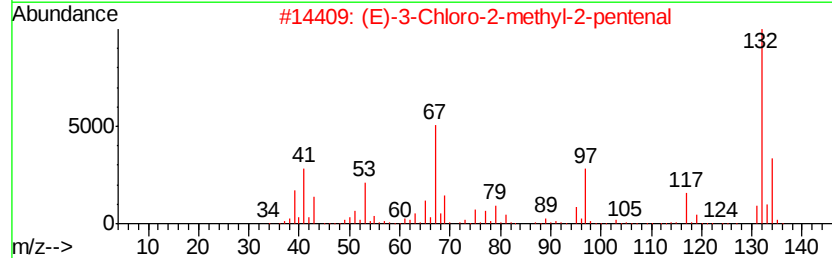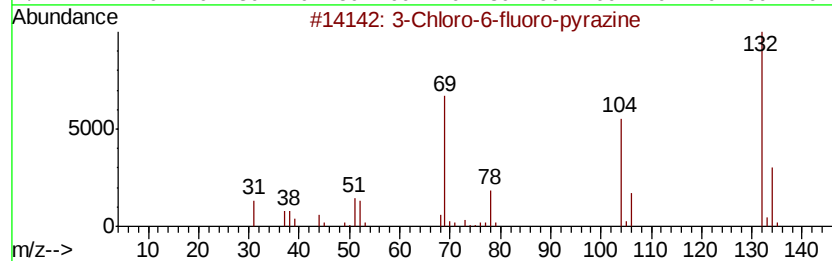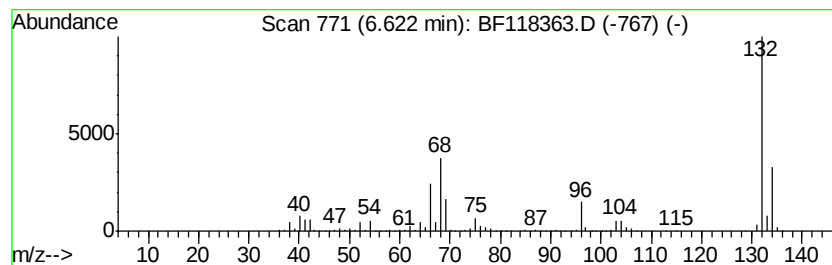

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF122819\
Data File : BF118363.D
Acq On : 28 Dec 2019 14:09
Operator : JU
Sample : PB125767BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB125767BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF122419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.62	6.62	70.8	ng	2844780	1	6.85	804198	20.0