


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF122819\
 Data File : BF118356.D
 Acq On : 28 Dec 2019 10:45
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF122419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 24 15:58:52 2019

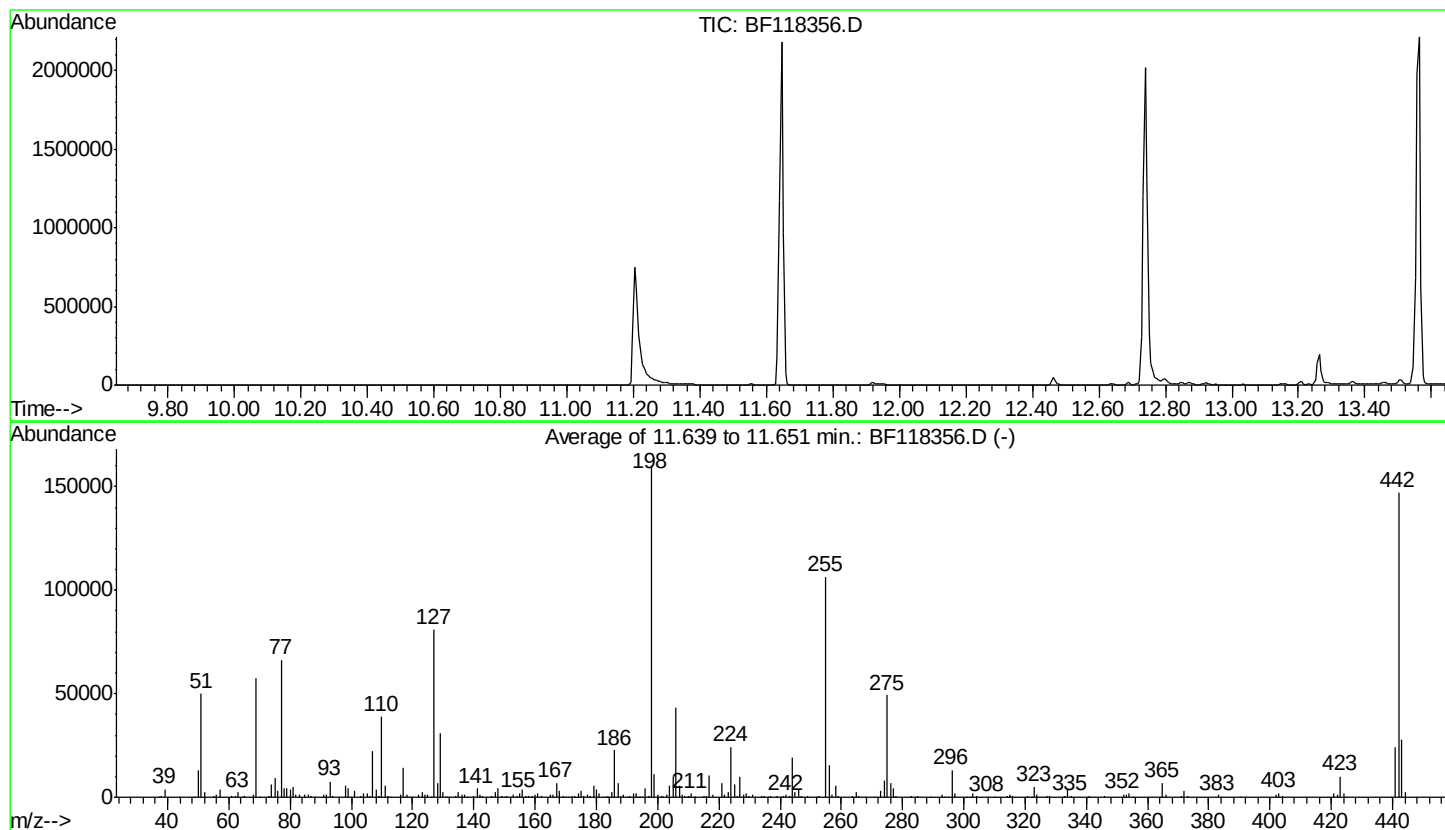

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.2	49941	PASS
68	69	0.00	2	2.0	1125	PASS
69	198	0.00	100	35.9	57546	PASS
70	69	0.00	2	0.5	293	PASS
127	198	10	80	50.4	80770	PASS
197	198	0.00	2	0.5	817	PASS
198	198	100	100	100.0	160141	PASS
199	198	5	9	6.9	11082	PASS
275	198	10	60	30.9	49440	PASS
365	198	1	100	4.3	6851	PASS
441	198	0.01	100	15.1	24208	PASS
442	198	50	100	91.8	146949	PASS
443	442	15	24	18.8	27624	PASS