


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122821\
 Data File : BF126377.D
 Acq On : 28 Dec 2021 11:48
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 22 13:00:11 2021

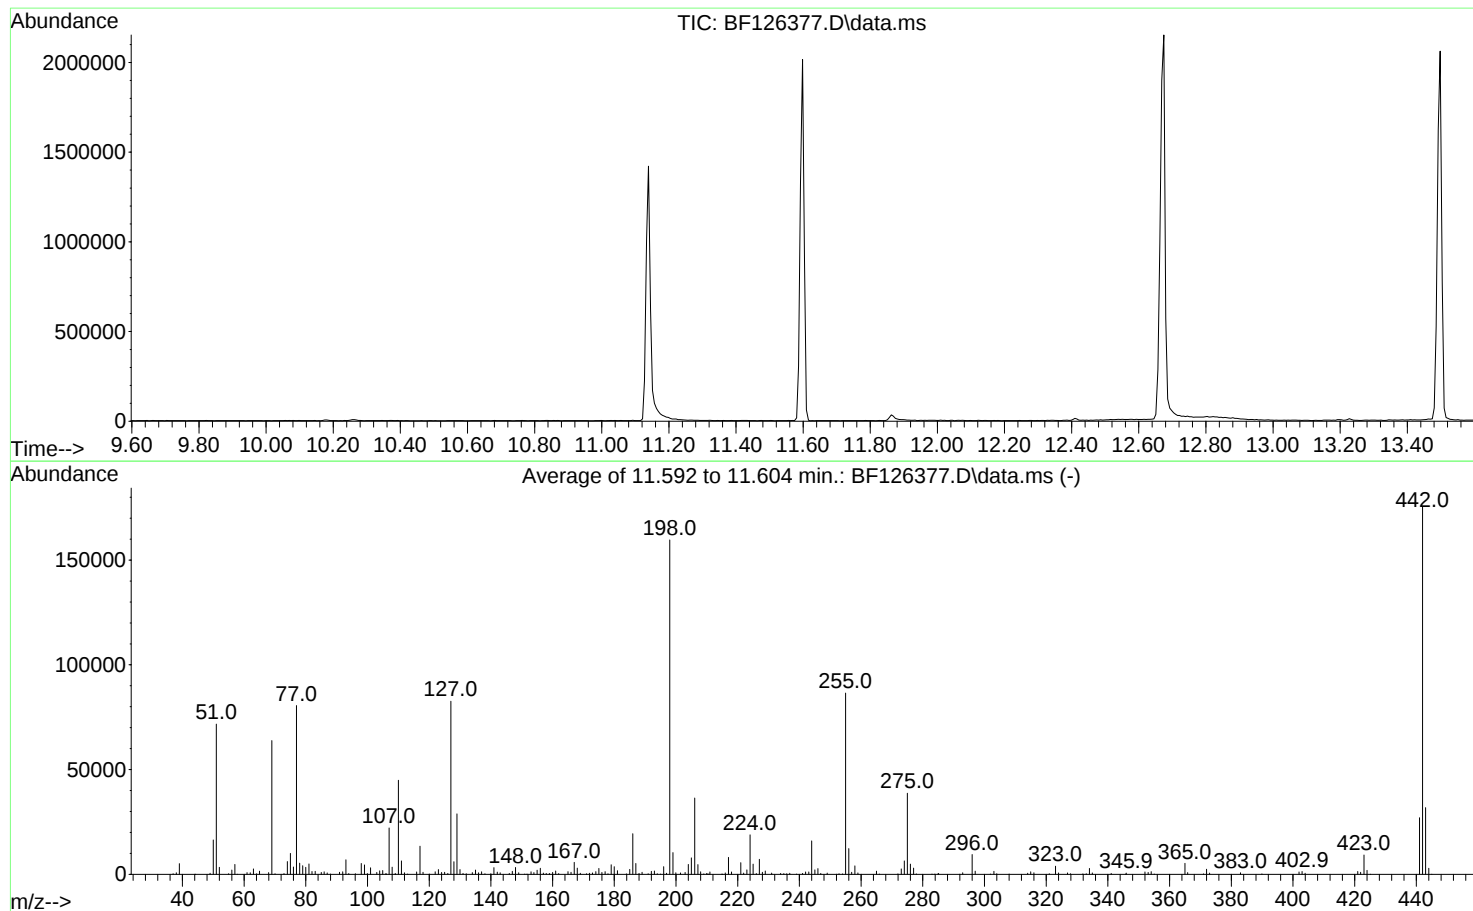

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.9	71720	PASS
68	69	0.00	2	1.3	861	PASS
69	198	0.00	100	40.0	63816	PASS
70	69	0.00	2	0.5	290	PASS
127	198	10	80	51.8	82624	PASS
197	198	0.00	2	0.3	505	PASS
198	198	100	100	100.0	159589	PASS
199	198	5	9	6.5	10385	PASS
275	198	10	60	24.2	38680	PASS
365	198	1	100	3.3	5271	PASS
441	198	0.01	100	17.0	27052	PASS
442	442	50	100	100.0	175560	PASS
443	442	15	24	18.1	31864	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/28/2021	BNA_F	<u>BF126377.D</u>
Compound Name	Response	Retention Time
DDT	351326	13.49
DDD	1394	13.19
DDE	474	12.86
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1868	353194	0.53

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122821\
 Data File : BF126377.D
 Acq On : 28 Dec 2021 11:48
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 28 15:26:15 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 22 13:00:11 2021
 Response via : Initial Calibration

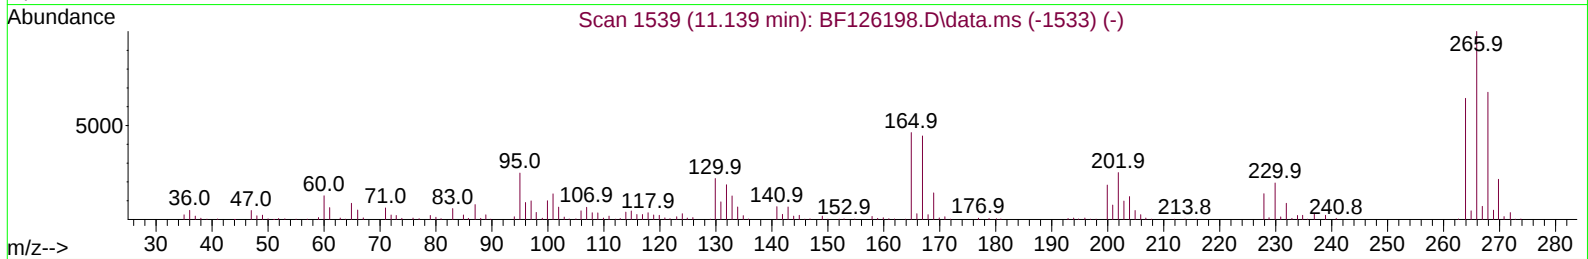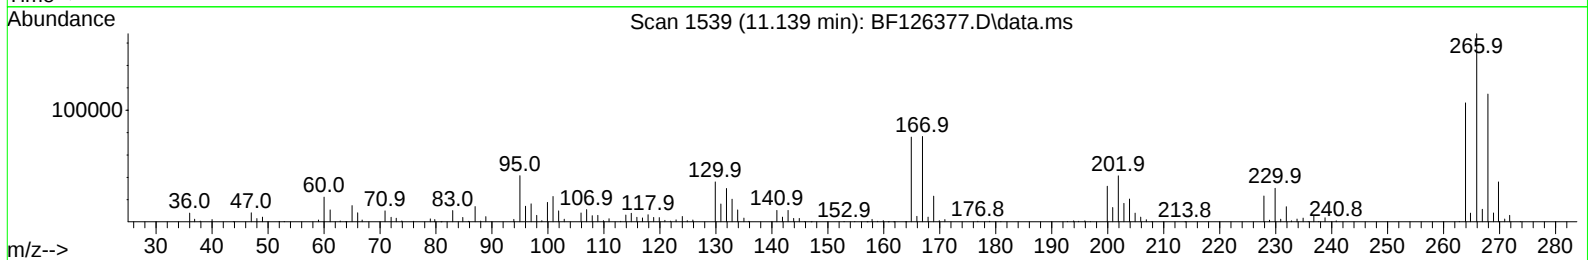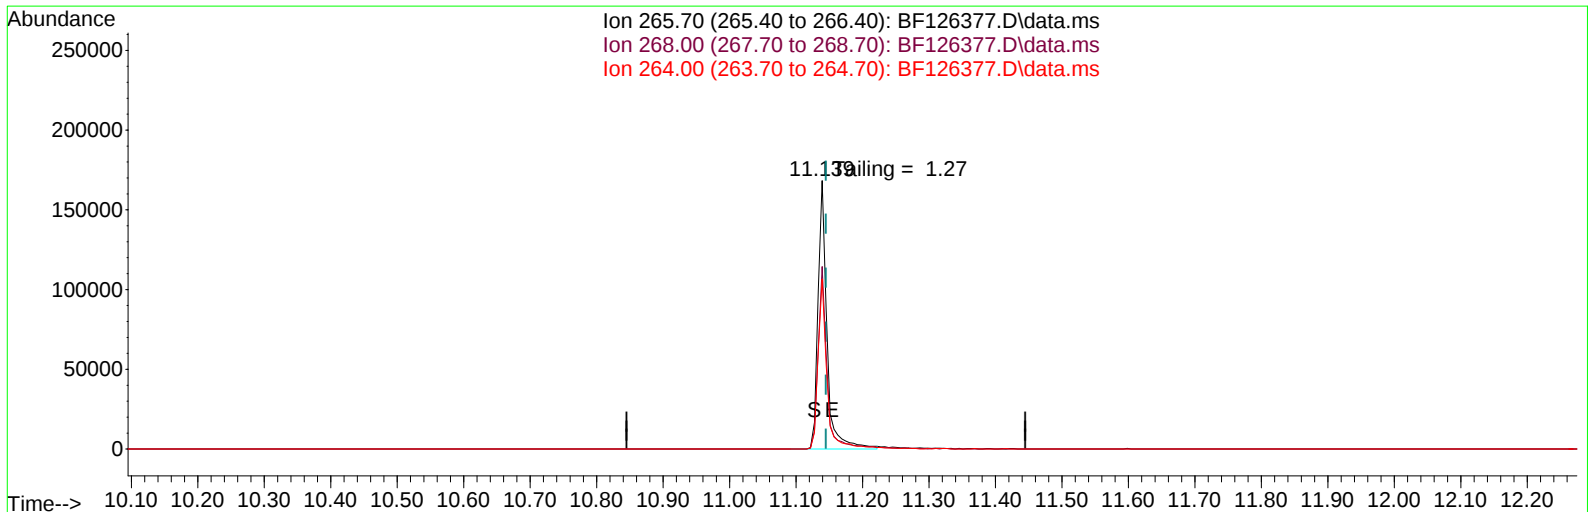

TIC: BF126377.D\data.ms

(70) Pentachlorophenol (C)

11.139min (-0.006) 51536.26 ng




response 161096

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	67.96
264.00	69.90	63.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122821\
 Data File : BF126377.D
 Acq On : 28 Dec 2021 11:48
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 28 15:26:15 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 22 13:00:11 2021
 Response via : Initial Calibration

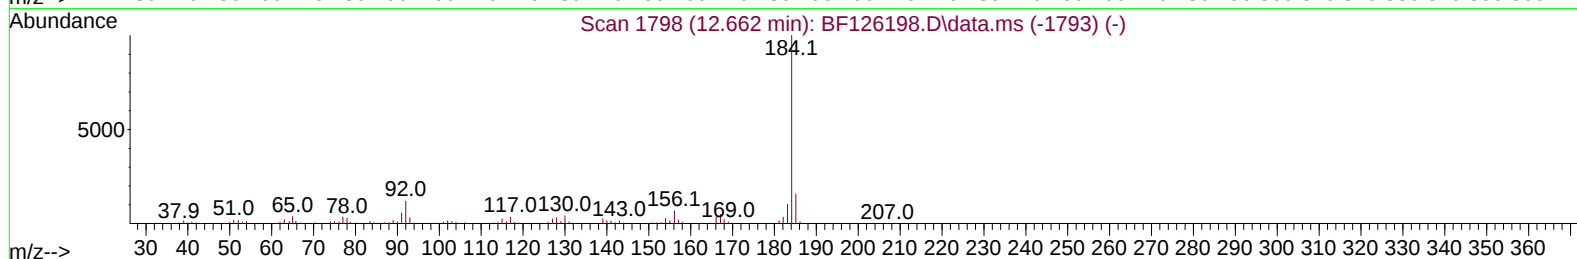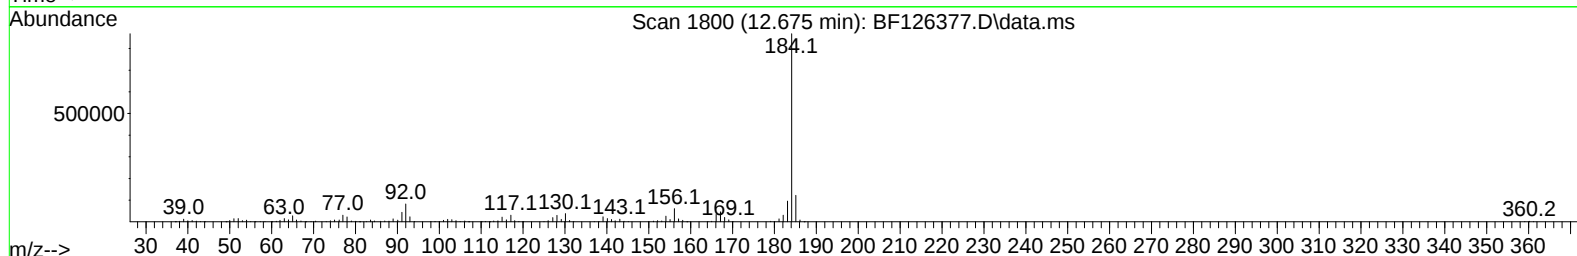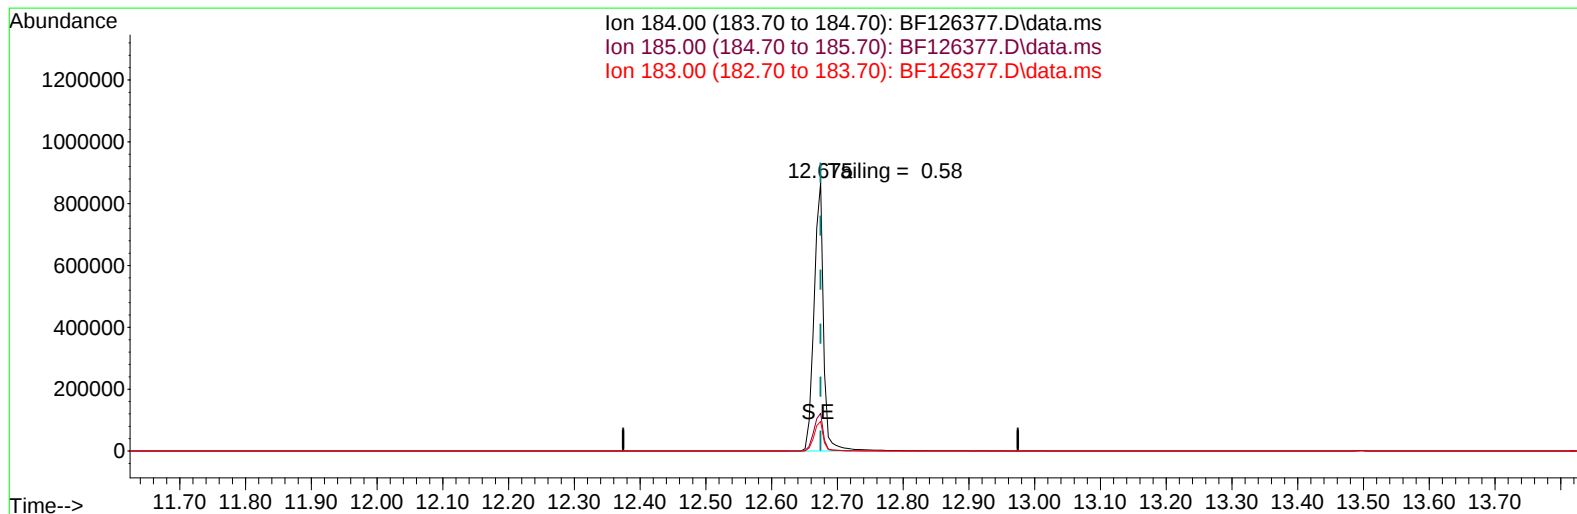

TIC: BF126377.D\data.ms

(77) Benzidine

12.675min (+ 0.000) 0.00 ng

response 877881

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.10
183.00	10.10	11.03
0.00	0.00	0.00