
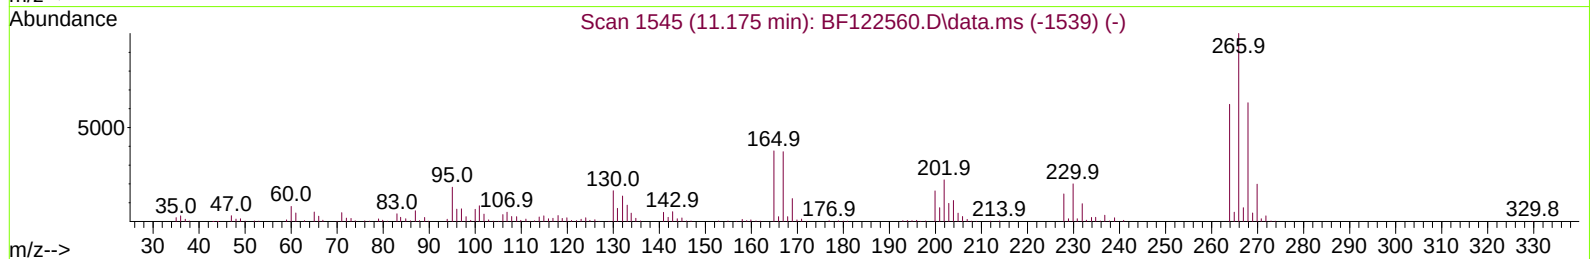
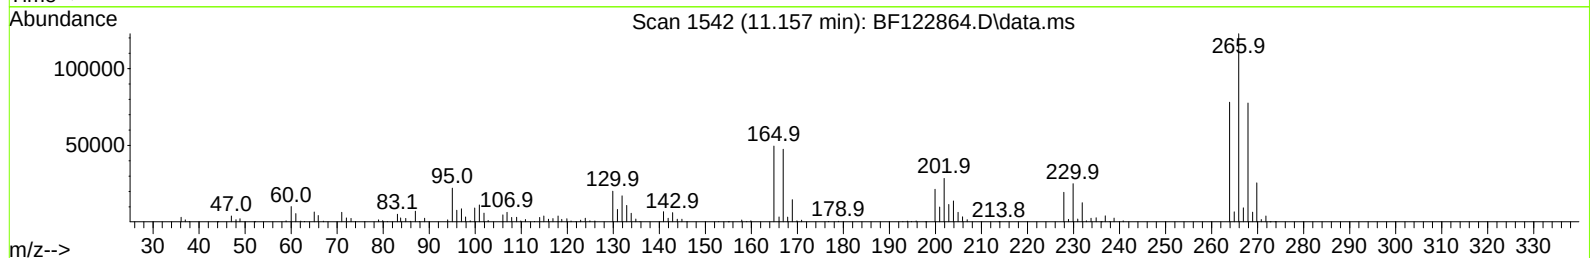


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122920\
Data File : BF122864.D
Acq On : 29 Dec 2020 14:16
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 30 01:00:35 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 15 18:14:23 2020
Response via : Initial Calibration

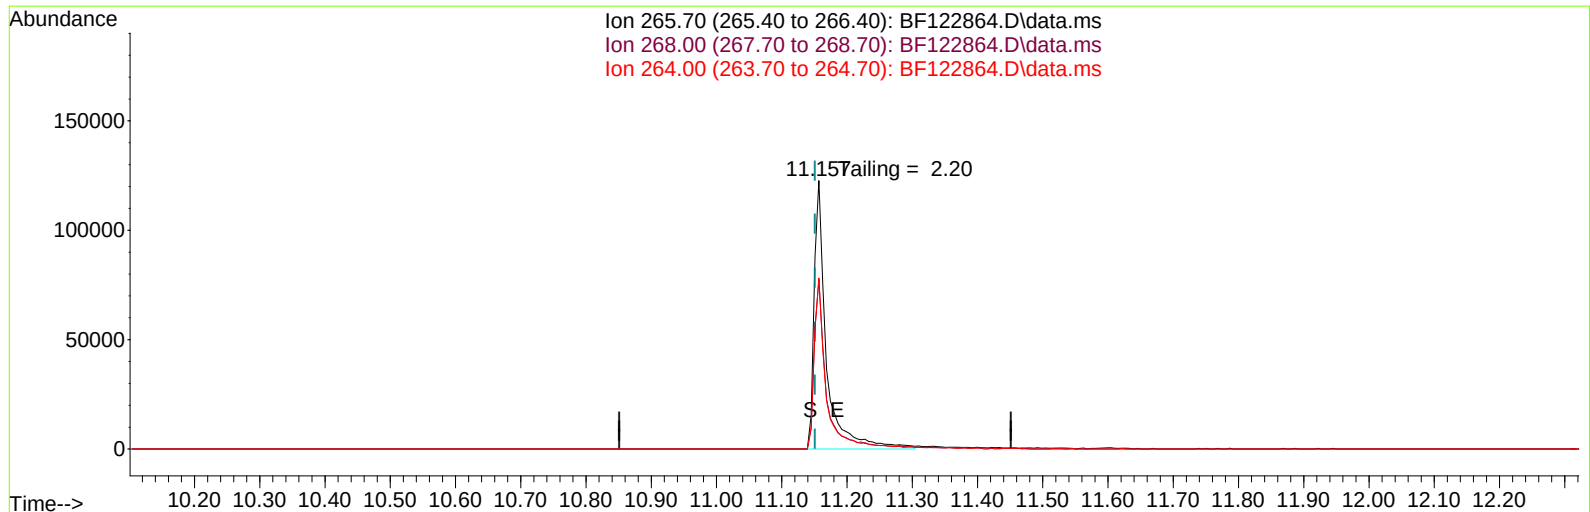

TIC: BF122864.D\data.ms

(70) Pentachlorophenol (C)




11.157min (+ 0.006) 34970.49 ng

response 163755

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.23
264.00	62.30	63.67
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122920\  
Data File : BF122864.D  
Acq On    : 29 Dec 2020  14:16  
Operator  : JU/CG  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Dec 30 01:00:35 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 15 18:14:23 2020
Response via : Initial Calibration

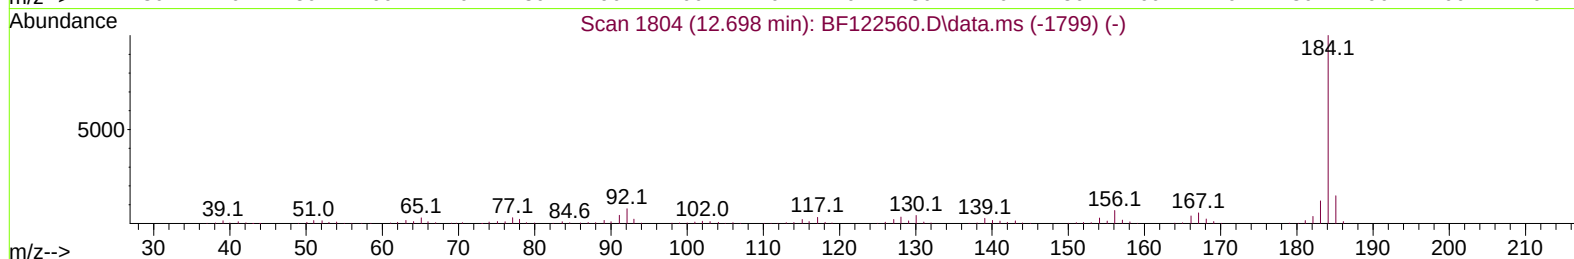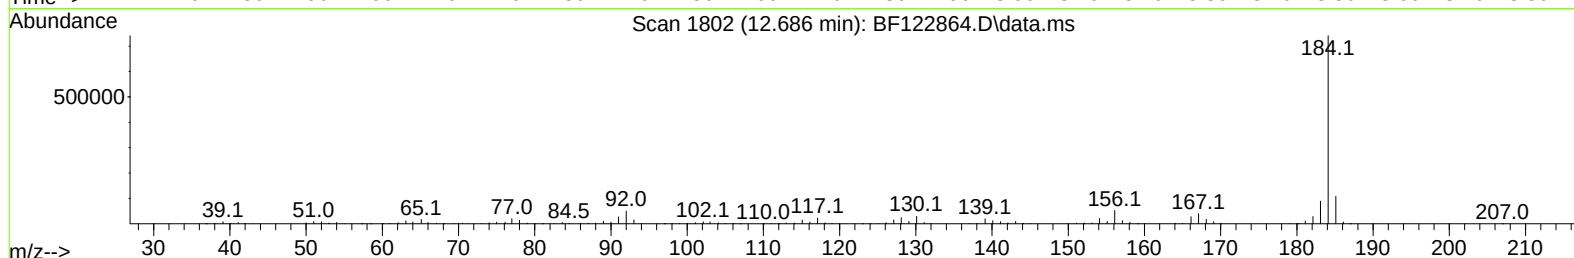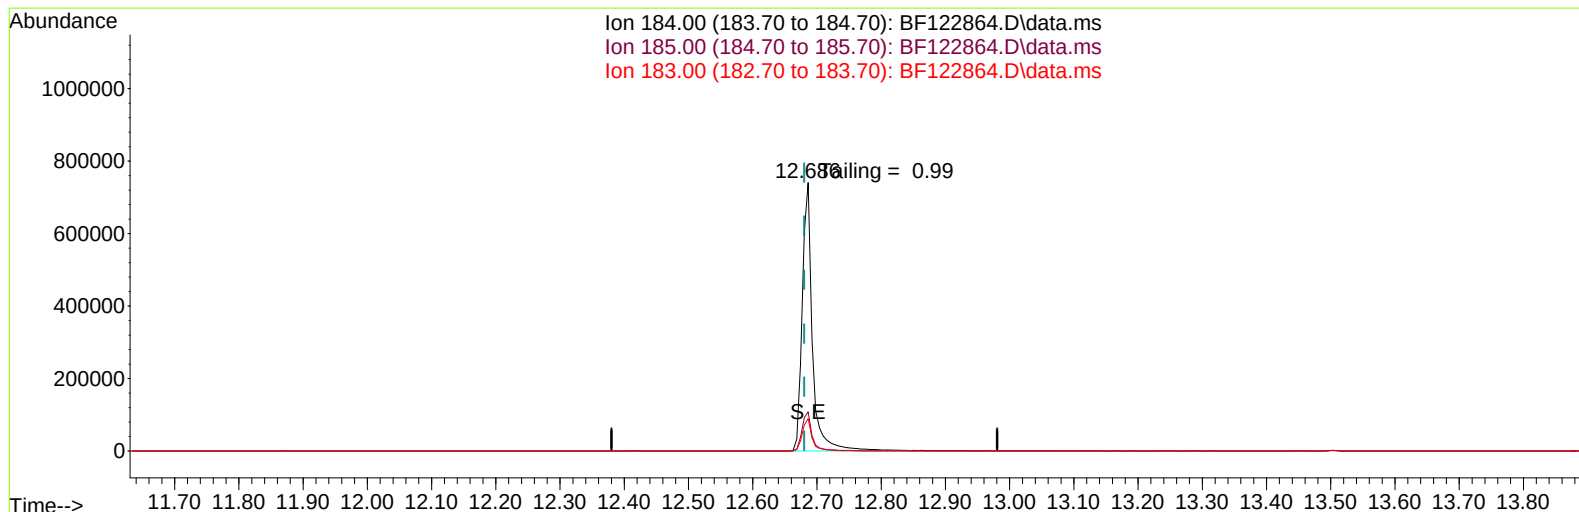

TIC: BF122864.D\data.ms

(77) Benzidine

12.686min (+ 0.006) 0.00 ng

response **822005**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.70	14.62
--------	-------	-------

183.00	12.10	12.04
--------	-------	-------

0.00 0.00 0.00