

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122920\
 Data File : BF122868.D
 Acq On : 29 Dec 2020 17:42
 Operator : JU/CG
 Sample : L5215-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 72-11991

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122868.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.134	3	8	23	rVB	376477	502735	10.96%	1.623%
2	5.445	567	571	574	rBV	3181864	3068119	66.90%	9.902%
3	6.457	738	743	770	rBV	2910789	3342839	72.89%	10.789%
4	6.816	801	804	814	rVB	1224966	1016272	22.16%	3.280%
5	7.386	895	901	913	rBV	2035593	2207301	48.13%	7.124%
6	8.104	1018	1023	1044	rBV	1412478	1349615	29.43%	4.356%
7	9.180	1200	1206	1209	rBV	4214867	3996307	87.14%	12.898%
8	9.292	1221	1225	1238	rVB4	28185	55194	1.20%	0.178%
9	9.569	1268	1272	1282	rBV	236582	251236	5.48%	0.811%
10	9.857	1316	1321	1333	rBV	1690645	1574415	34.33%	5.081%
11	10.192	1367	1378	1379	rBV5	15905	46162	1.01%	0.149%
12	10.651	1451	1456	1472	rBV	2577564	2812506	61.33%	9.077%
13	11.345	1570	1574	1581	rBV	1754157	1587899	34.63%	5.125%
14	11.869	1660	1663	1671	rBV2	213124	286949	6.26%	0.926%
15	12.563	1778	1781	1785	rVB2	38867	49074	1.07%	0.158%
16	12.651	1794	1796	1801	rBV2	41554	47325	1.03%	0.153%
17	12.933	1838	1844	1847	rBV	4413102	4585972	100.00%	14.801%
18	13.863	1994	2002	2017	rBV3	190183	717231	15.64%	2.315%
19	13.986	2019	2023	2035	rVB	1360858	1387408	30.25%	4.478%
20	14.445	2099	2101	2106	rVB2	69038	67800	1.48%	0.219%
21	14.510	2107	2112	2124	rBV6	68564	246692	5.38%	0.796%
22	15.086	2206	2210	2214	rVB	125776	141450	3.08%	0.457%
23	15.451	2266	2272	2281	rBV	928219	1238548	27.01%	3.997%
24	15.886	2341	2346	2353	rBV	98296	149717	3.26%	0.483%
25	16.009	2363	2367	2369	rBV3	41129	64707	1.41%	0.209%
26	16.380	2426	2430	2434	rBV	39357	67537	1.47%	0.218%
27	16.956	2524	2528	2537	rVB3	34630	70374	1.53%	0.227%
28	17.133	2554	2558	2563	rBV5	26917	52721	1.15%	0.170%




Sum of corrected areas: 30984105

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122920\
Data File : BF122868.D
Acq On : 29 Dec 2020 17:42
Operator : JU/CG
Sample : L5215-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
72-11991

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

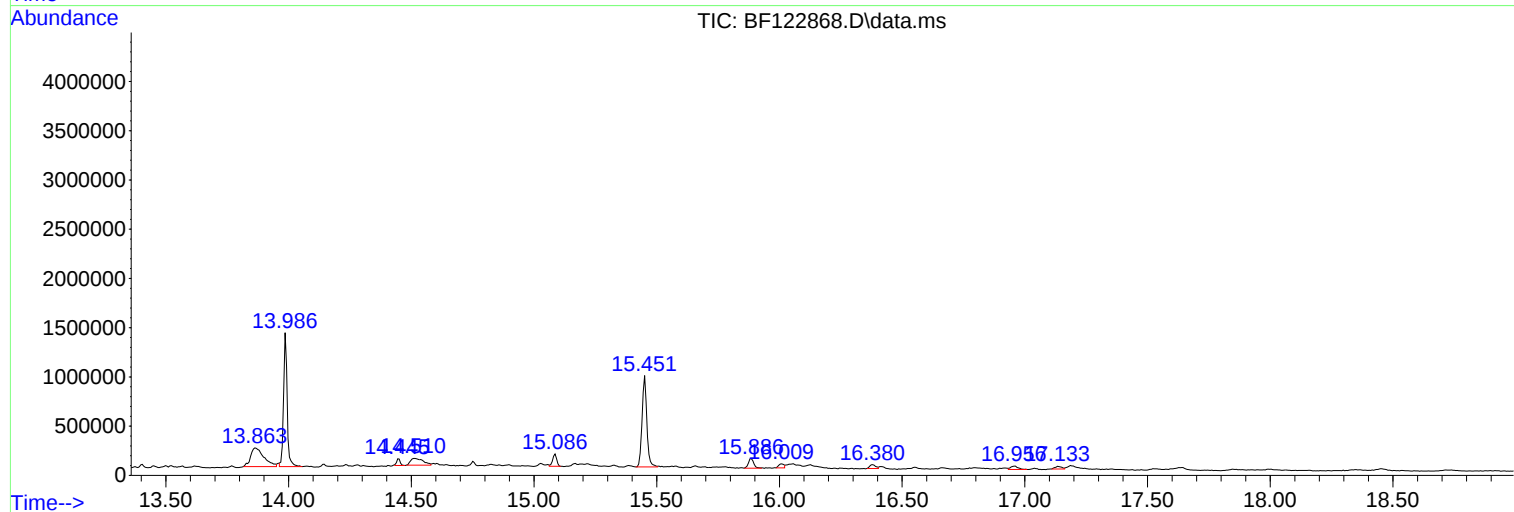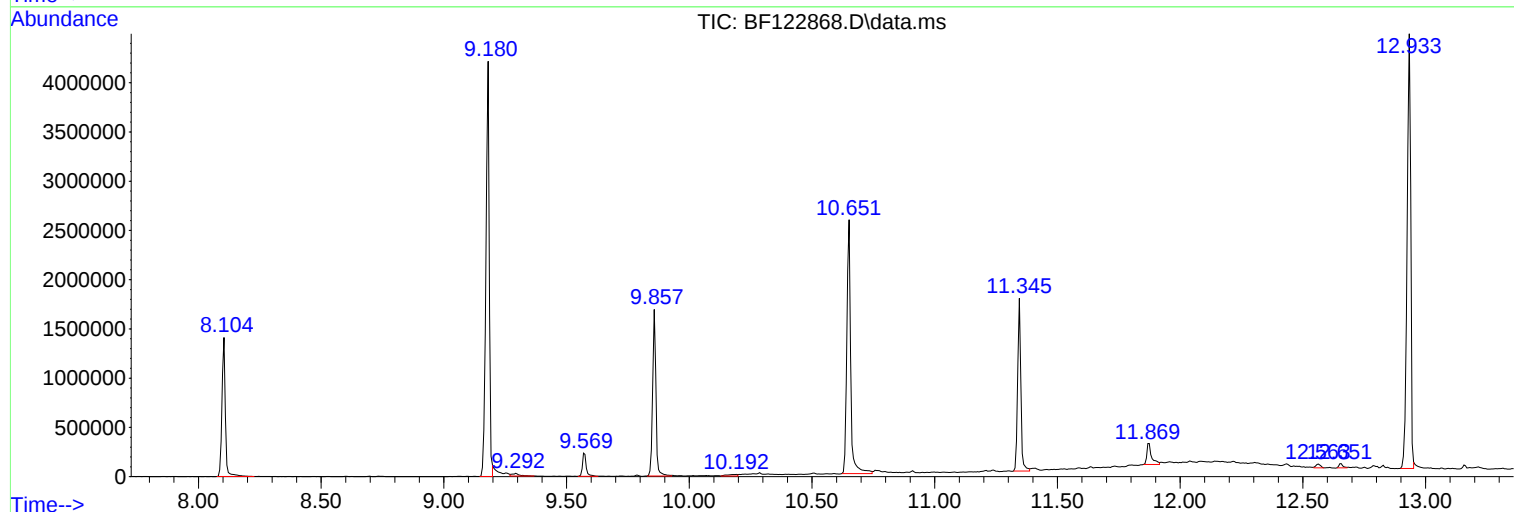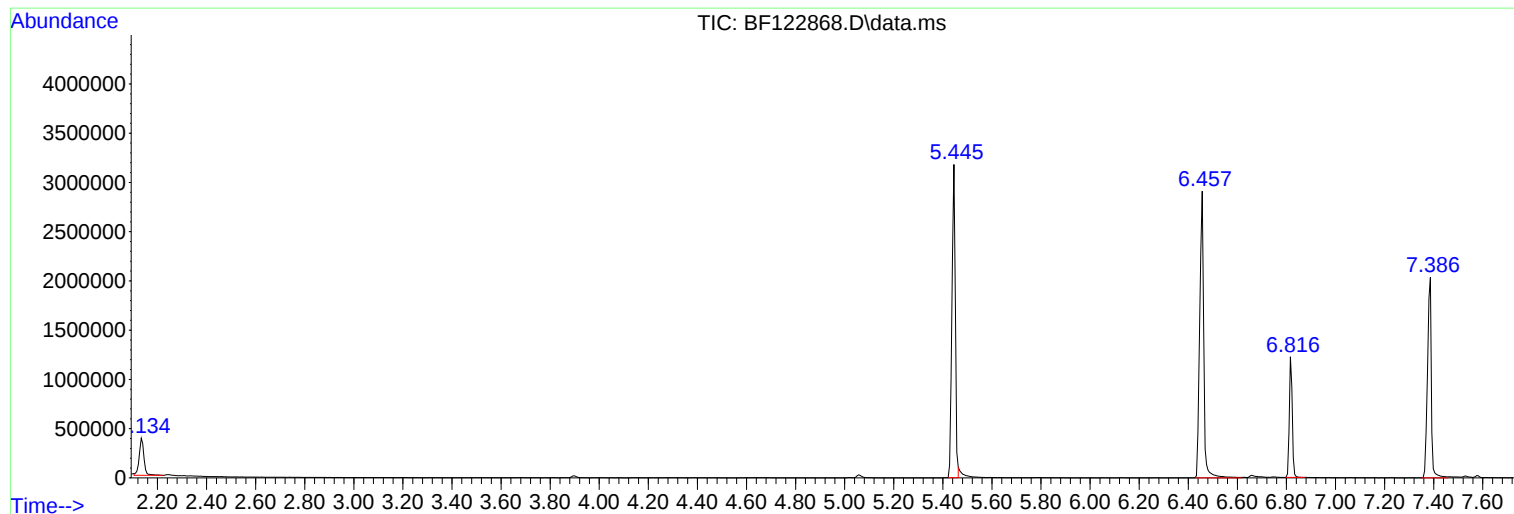

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122920\
Data File : BF122868.D
Acq On : 29 Dec 2020 17:42
Operator : JU/CG
Sample : L5215-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
72-11991

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122920\
Data File : BF122868.D
Acq On : 29 Dec 2020 17:42
Operator : JU/CG
Sample : L5215-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
72-11991

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
