
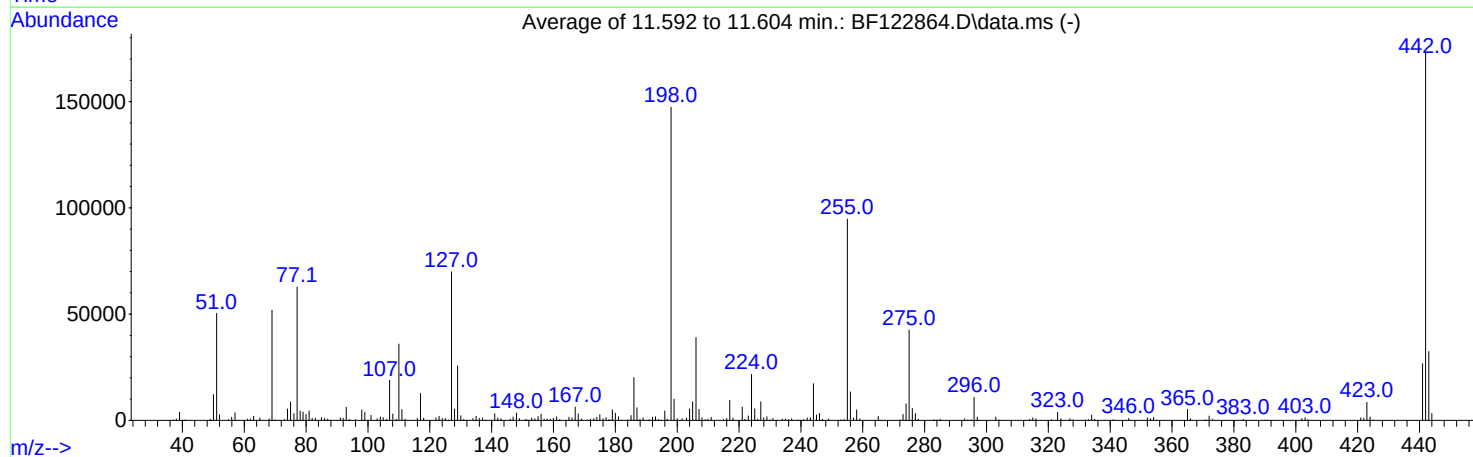


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122920\
 Data File : BF122864.D
 Acq On : 29 Dec 2020 14:16
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 15 18:14:23 2020

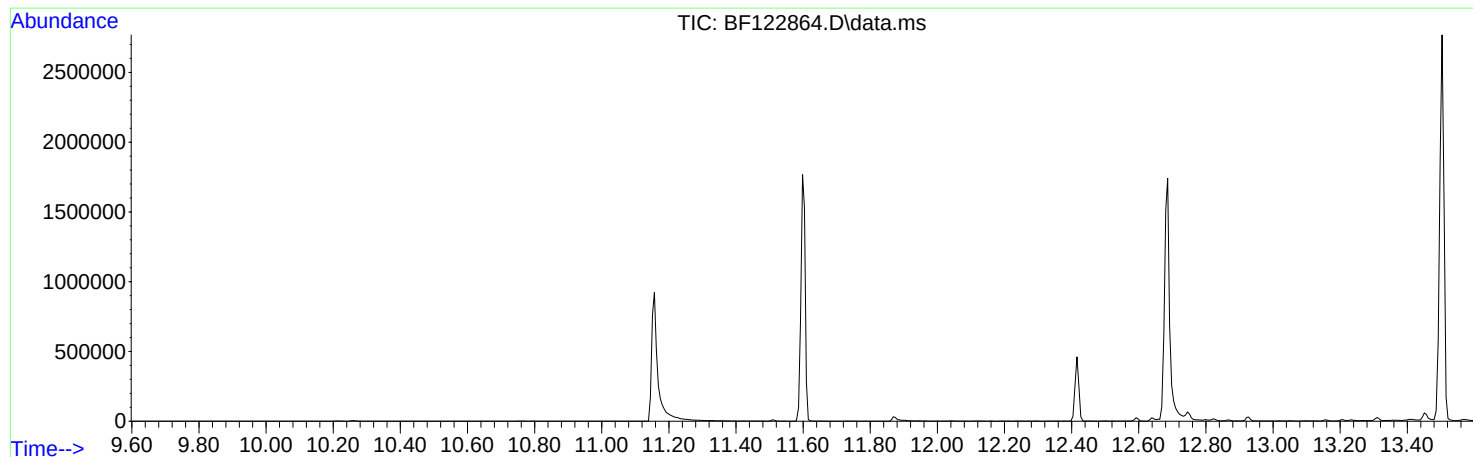

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	50339	PASS
68	69	0.00	2	1.4	749	PASS
69	198	0.00	100	35.2	51864	PASS
70	69	0.00	2	0.4	224	PASS
127	198	10	80	47.4	69891	PASS
197	198	0.00	2	0.4	610	PASS
198	198	100	100	100.0	147328	PASS
199	198	5	9	6.8	10053	PASS
275	198	10	60	28.8	42456	PASS
365	198	1	100	3.5	5191	PASS
441	198	0.01	100	18.1	26662	PASS
442	442	100	100	100.0	173107	PASS
443	442	15	24	18.7	32363	PASS