
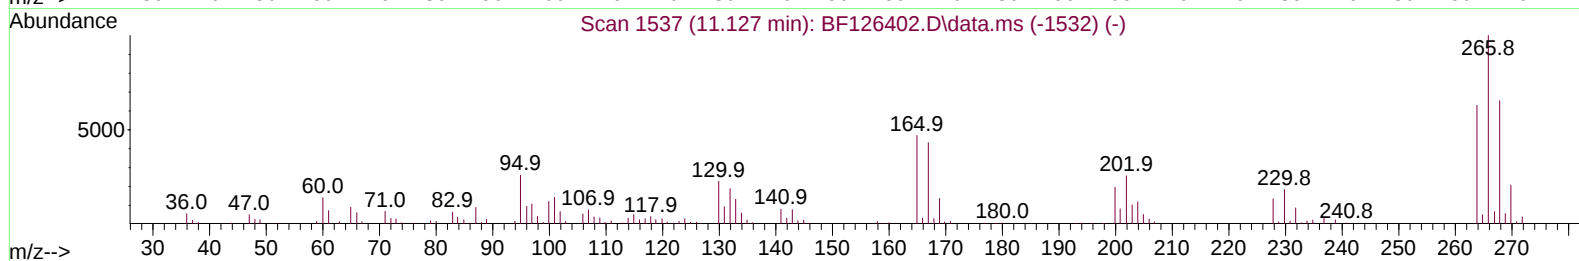
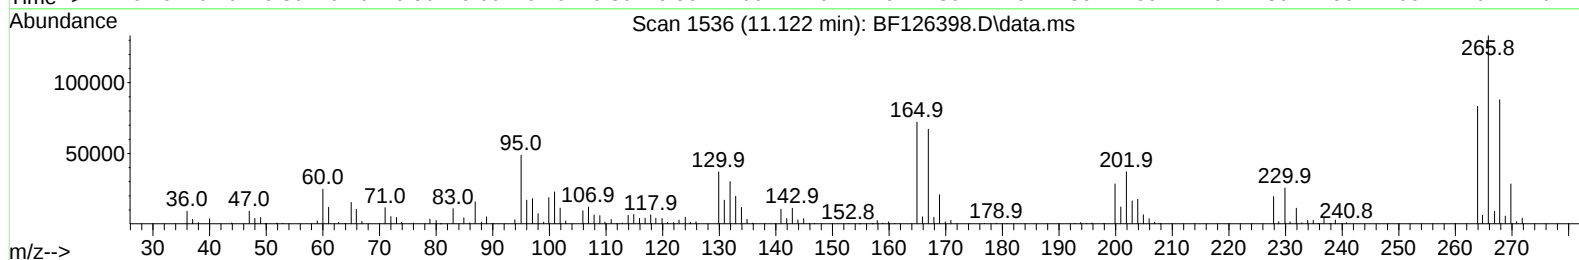


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122921\
Data File : BF126398.D
Acq On : 29 Dec 2021 16:45
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 30 05:25:56 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 30 04:30:49 2021
Response via : Initial Calibration

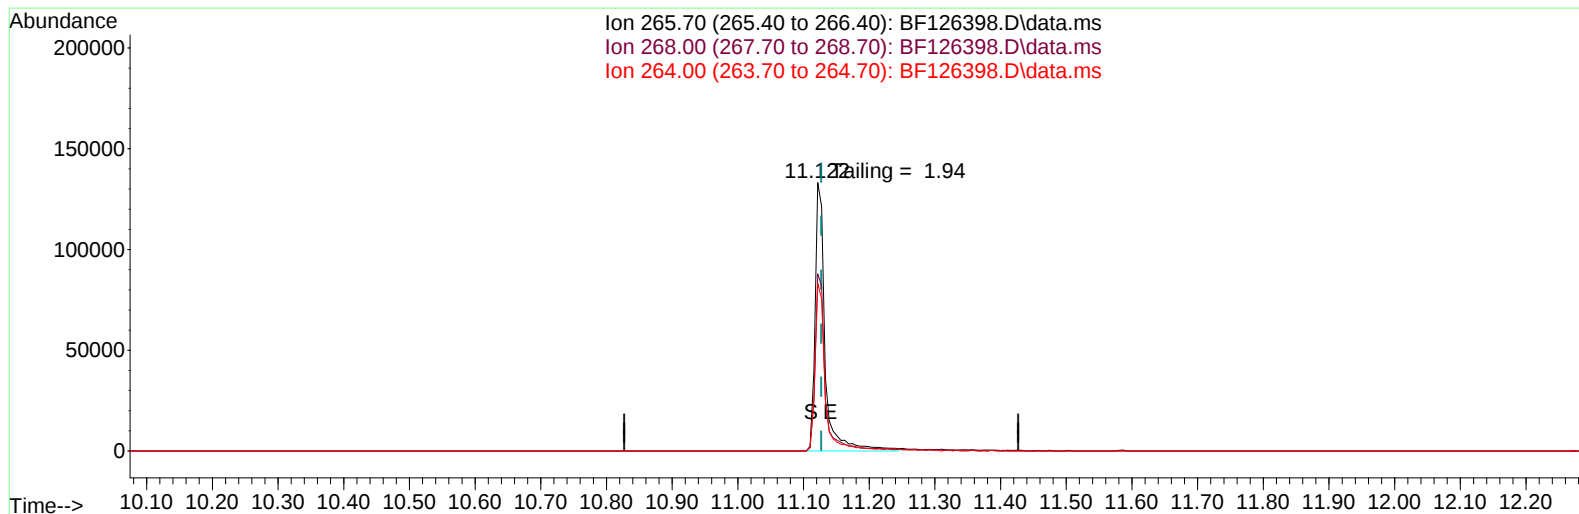

TIC: BF126398.D\data.ms

(70) Pentachlorophenol (C)




11.122min (-0.005) 56532.35 ng

response 144961

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	66.03
264.00	63.00	62.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122921\
Data File : BF126398.D
Acq On : 29 Dec 2021 16:45
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 30 05:25:56 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 30 04:30:49 2021
Response via : Initial Calibration

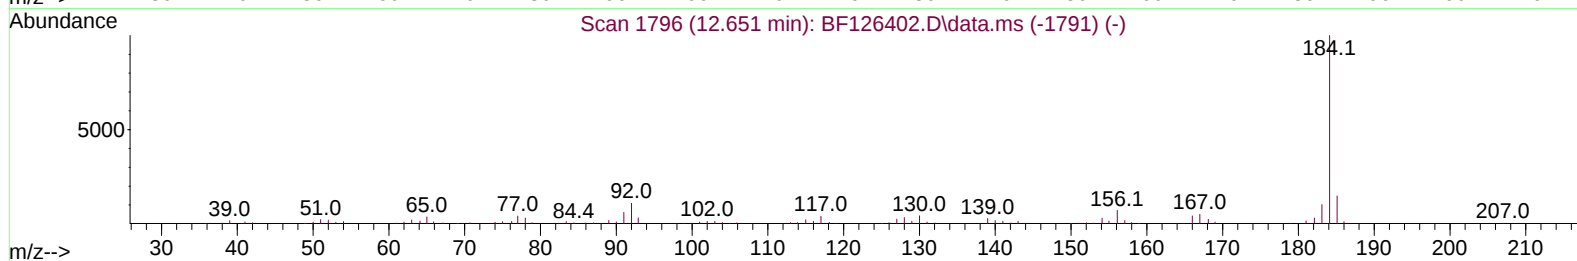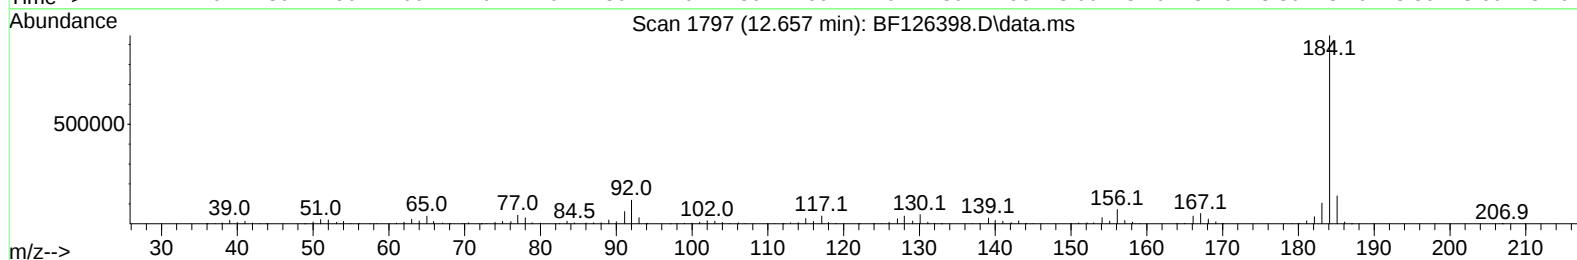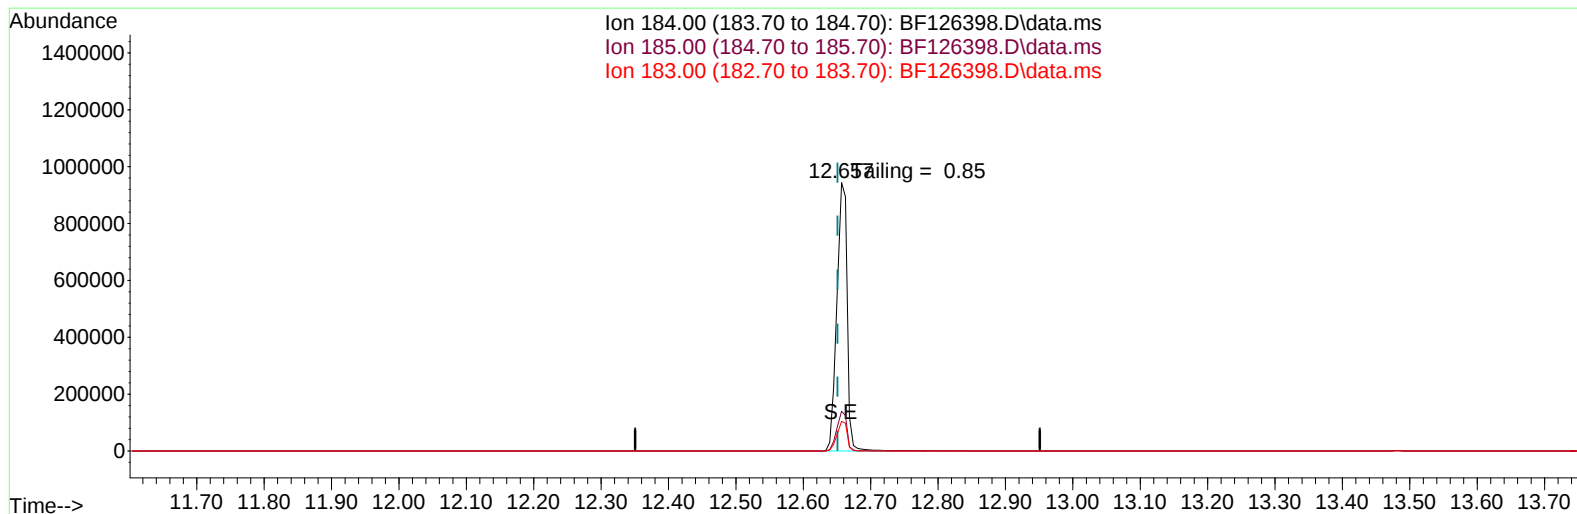

TIC: BF126398.D\data.ms

(77) Benzidine

12.657min (+ 0.006) 86378.08 ng

response 1010082

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.81
183.00	10.20	11.02
0.00	0.00	0.00