

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122921\
 Data File : BF126407.D
 Acq On : 29 Dec 2021 23:08
 Operator : JU/CG
 Sample : PB141666BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB141666BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126407.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.028	496	500	514	rVB	47291	64234	1.43%	0.229%
2	5.416	560	566	569	rBV	4013443	4448314	99.09%	15.861%
3	6.428	732	738	741	rBV	3748849	4489348	100.00%	16.008%
4	6.792	797	800	804	rBV	1067677	953853	21.25%	3.401%
5	7.357	890	896	899	rBV	2753396	3132158	69.77%	11.168%
6	8.075	1014	1018	1022	rBV	1301840	1308526	29.15%	4.666%
7	9.157	1196	1202	1205	rBV	4047592	4107376	91.49%	14.646%
8	9.833	1312	1317	1320	rBV	1551298	1286170	28.65%	4.586%
9	10.621	1447	1451	1454	rBV	2372177	2212753	49.29%	7.890%
10	11.316	1565	1569	1573	rBV	1367284	1175703	26.19%	4.192%
11	12.910	1835	1840	1843	rBV	3415783	3390007	75.51%	12.088%
12	13.957	2014	2018	2021	rBV	821665	799329	17.81%	2.850%
13	15.392	2257	2262	2267	rBV	551369	677021	15.08%	2.414%




Sum of corrected areas: 28044792

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122921\
Data File : BF126407.D
Acq On : 29 Dec 2021 23:08
Operator : JU/CG
Sample : PB141666BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB141666BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

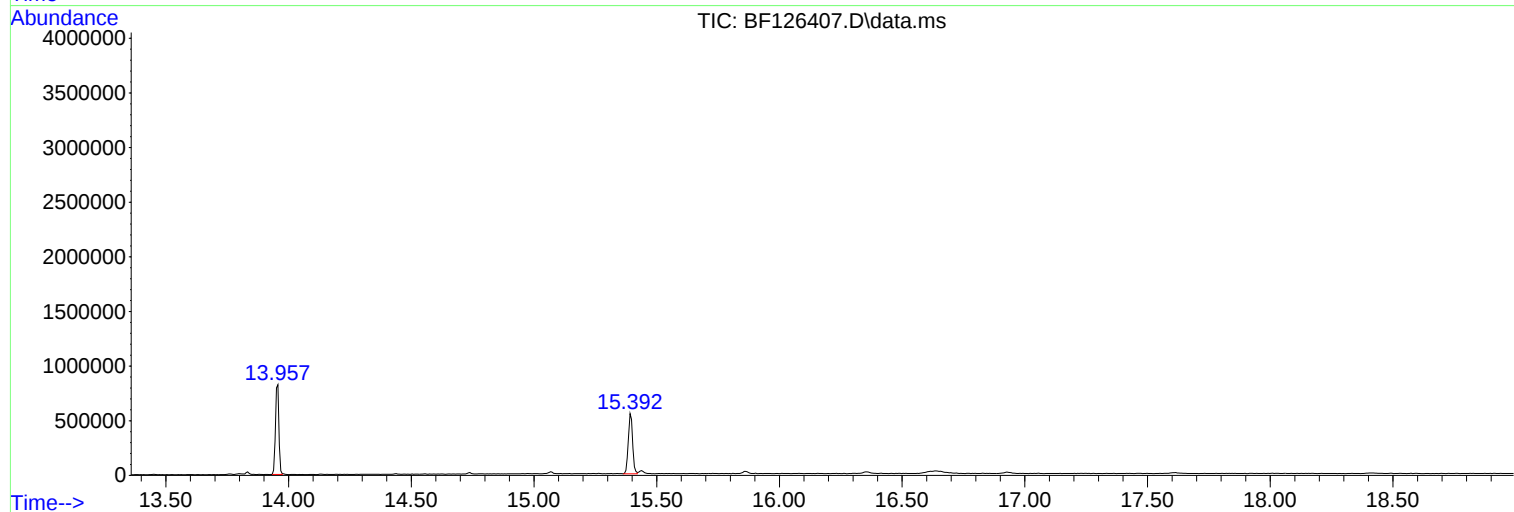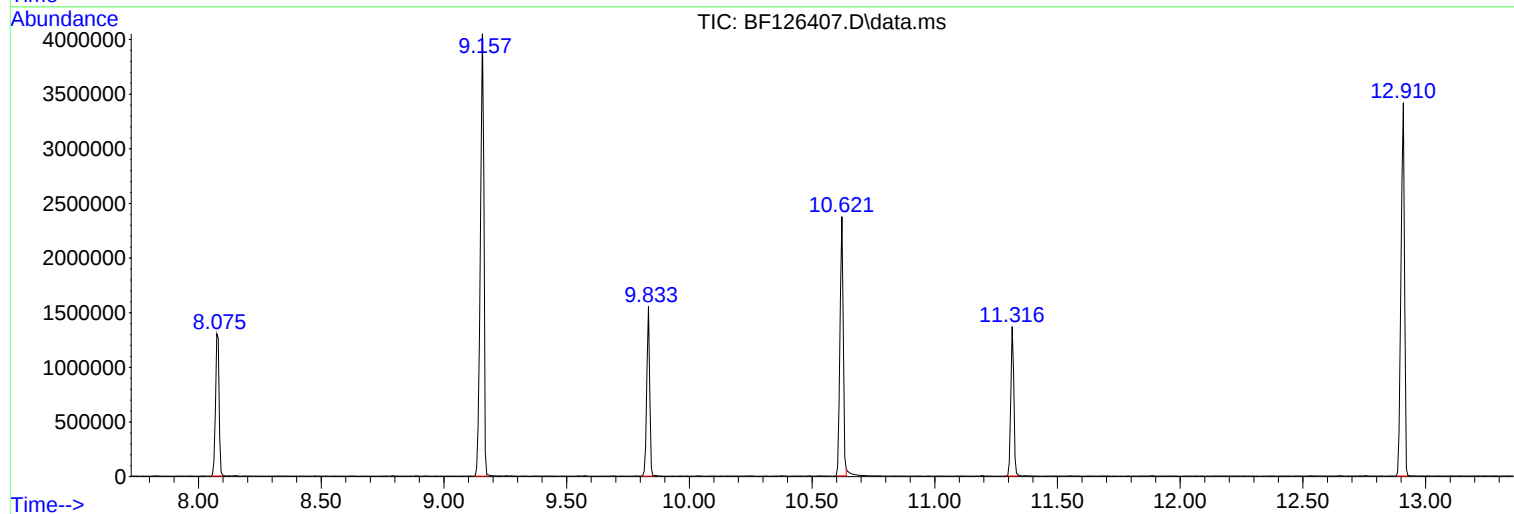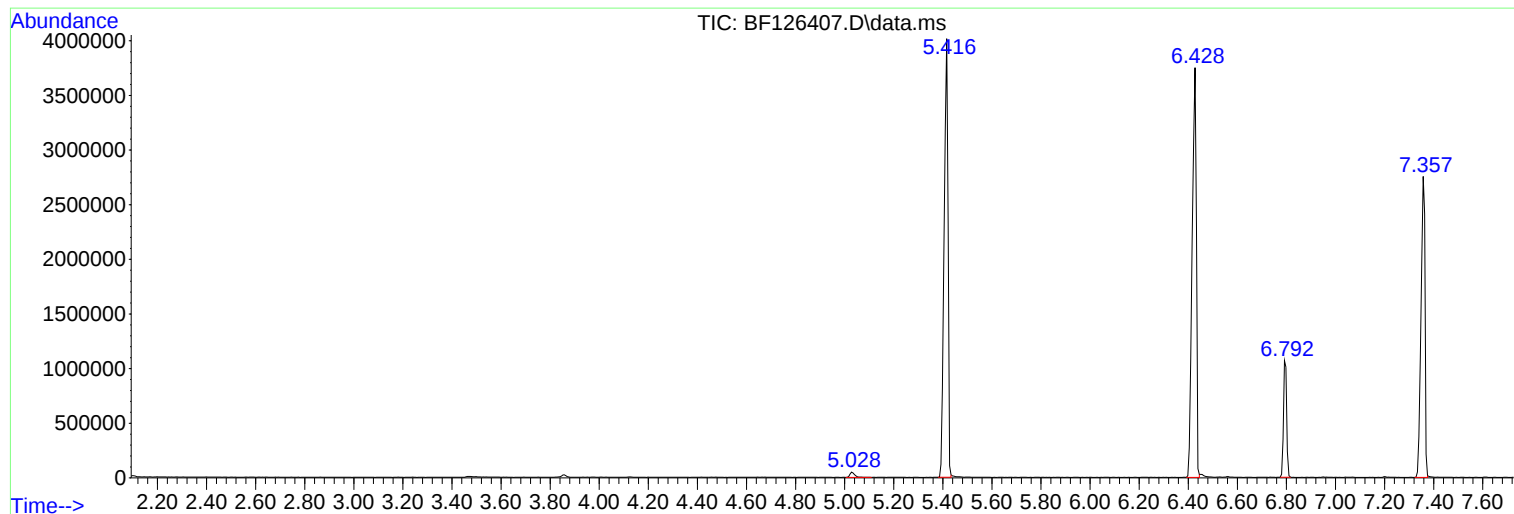

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122921\
Data File : BF126407.D
Acq On : 29 Dec 2021 23:08
Operator : JU/CG
Sample : PB141666BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB141666BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122921\
Data File : BF126407.D
Acq On : 29 Dec 2021 23:08
Operator : JU/CG
Sample : PB141666BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB141666BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------