
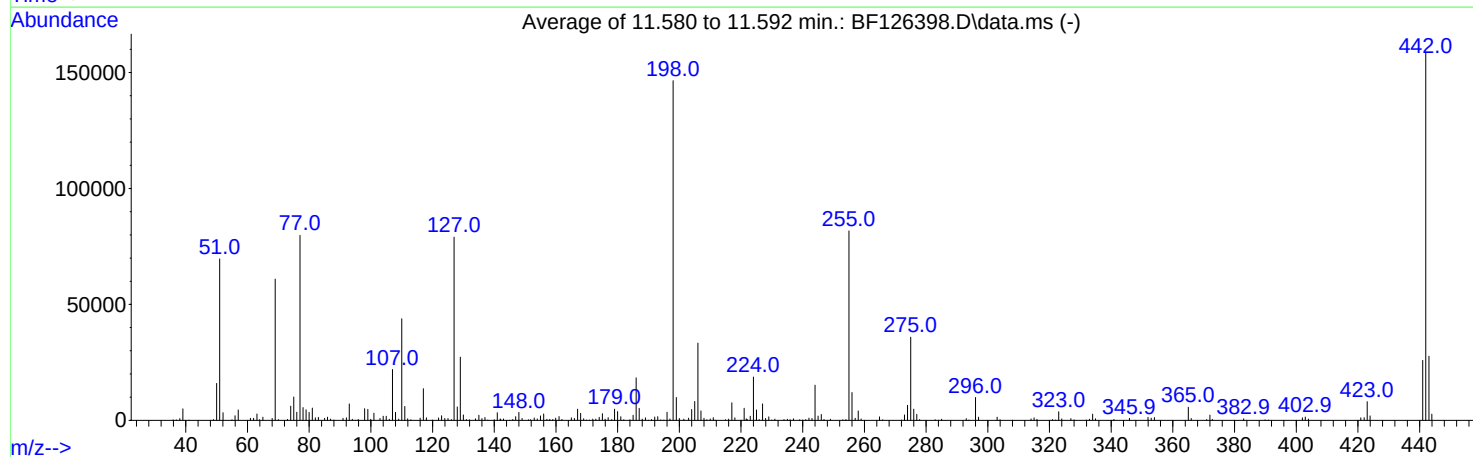


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122921\
 Data File : BF126398.D
 Acq On : 29 Dec 2021 16:45
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 30 04:30:49 2021

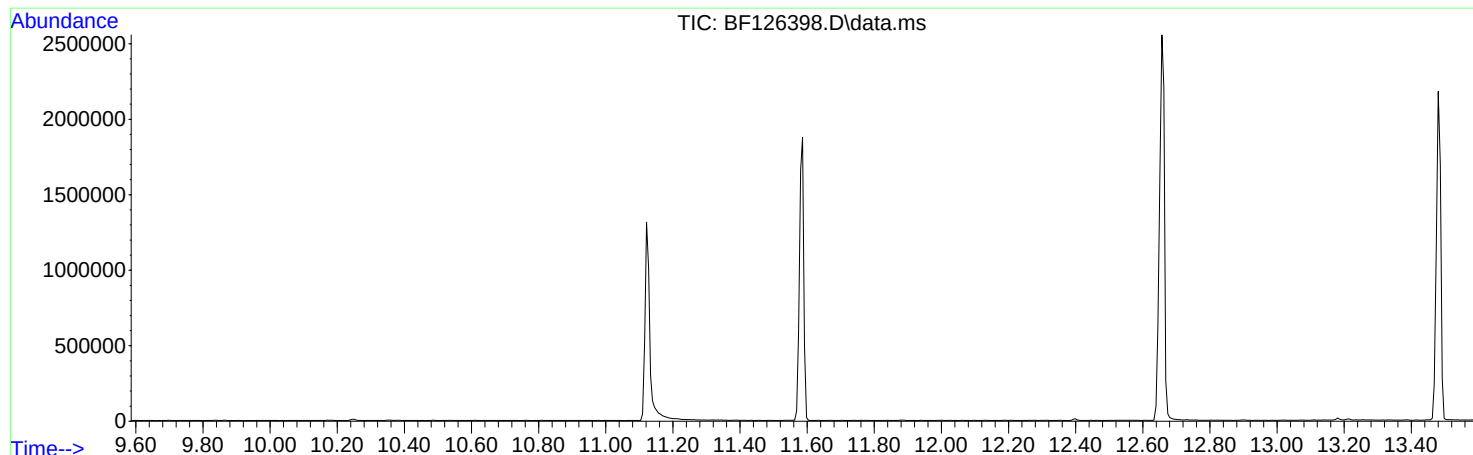




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.5	69611	PASS
68	69	0.00	2	1.4	863	PASS
69	198	0.00	100	41.6	60909	PASS
70	69	0.00	2	0.5	320	PASS
127	198	10	80	53.9	79011	PASS
197	198	0.00	2	0.4	640	PASS
198	198	100	100	100.0	146509	PASS
199	198	5	9	6.7	9877	PASS
275	198	10	60	24.5	35867	PASS
365	198	1	100	3.9	5662	PASS
441	198	0.01	100	17.7	25909	PASS
442	442	50	100	100.0	158651	PASS
443	442	15	24	17.5	27699	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122921\
 Data File : BF126398.D
 Acq On : 29 Dec 2021 16:45
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 30 05:25:56 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 30 04:30:49 2021
 Response via : Initial Calibration

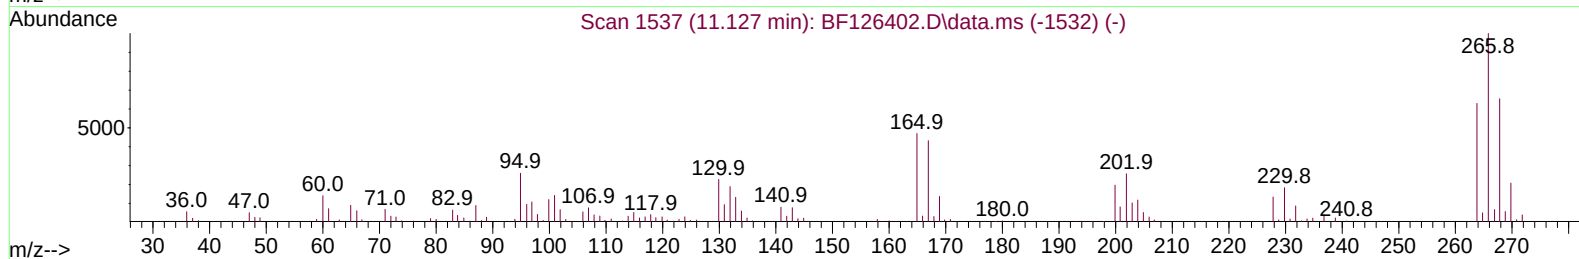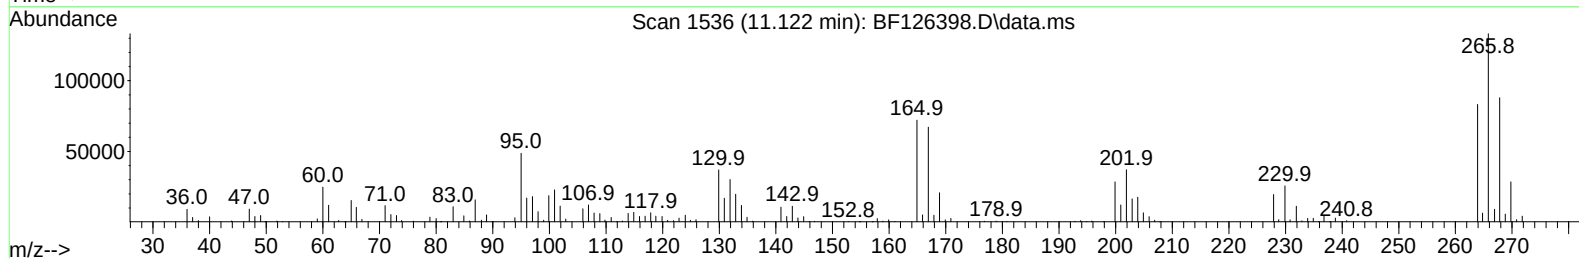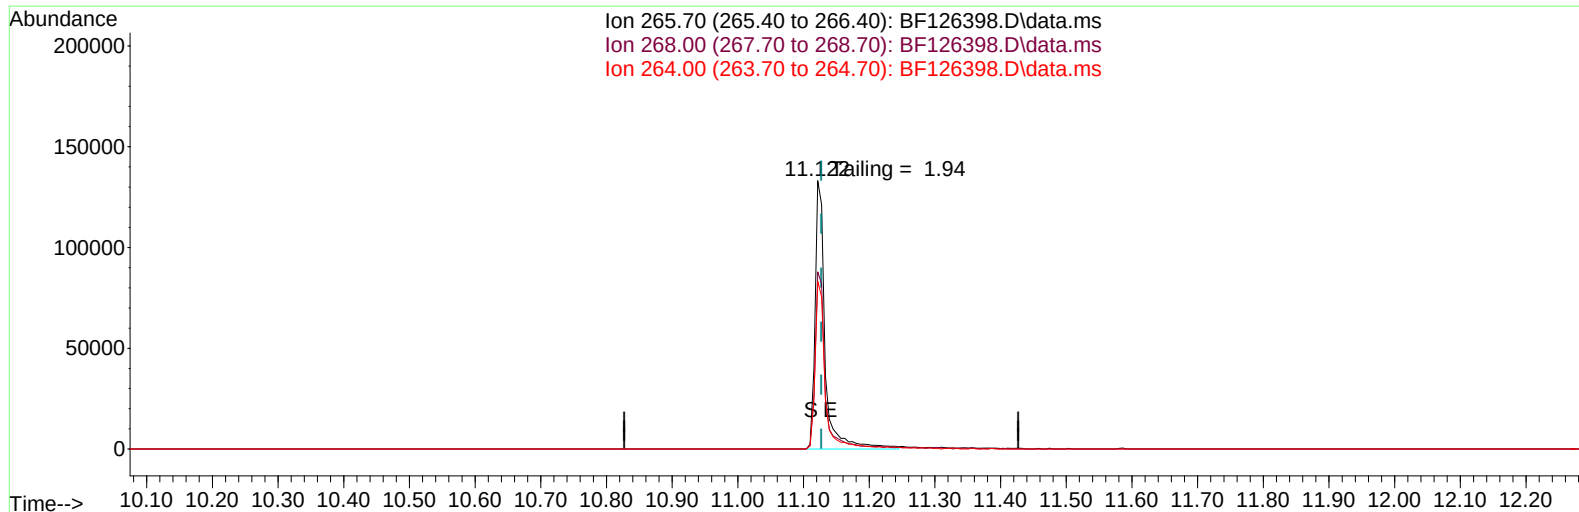

TIC: BF126398.D\data.ms

(70) Pentachlorophenol (C)

11.122min (-0.005) 56532.35 ng




response 144961

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	66.03
264.00	63.00	62.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122921\
Data File : BF126398.D
Acq On : 29 Dec 2021 16:45
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 30 05:25:56 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 30 04:30:49 2021
Response via : Initial Calibration

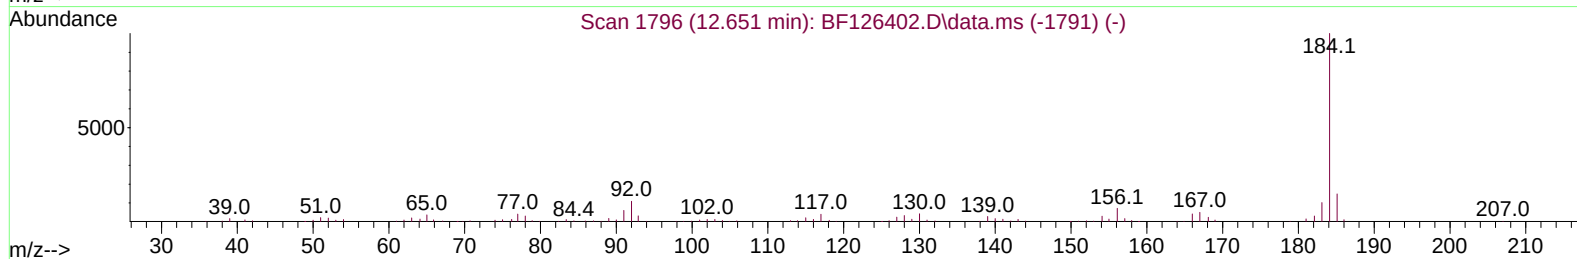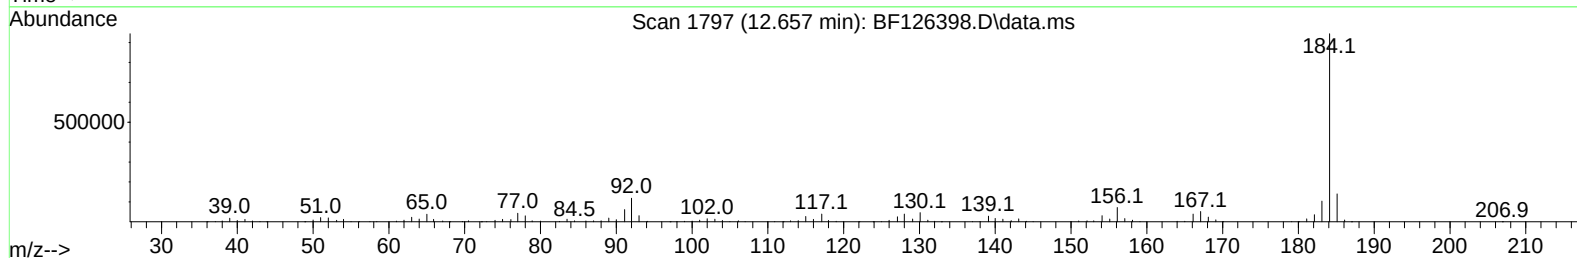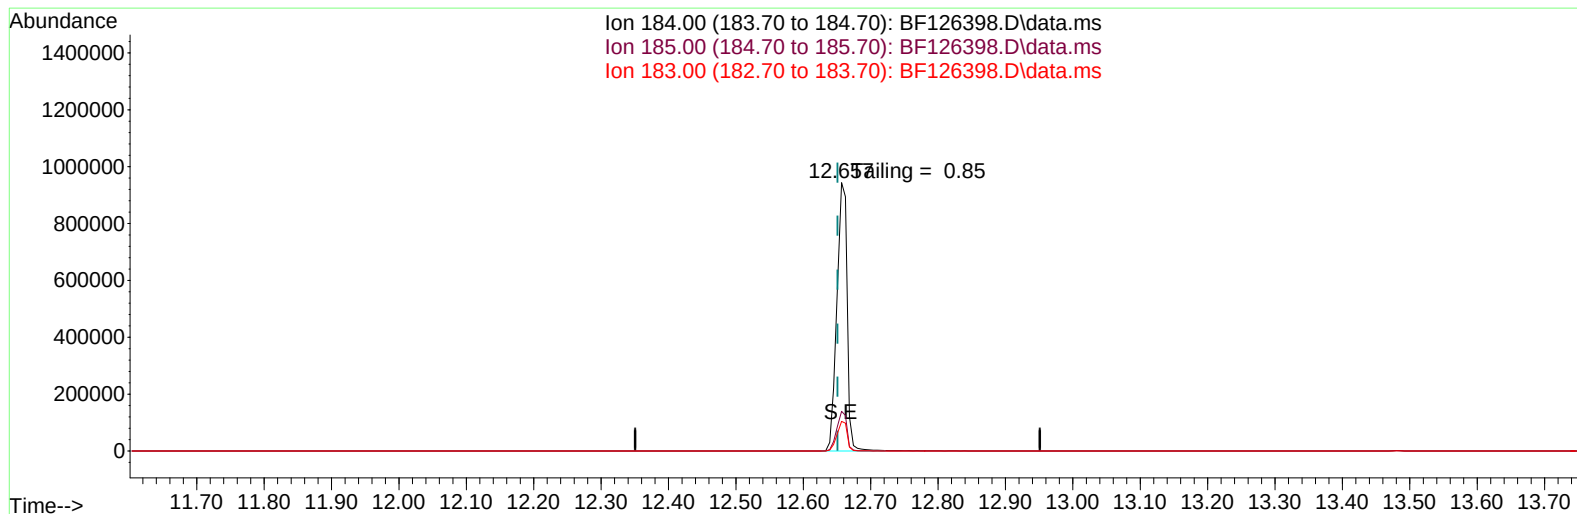

TIC: BF126398.D\data.ms

(77) Benzidine

12.657min (+ 0.006) 86378.08 ng

response 1010082

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.81
183.00	10.20	11.02
0.00	0.00	0.00

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/29/2021	BNA_F	<u>BF126398.D</u>
Compound Name	Response	Retention Time
DDT	367044	13.48
DDD	4758	13.18
DDE	0	12.863
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4758	371802	1.28