


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF123019\
 Data File : BF118380.D
 Acq On : 30 Dec 2019 14:31
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF122419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 24 15:58:52 2019

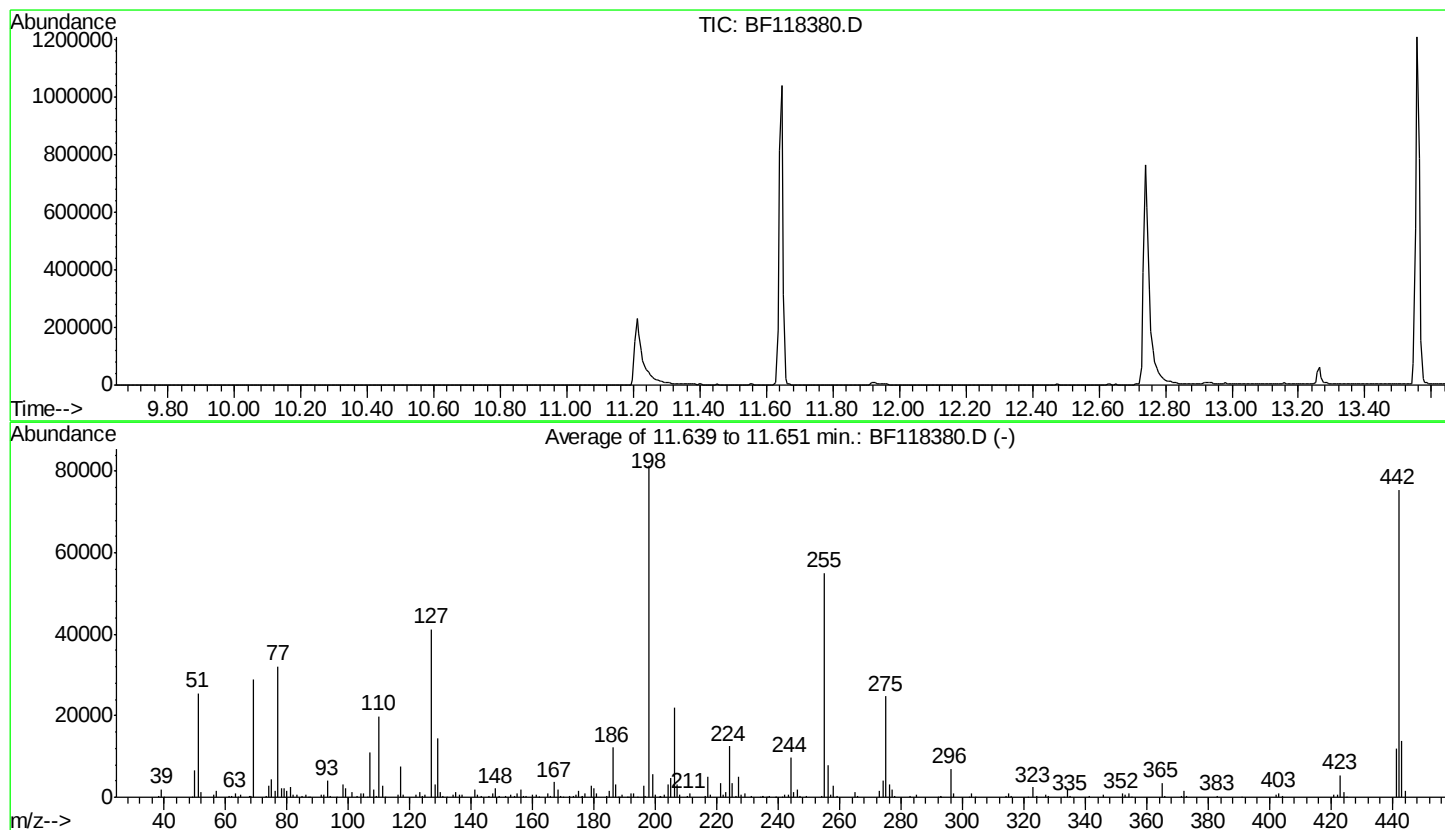

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.3	25483	PASS
68	69	0.00	2	1.0	300	PASS
69	198	0.00	100	35.7	29030	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.7	41314	PASS
197	198	0.00	2	0.3	248	PASS
198	198	100	100	100.0	81413	PASS
199	198	5	9	7.1	5793	PASS
275	198	10	60	30.4	24770	PASS
365	198	1	100	4.3	3528	PASS
441	198	0.01	100	14.5	11840	PASS
442	198	50	100	92.8	75560	PASS
443	442	15	24	18.4	13922	PASS