
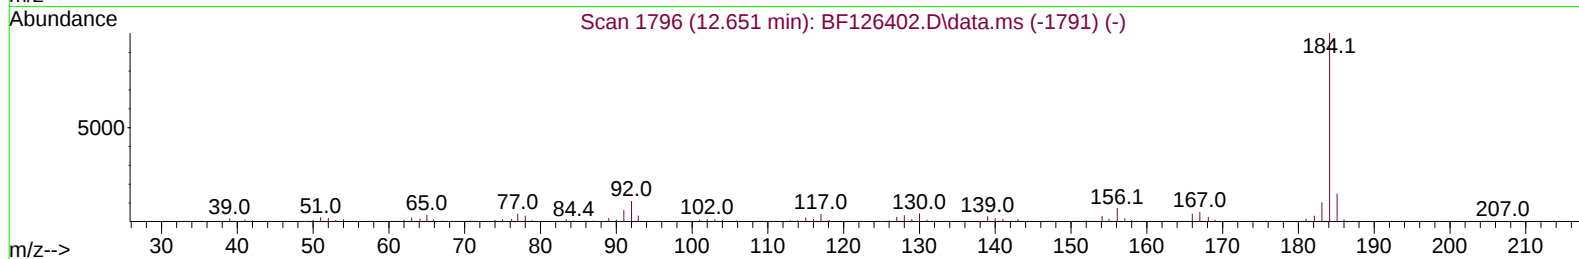
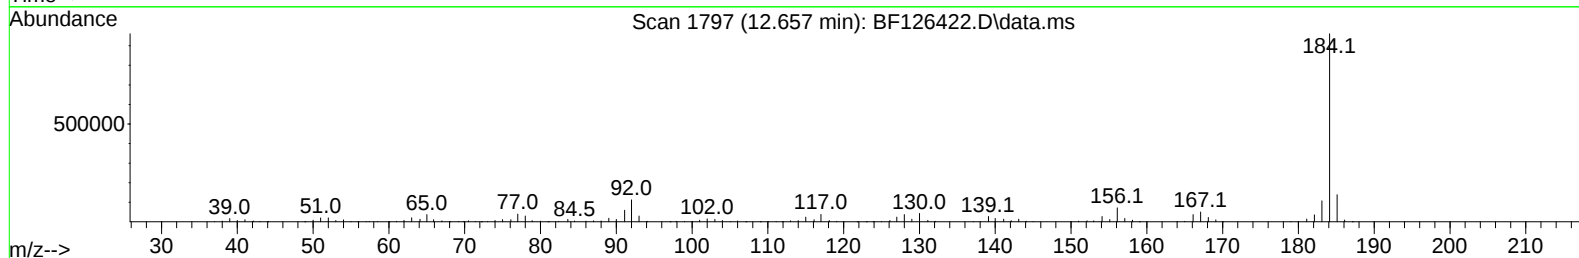


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123021\
Data File : BF126422.D
Acq On : 30 Dec 2021 16:35
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 31 01:17:42 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 30 04:30:49 2021
Response via : Initial Calibration

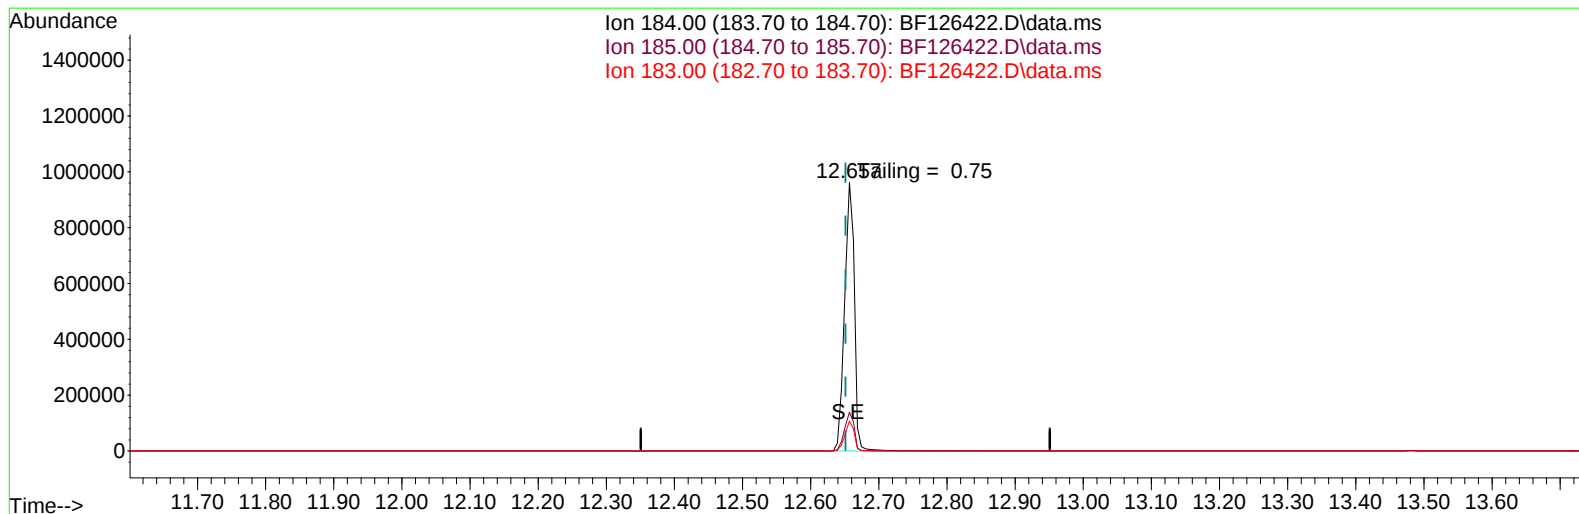

TIC: BF126422.D\data.ms

(77) Benzidine




12.657min (+ 0.006) 0.00 ng

response 956712

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.42
183.00	10.20	11.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123021\
 Data File : BF126422.D
 Acq On : 30 Dec 2021 16:35
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 31 01:17:42 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 30 04:30:49 2021
 Response via : Initial Calibration

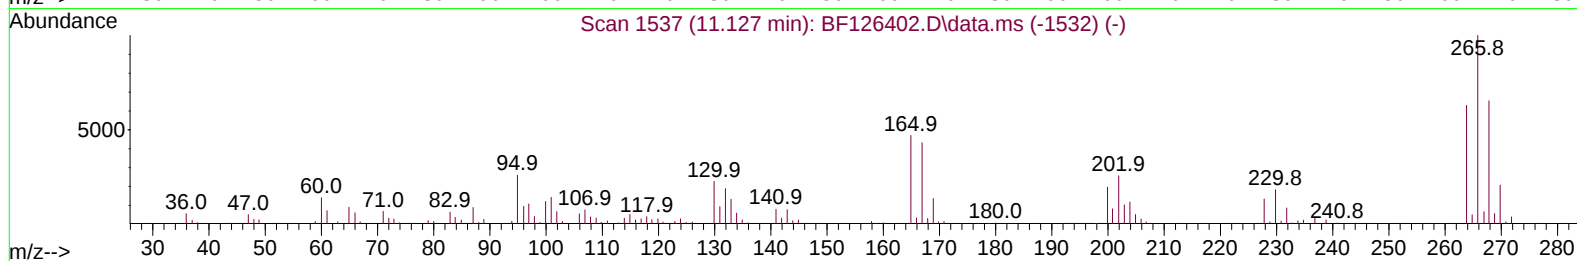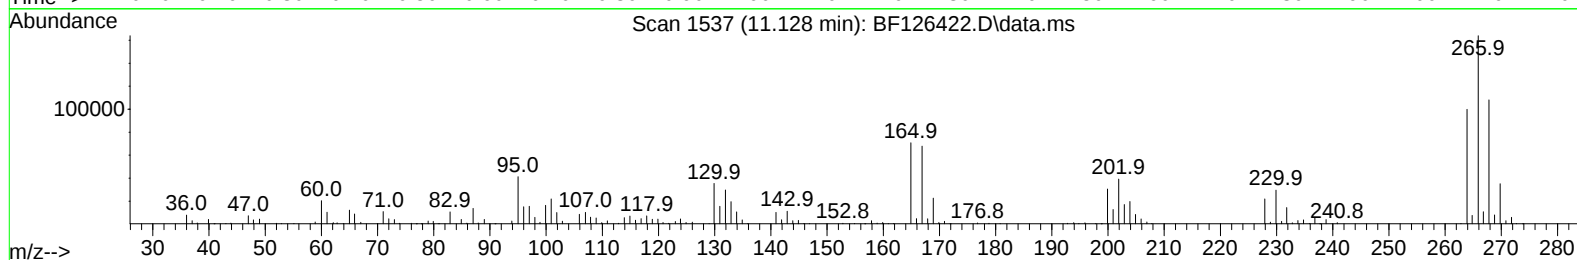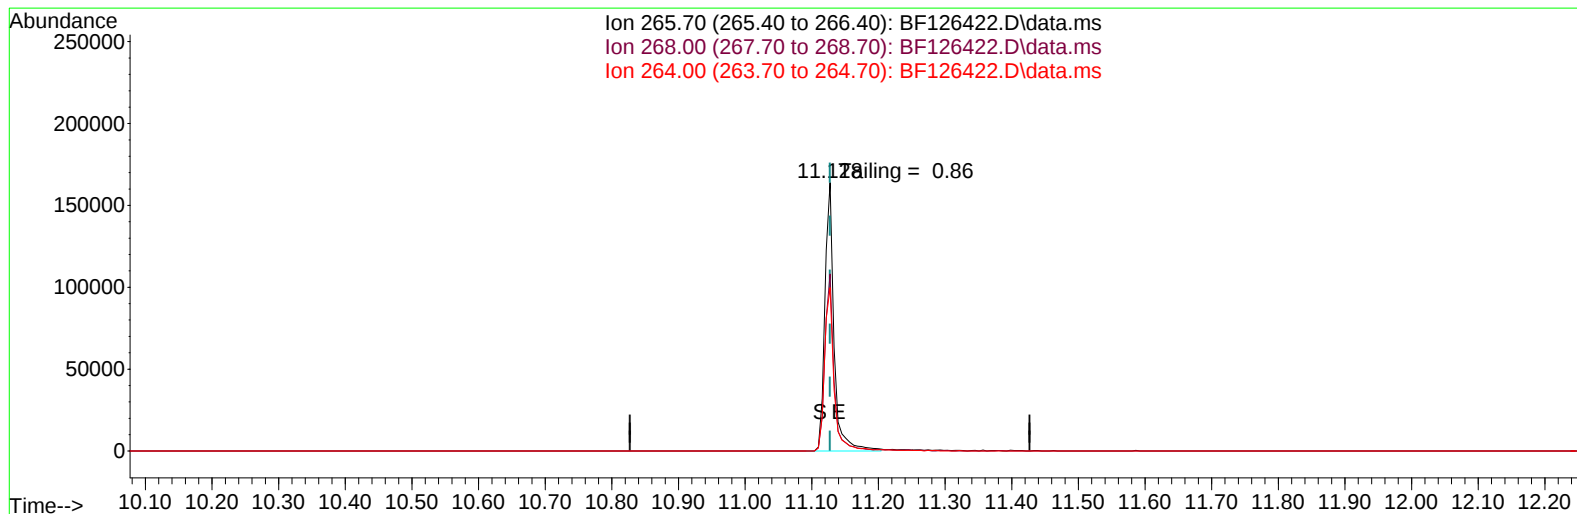

TIC: BF126422.D\data.ms

(70) Pentachlorophenol (C)

11.128min (+ 0.001) 63379.07 ng

response 158701

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	65.97
264.00	63.00	60.88
0.00	0.00	0.00