

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123021\
 Data File : BF126410.D
 Acq On : 30 Dec 2021 9:53
 Operator : JU/CG
 Sample : PB141738BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB141738BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126410.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.216	18	22	27	rVB	50449	61443	1.35%	0.213%
2	5.028	496	500	508	rBV	45673	64648	1.42%	0.224%
3	5.416	561	566	569	rBV	4035025	4553933	100.00%	15.814%
4	6.428	732	738	741	rBV	3859806	4522367	99.31%	15.704%
5	6.792	797	800	804	rBV	1095369	966116	21.21%	3.355%
6	7.357	890	896	899	rBV	2891859	3191050	70.07%	11.081%
7	8.075	1014	1018	1022	rBV	1279694	1326053	29.12%	4.605%
8	9.157	1196	1202	1205	rBV	4022541	4221749	92.71%	14.660%
9	9.833	1312	1317	1320	rBV	1476269	1307391	28.71%	4.540%
10	10.621	1446	1451	1454	rBV	2394041	2258679	49.60%	7.843%
11	11.316	1565	1569	1576	rVB	1392059	1213938	26.66%	4.216%
12	12.910	1835	1840	1843	rBV	3333959	3428935	75.30%	11.907%
13	13.951	2013	2017	2021	rBV	923008	842043	18.49%	2.924%
14	15.392	2257	2262	2267	rBV	603030	741337	16.28%	2.574%
15	15.862	2337	2342	2349	rVB	29954	47018	1.03%	0.163%
16	16.351	2420	2425	2433	rBV2	26925	50223	1.10%	0.174%




Sum of corrected areas: 28796923

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123021\
Data File : BF126410.D
Acq On : 30 Dec 2021 9:53
Operator : JU/CG
Sample : PB141738BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB141738BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

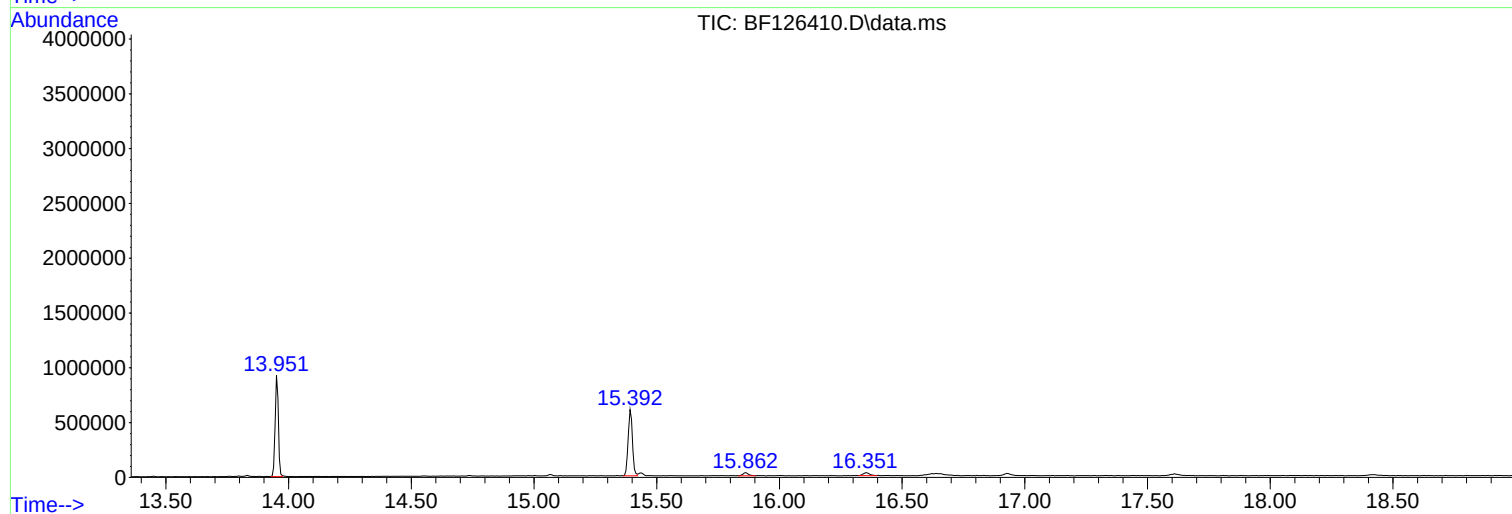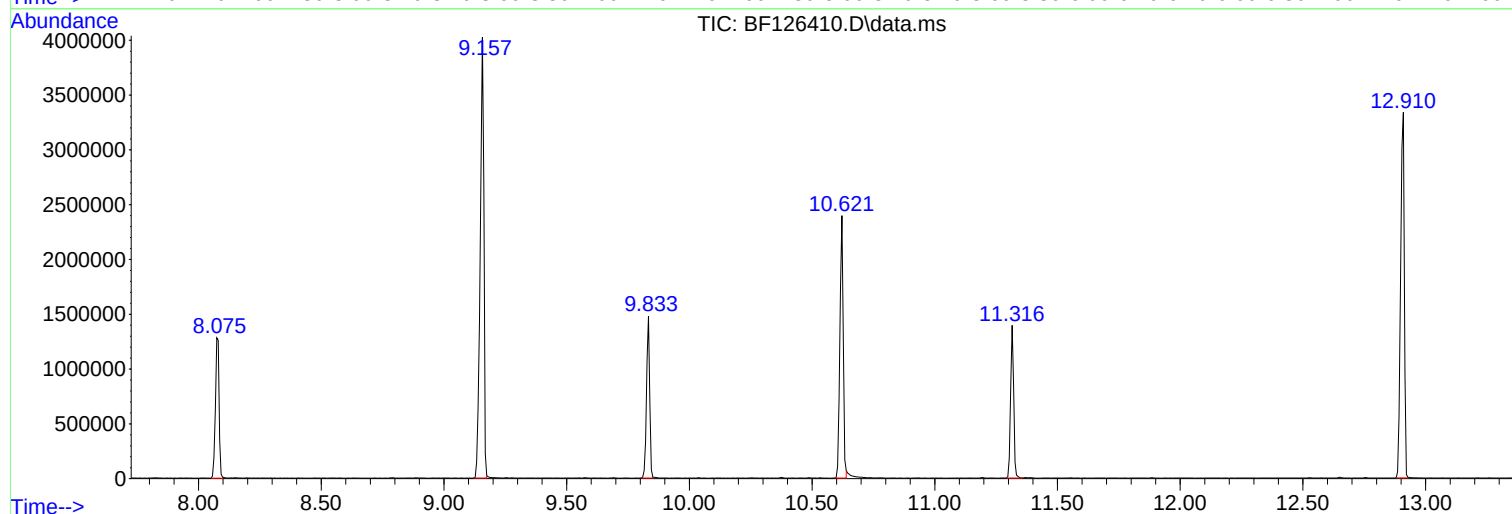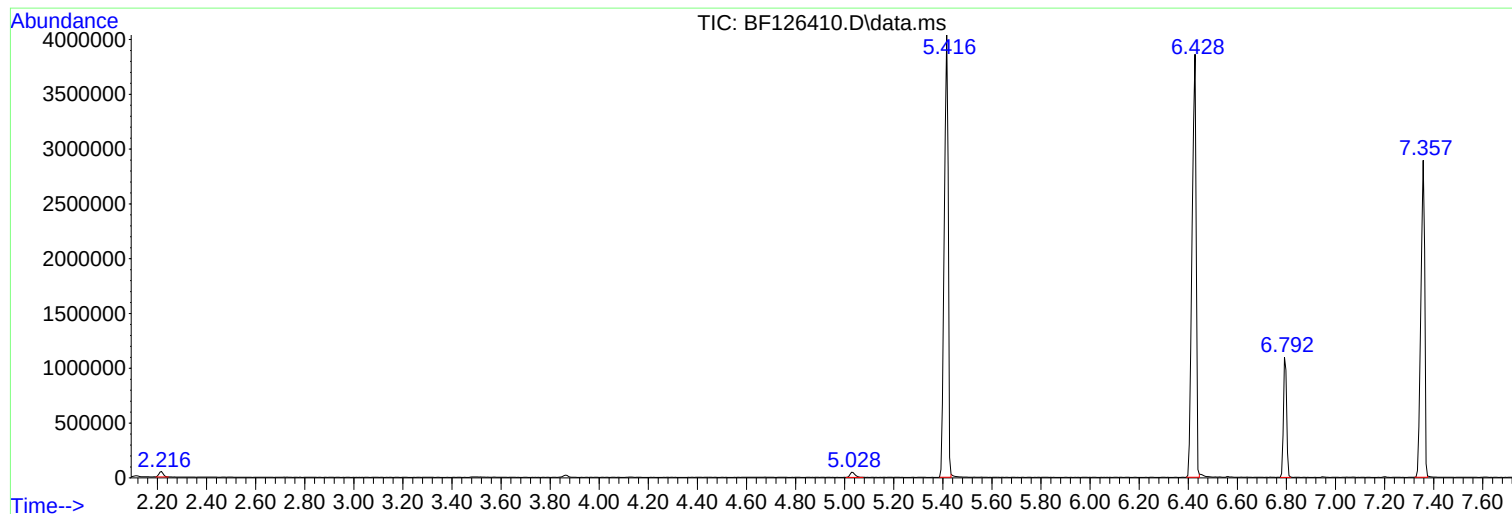

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123021\
Data File : BF126410.D
Acq On : 30 Dec 2021 9:53
Operator : JU/CG
Sample : PB141738BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB141738BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123021\
Data File : BF126410.D
Acq On : 30 Dec 2021 9:53
Operator : JU/CG
Sample : PB141738BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB141738BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------