

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123021\
 Data File : BF126417.D
 Acq On : 30 Dec 2021 13:43
 Operator : JU/CG
 Sample : M5238-01 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OK-02-122321

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126417.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.816	289	294	299	rVB	18297	25633	1.92%	0.267%
2	5.398	559	563	573	rVB	811503	688510	51.48%	7.183%
3	6.416	733	736	746	rVB	831692	680050	50.84%	7.095%
4	6.798	797	801	804	rBV	1263285	1032244	77.17%	10.769%
5	7.351	892	895	899	rBV	480095	411889	30.79%	4.297%
6	8.080	1015	1019	1022	rBV	1687503	1337557	100.00%	13.954%
7	8.680	1116	1121	1124	rBV2	19268	17527	1.31%	0.183%
8	9.157	1198	1202	1208	rBV	774962	657079	49.13%	6.855%
9	9.245	1213	1217	1221	rVV	35662	33766	2.52%	0.352%
10	9.774	1304	1307	1311	rVB	37661	33896	2.53%	0.354%
11	9.833	1311	1317	1321	rBV	1443555	1221627	91.33%	12.745%
12	10.251	1384	1388	1389	rBV2	27597	23934	1.79%	0.250%
13	10.269	1389	1391	1395	rVB	38565	32179	2.41%	0.336%
14	10.433	1416	1419	1424	rBV7	8172	16110	1.20%	0.168%
15	10.492	1424	1429	1432	rVV	28044	35281	2.64%	0.368%
16	10.616	1447	1450	1456	rBV	314676	278027	20.79%	2.901%
17	10.745	1469	1472	1473	rBV	49420	44673	3.34%	0.466%
18	11.192	1545	1548	1550	rBV2	37506	29050	2.17%	0.303%
19	11.221	1550	1553	1559	rVB2	37076	44735	3.34%	0.467%
20	11.316	1566	1569	1572	rBV	1084909	985996	73.72%	10.286%
21	11.339	1572	1573	1577	rVV	94209	64653	4.83%	0.674%
22	11.392	1580	1582	1586	rVB	25324	21423	1.60%	0.223%
23	11.621	1618	1621	1624	rVB	27237	23654	1.77%	0.247%
24	11.851	1657	1660	1662	rBV2	26717	24551	1.84%	0.256%
25	12.527	1772	1775	1779	rBV	97641	89426	6.69%	0.933%
26	12.757	1812	1814	1817	rVB	104054	79375	5.93%	0.828%
27	12.904	1835	1839	1842	rBV	550604	492206	36.80%	5.135%
28	13.957	2014	2018	2021	rBV	814315	733979	54.87%	7.657%
29	15.398	2260	2263	2267	rVB2	397577	426344	31.87%	4.448%


Sum of corrected areas: 9585374

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123021\
Data File : BF126417.D
Acq On : 30 Dec 2021 13:43
Operator : JU/CG
Sample : M5238-01 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-02-122321

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

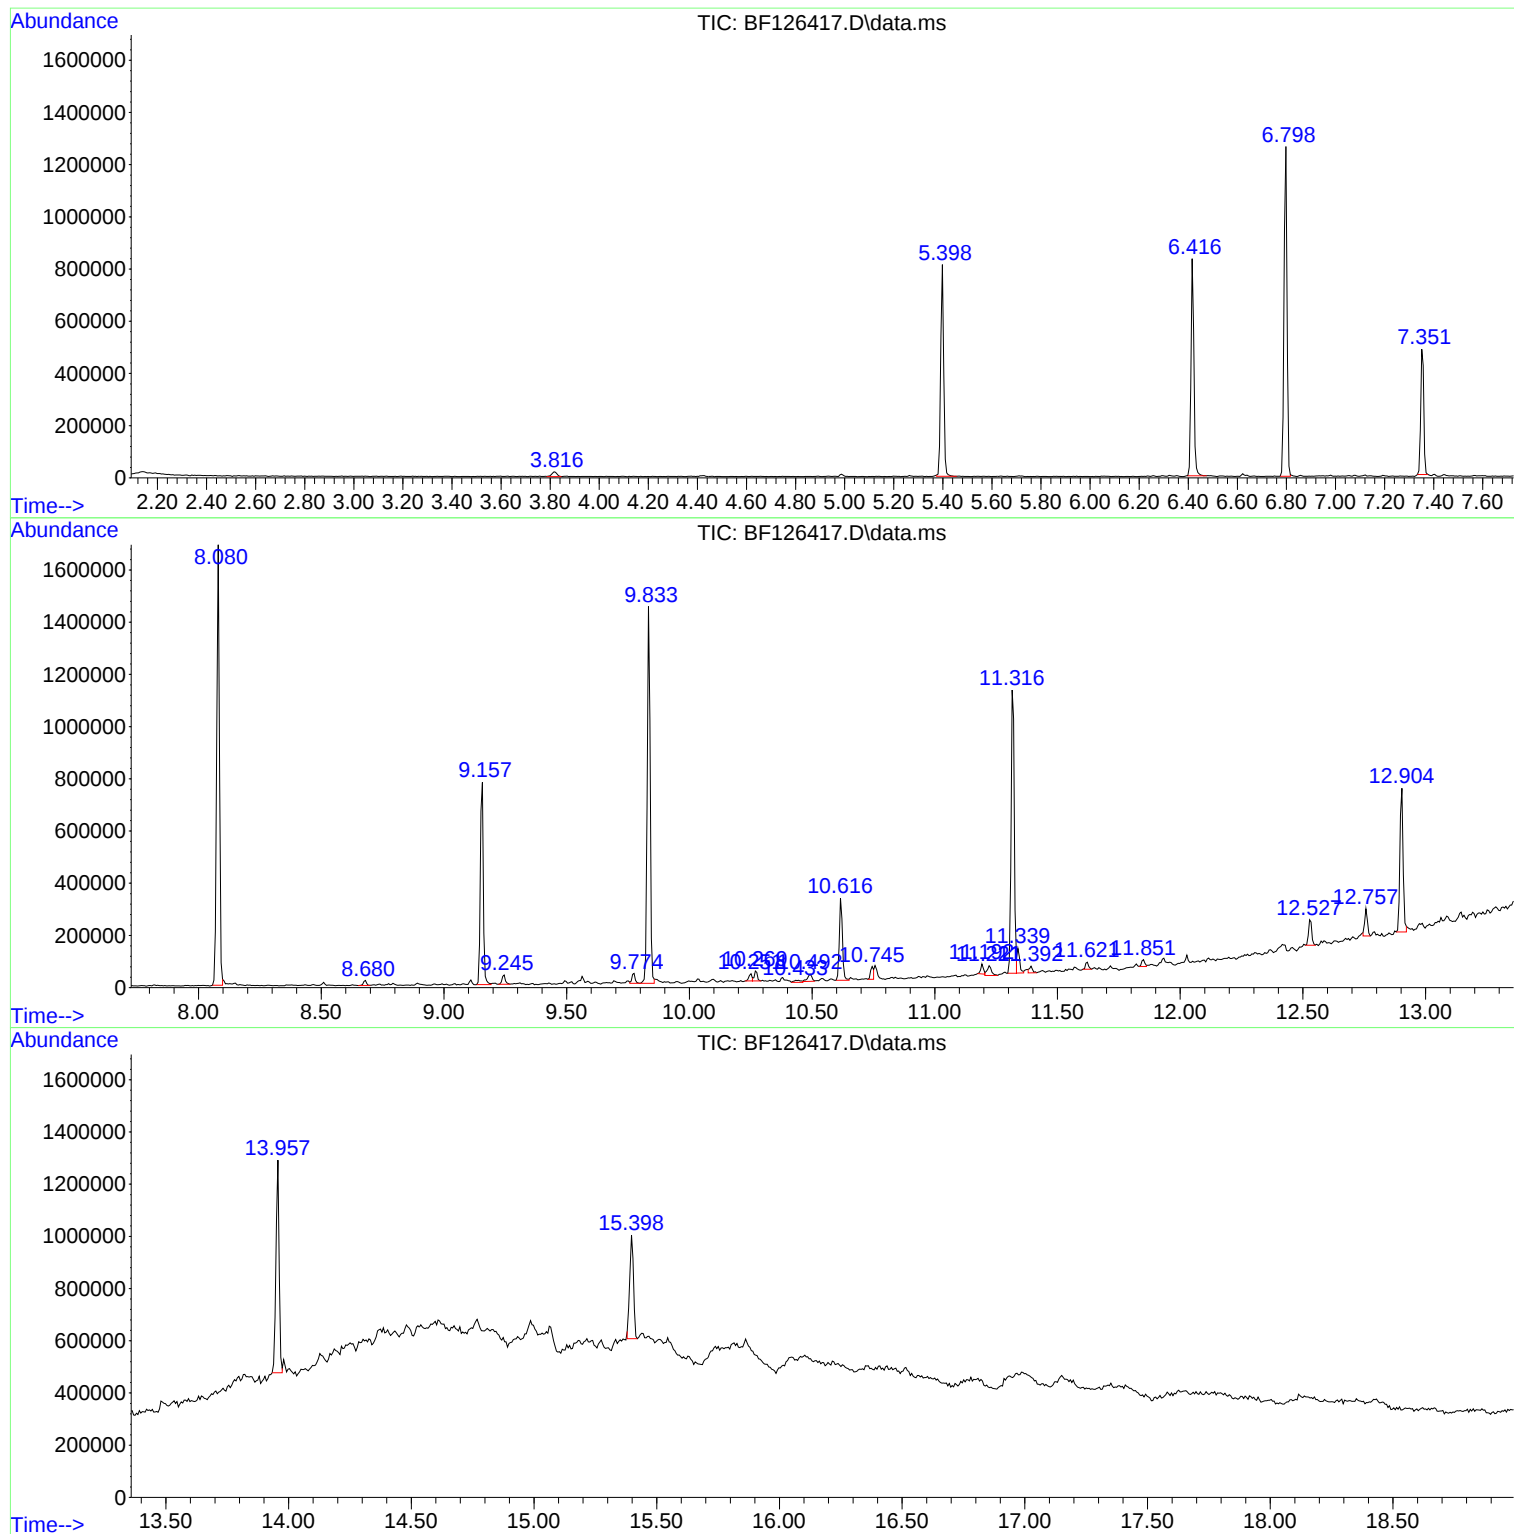

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123021\
Data File : BF126417.D
Acq On : 30 Dec 2021 13:43
Operator : JU/CG
Sample : M5238-01 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-02-122321

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123021\
Data File : BF126417.D
Acq On : 30 Dec 2021 13:43
Operator : JU/CG
Sample : M5238-01 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-02-122321

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------