


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123021\
 Data File : BF126408.D
 Acq On : 30 Dec 2021 8:48
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 30 04:30:49 2021

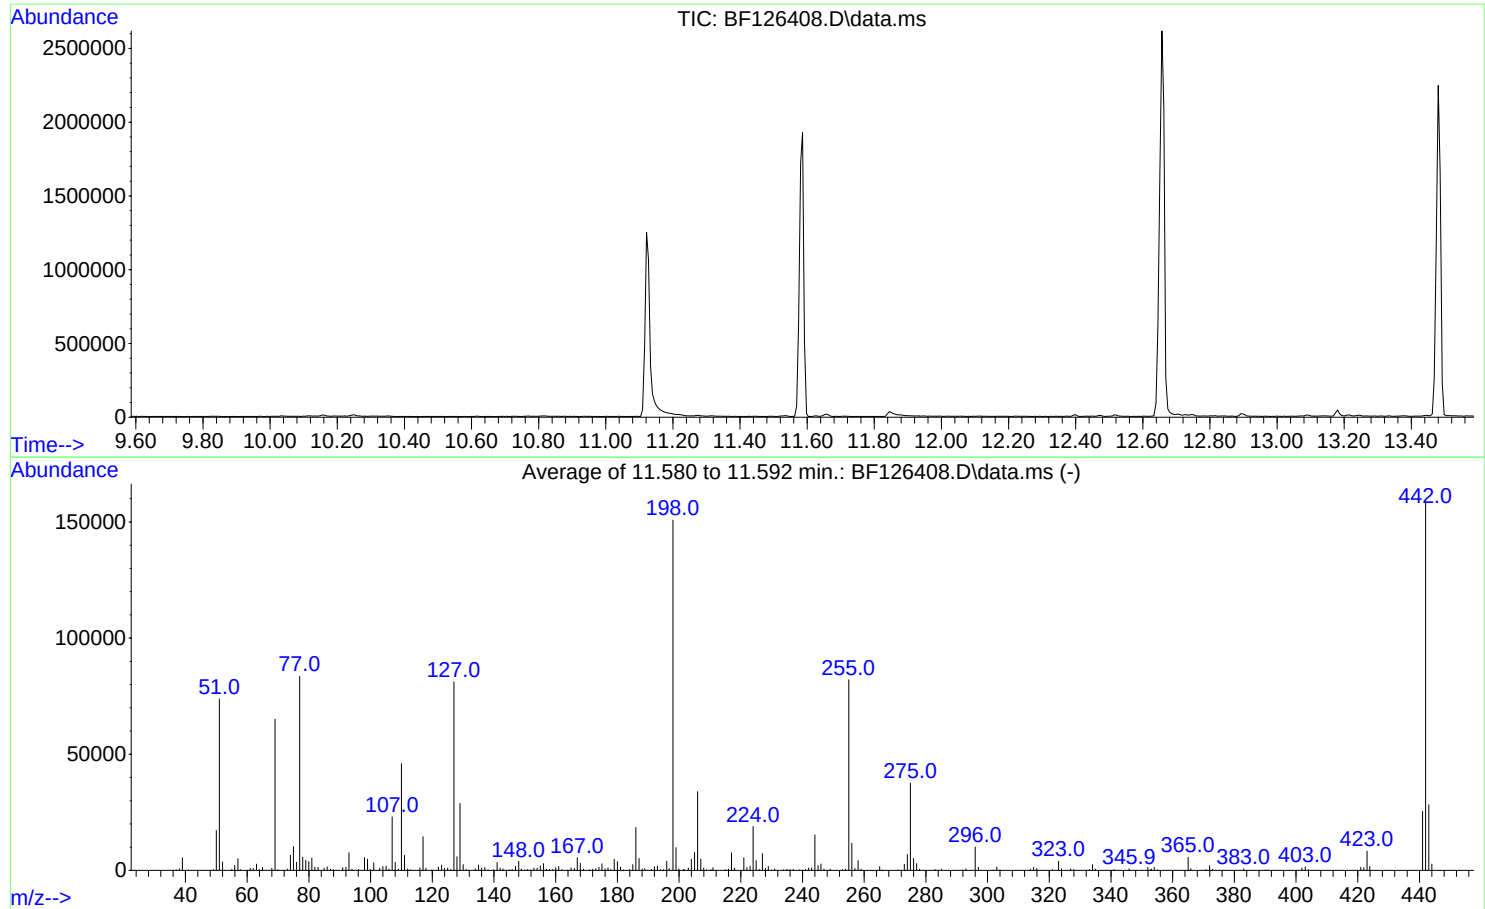




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.9	73785	PASS
68	69	0.00	2	1.4	911	PASS
69	198	0.00	100	43.1	65080	PASS
70	69	0.00	2	0.5	312	PASS
127	198	10	80	53.8	81165	PASS
197	198	0.00	2	0.5	793	PASS
198	198	100	100	100.0	150824	PASS
199	198	5	9	6.5	9791	PASS
275	198	10	60	24.9	37555	PASS
365	198	1	100	3.7	5622	PASS
441	198	0.01	100	16.8	25384	PASS
442	442	50	100	100.0	158384	PASS
443	442	15	24	17.8	28224	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123021\
Data File : BF126408.D
Acq On : 30 Dec 2021 8:48
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 31 07:11:20 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 30 04:30:49 2021
Response via : Initial Calibration

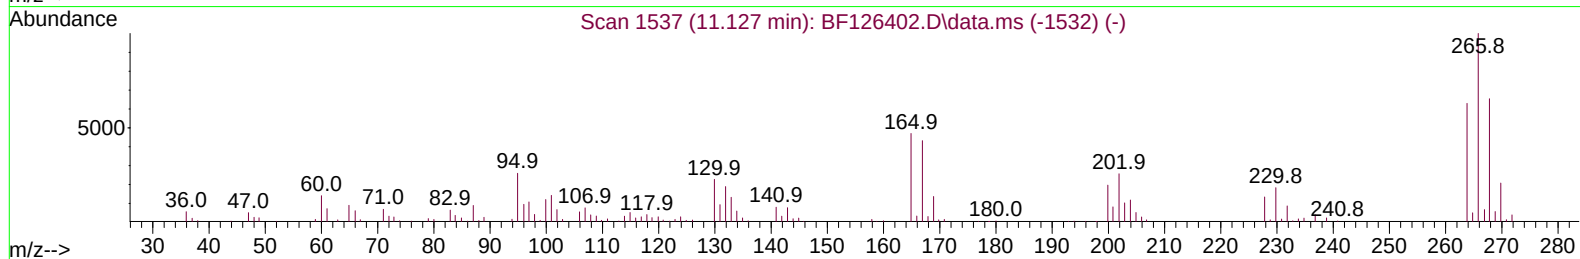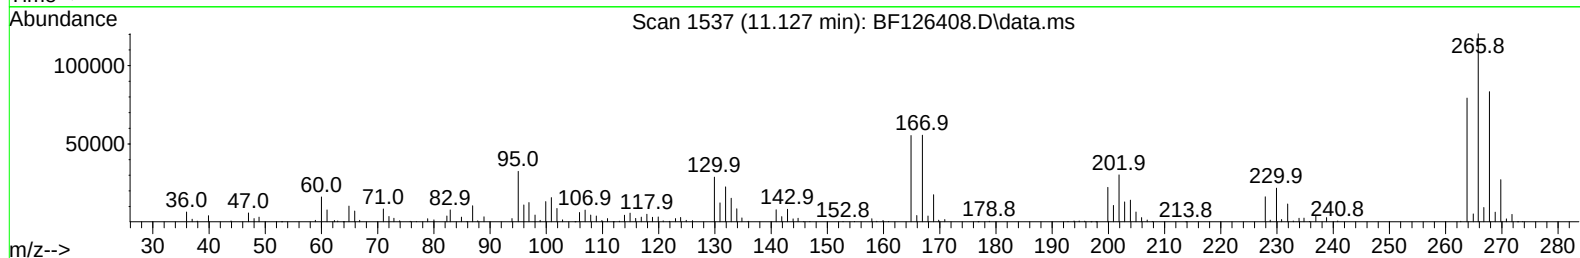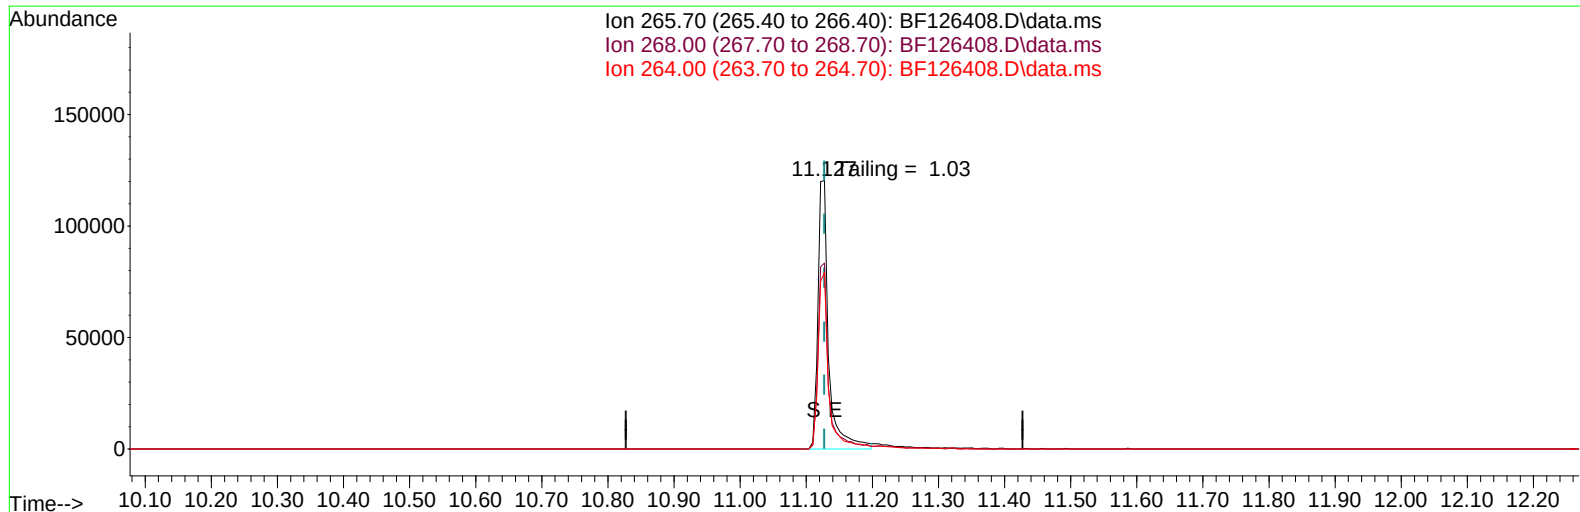

TIC: BF126408.D\data.ms

(70) Pentachlorophenol (C)

11.127min (+ 0.000) 23904.72 ng




response 142746

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	69.30
264.00	63.00	65.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123021\
Data File : BF126408.D
Acq On : 30 Dec 2021 8:48
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 31 07:11:20 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 30 04:30:49 2021
Response via : Initial Calibration

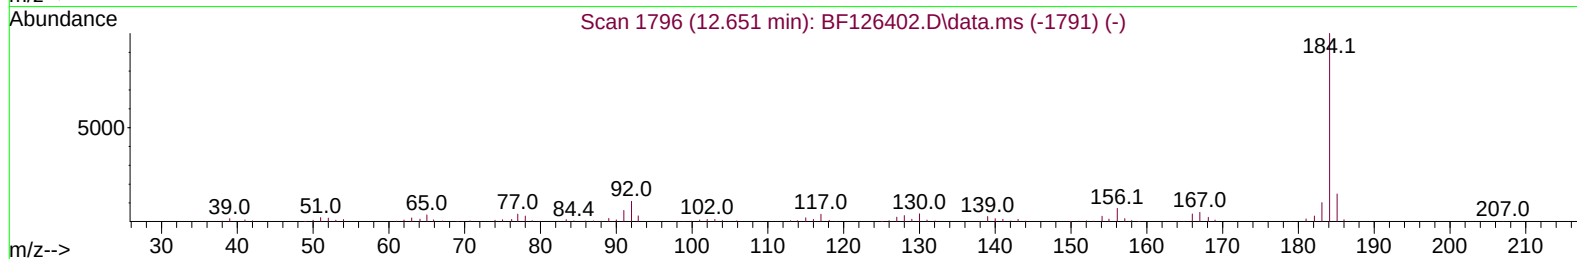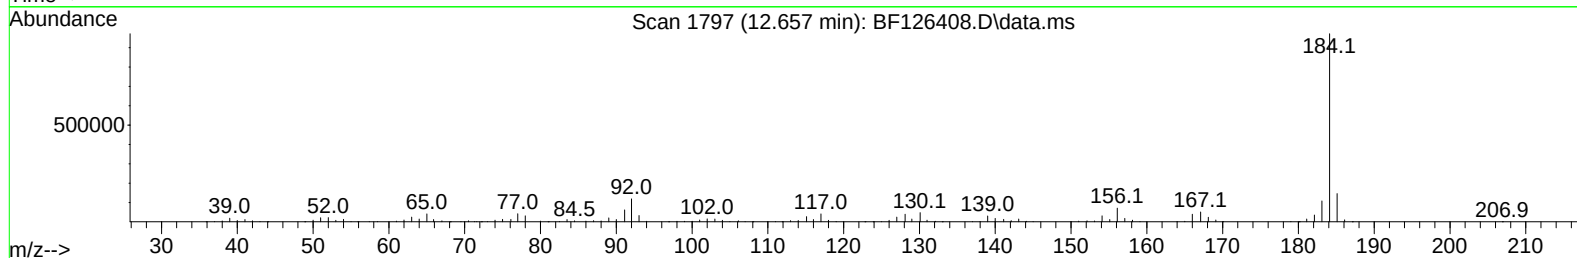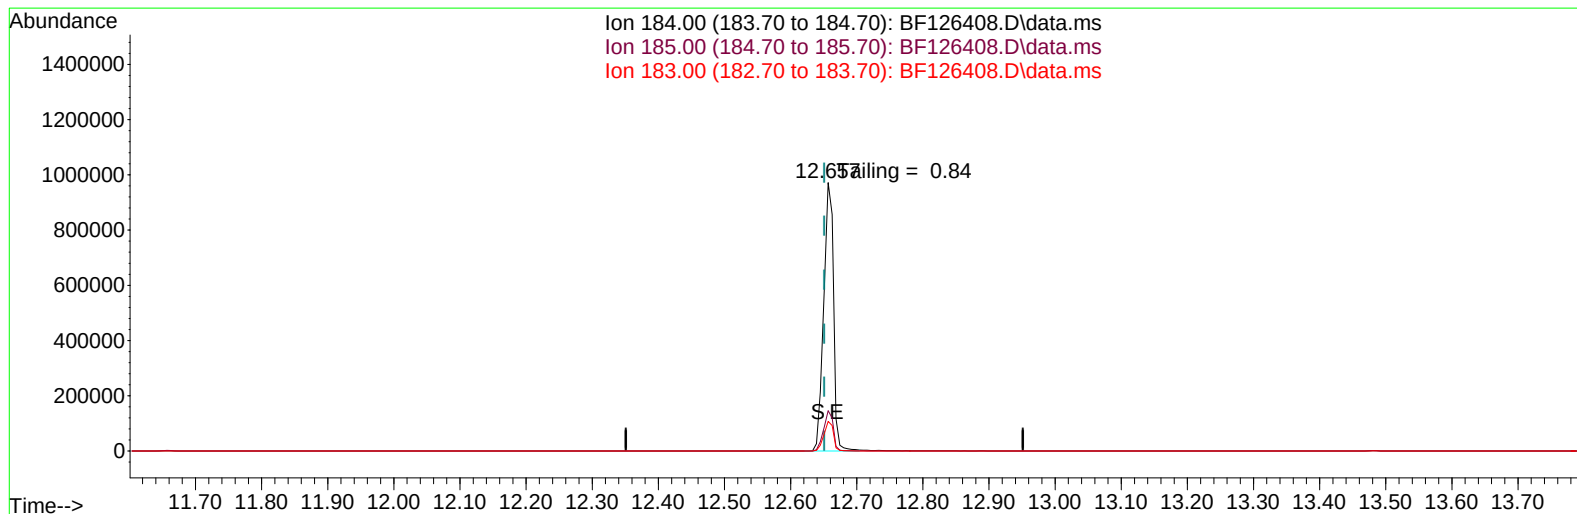

TIC: BF126408.D\data.ms

(77) Benzidine

12.657min (+ 0.006) 24408.78 ng

response 1007420

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	15.04
183.00	10.20	11.06
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/30/2021	BNA_F	BF126408.D
Compound Name	Response	Retention Time
DDT	364457	13.48
DDD	6305	13.18
DDE	426	12.84
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6731	371188	1.81