


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123021\
 Data File : BF126422.D
 Acq On : 30 Dec 2021 16:35
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 30 04:30:49 2021

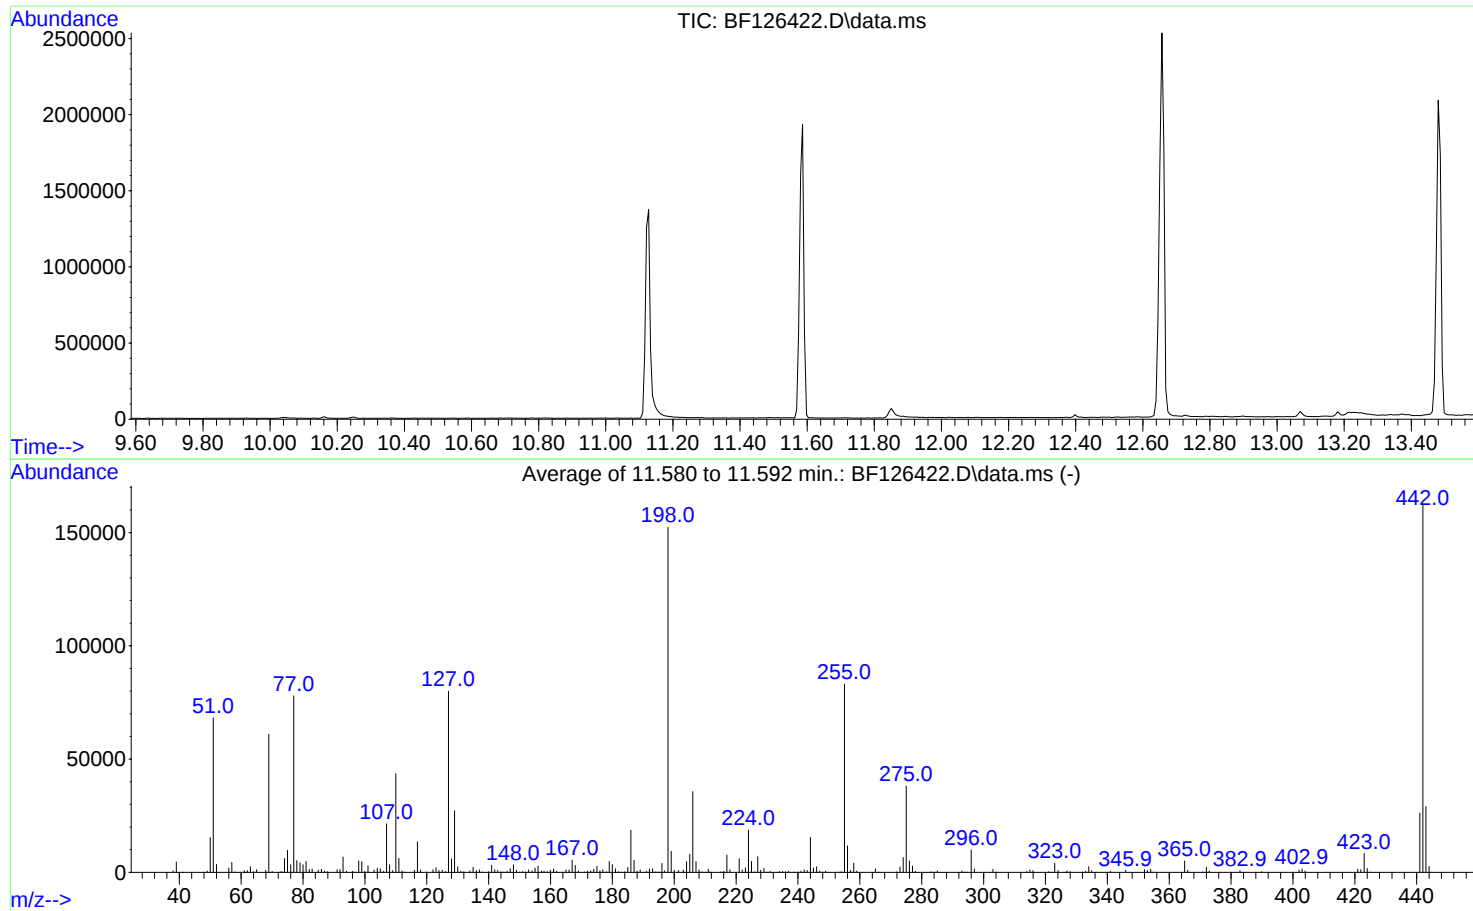




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.8	68234	PASS
68	69	0.00	2	1.6	950	PASS
69	198	0.00	100	40.0	60962	PASS
70	69	0.00	2	0.7	429	PASS
127	198	10	80	52.5	79944	PASS
197	198	0.00	2	0.4	662	PASS
198	198	100	100	100.0	152381	PASS
199	198	5	9	6.1	9359	PASS
275	198	10	60	25.0	38131	PASS
365	198	1	100	3.3	5000	PASS
441	198	0.01	100	17.2	26211	PASS
442	442	50	100	100.0	162400	PASS
443	442	15	24	17.9	29059	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123021\
Data File : BF126422.D
Acq On : 30 Dec 2021 16:35
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 31 01:17:42 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 30 04:30:49 2021
Response via : Initial Calibration

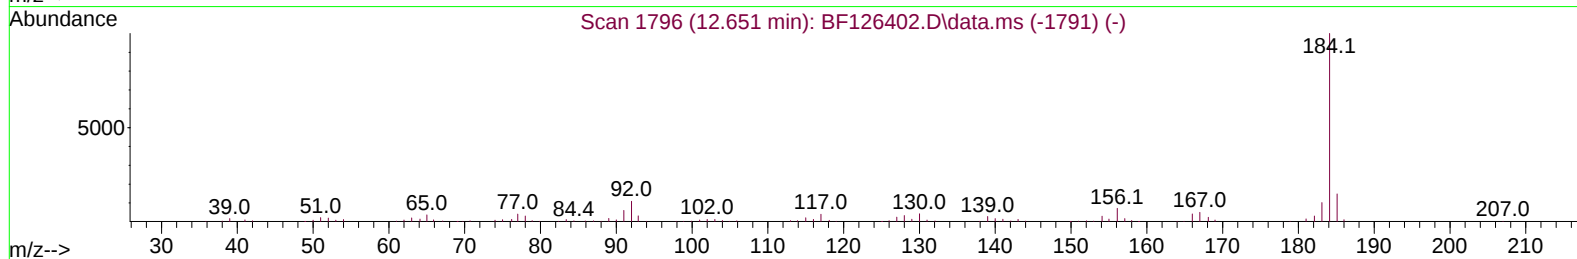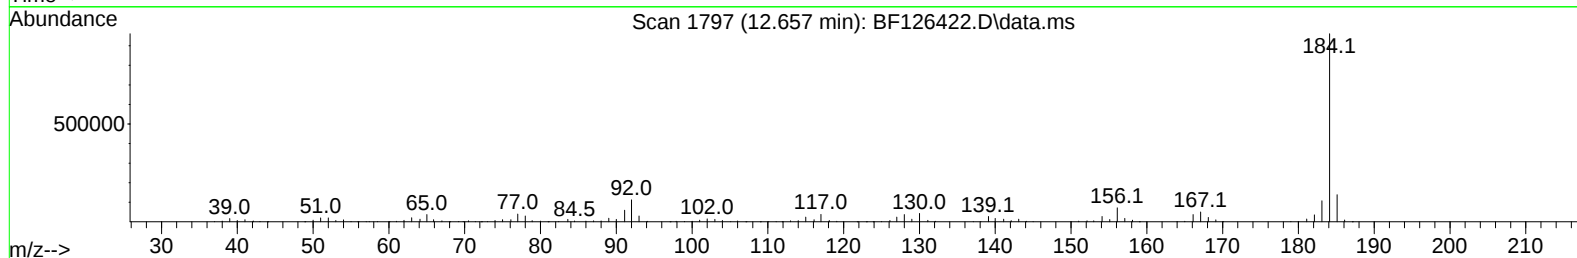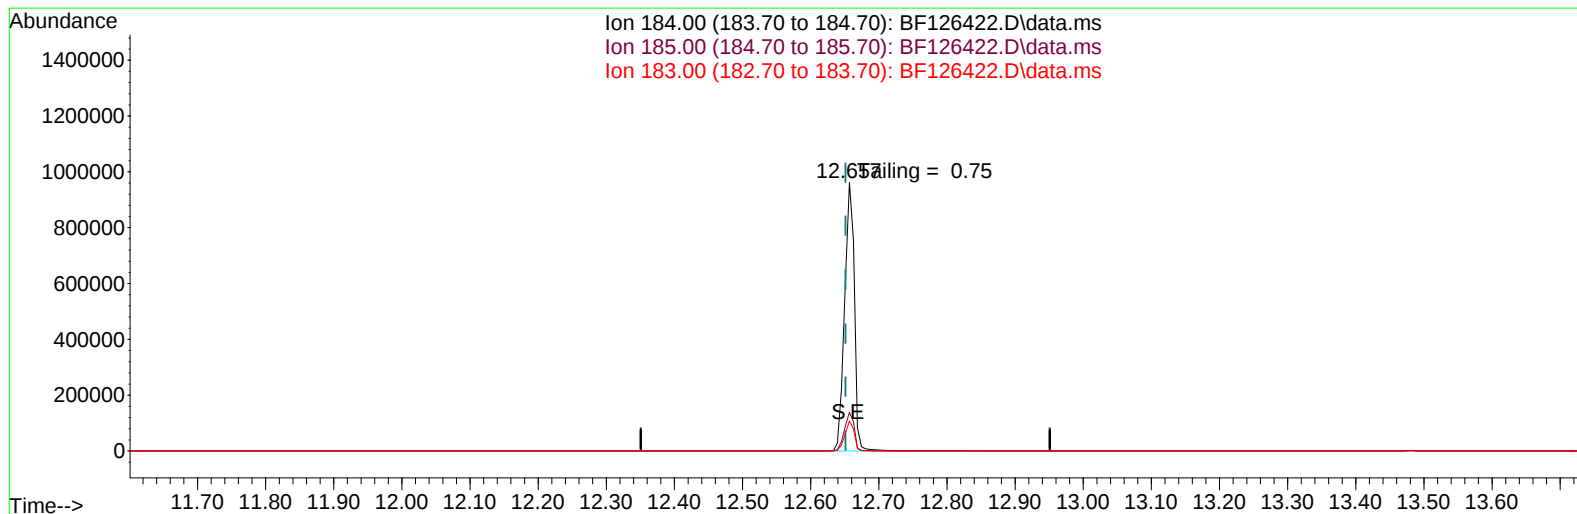

TIC: BF126422.D\data.ms

(77) Benzidine

12.657min (+ 0.006) 0.00 ng




response 956712

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.42
183.00	10.20	11.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123021\
 Data File : BF126422.D
 Acq On : 30 Dec 2021 16:35
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 31 01:17:42 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 30 04:30:49 2021
 Response via : Initial Calibration

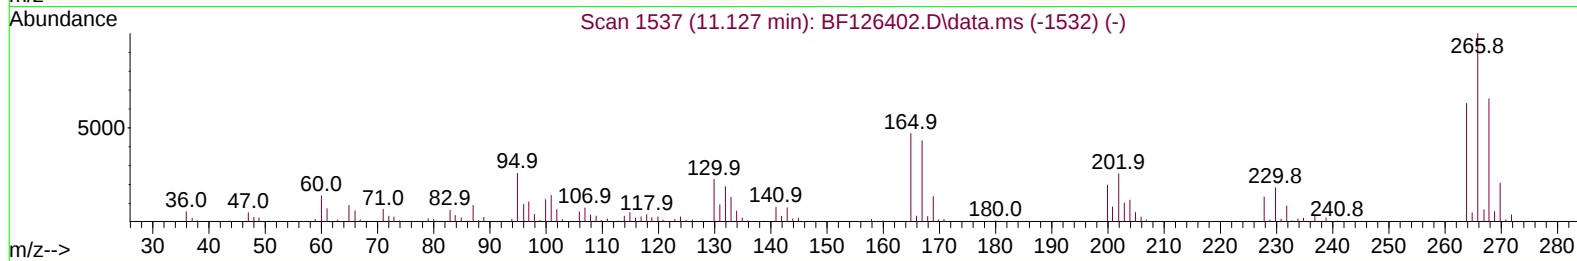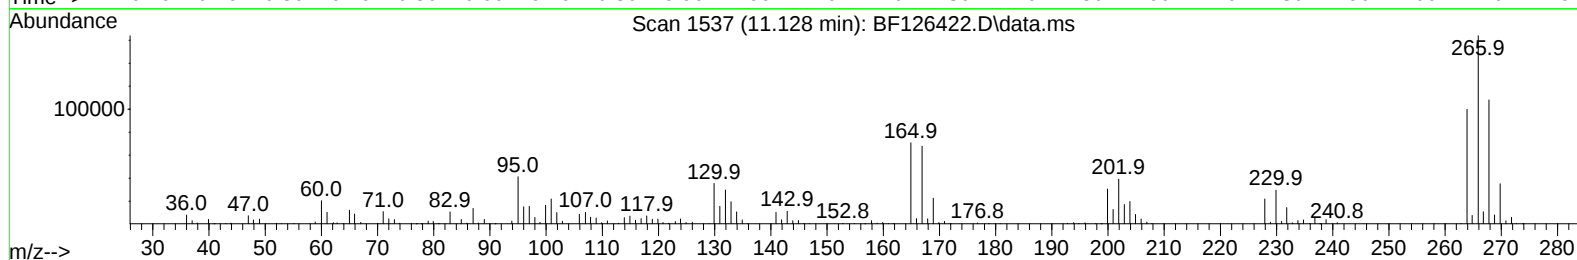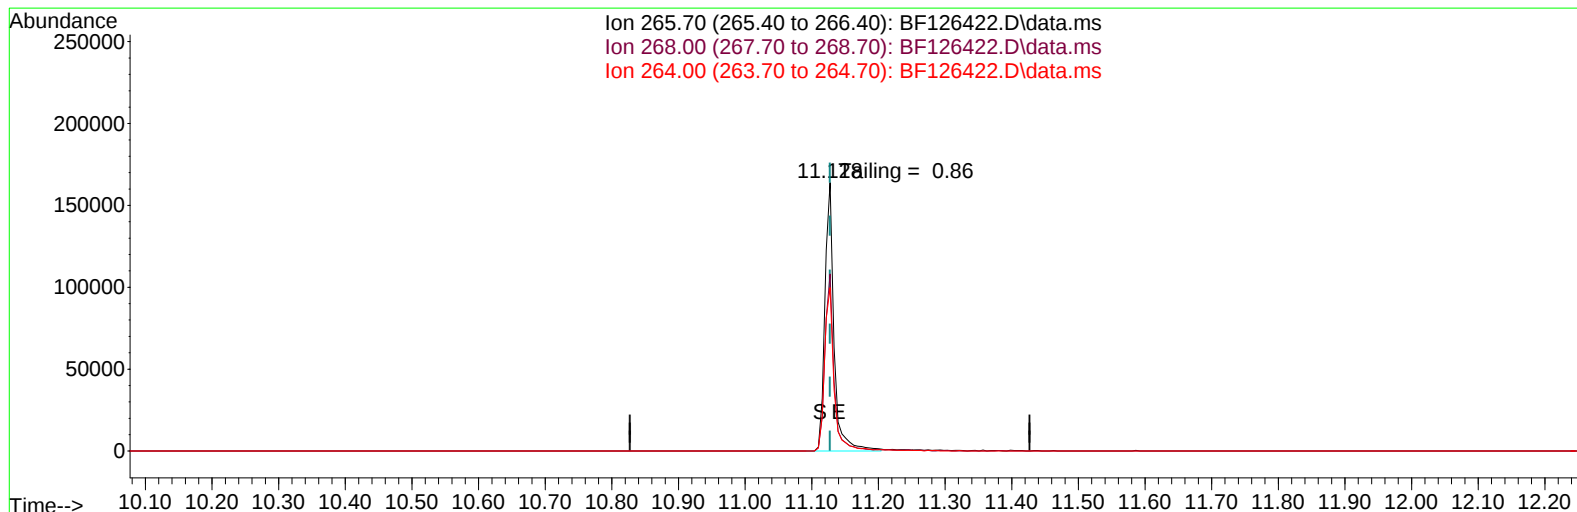

TIC: BF126422.D\data.ms

(70) Pentachlorophenol (C)

11.128min (+ 0.001) 63379.07 ng

response 158701

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	65.97
264.00	63.00	60.88
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/30/2021	BNA_F	<u>BF126422.D</u>
Compound Name	Response	Retention Time
DDT	360950	13.48
DDD	5039	13.18
DDE	334	12.84
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5373	366323	1.47

Instrument :
BNA_F
ClientSampleId :
DFTPP