
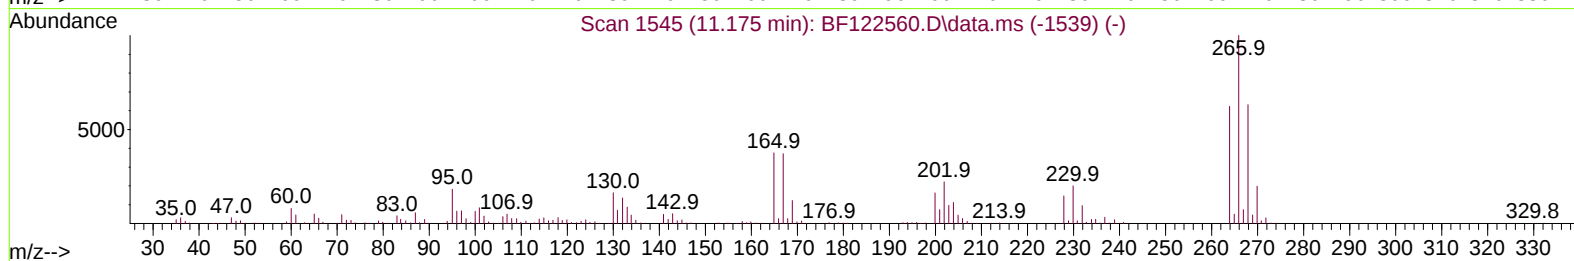
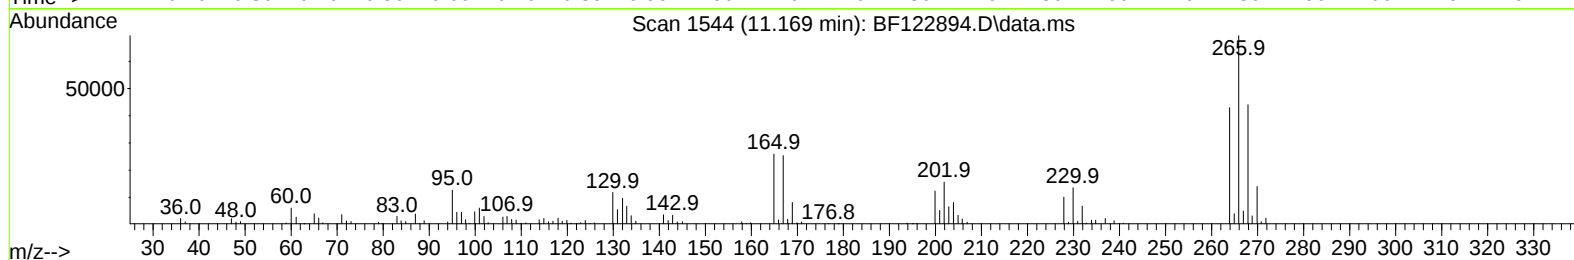


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123120\
Data File : BF122894.D
Acq On : 31 Dec 2020 13:18
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 01 01:39:29 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 31 15:53:00 2020
Response via : Initial Calibration

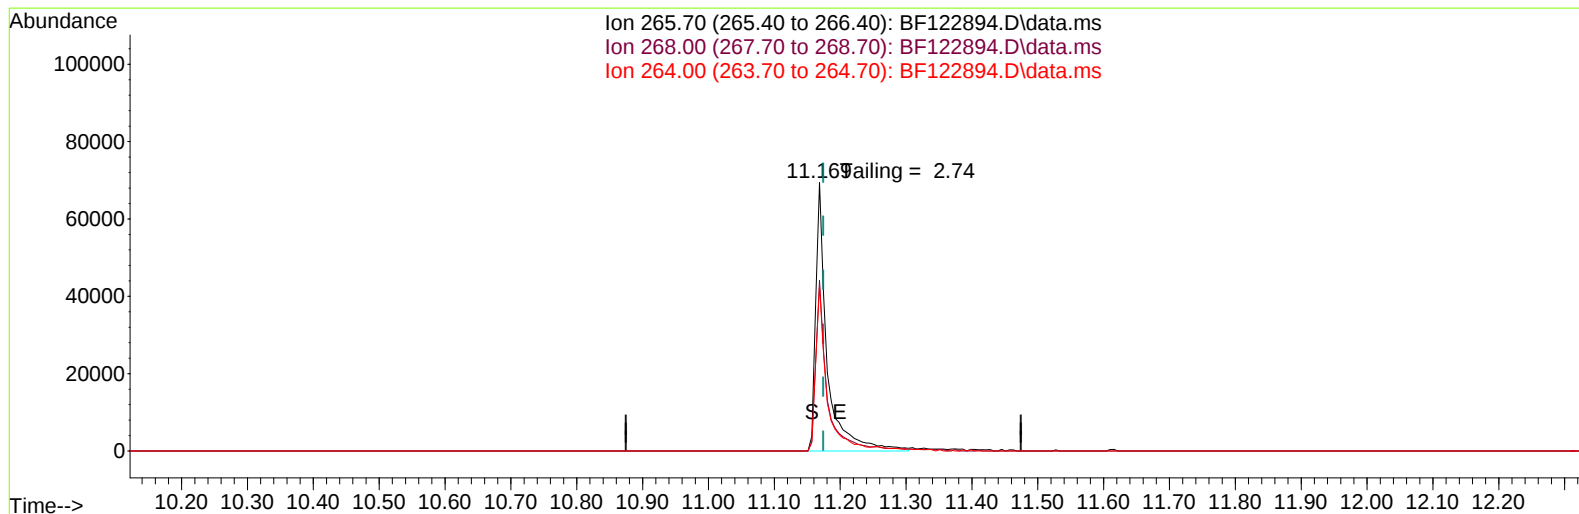

TIC: BF122894.D\data.ms

(70) Pentachlorophenol (C)




11.169min (-0.006) 28419.59 ng

response 85261

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.49
264.00	62.30	61.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123120\
Data File : BF122894.D
Acq On : 31 Dec 2020 13:18
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 01 01:39:29 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 31 15:53:00 2020
Response via : Initial Calibration

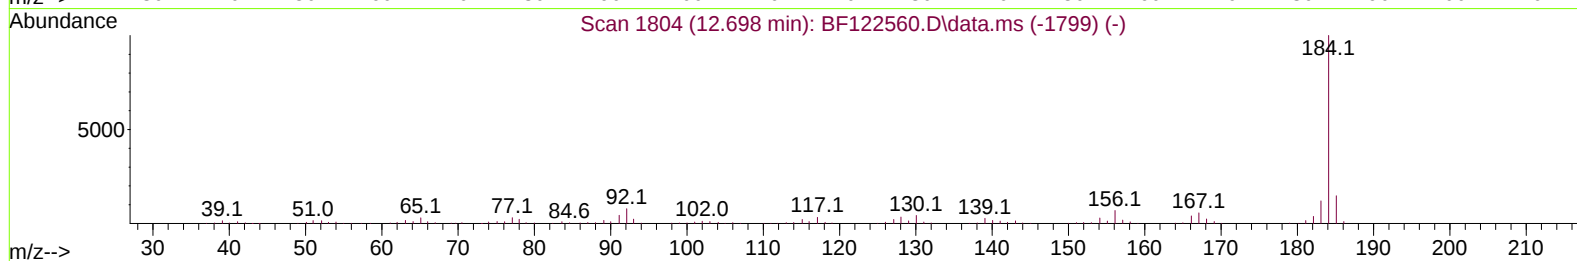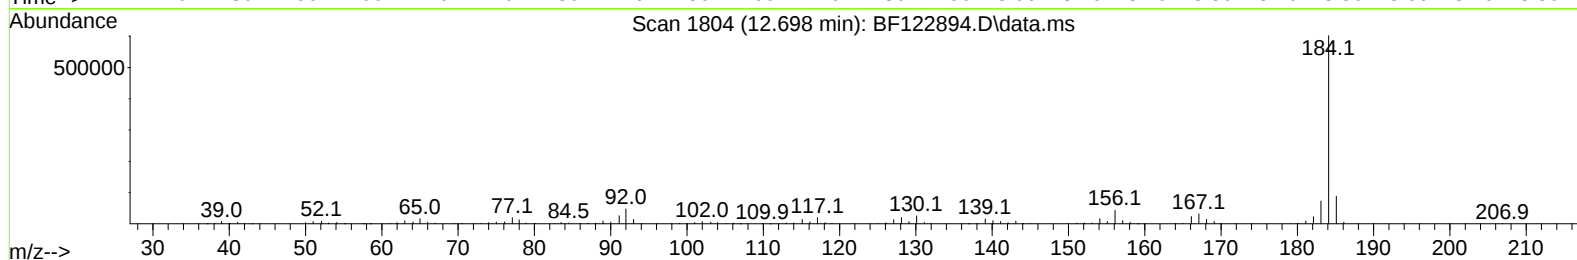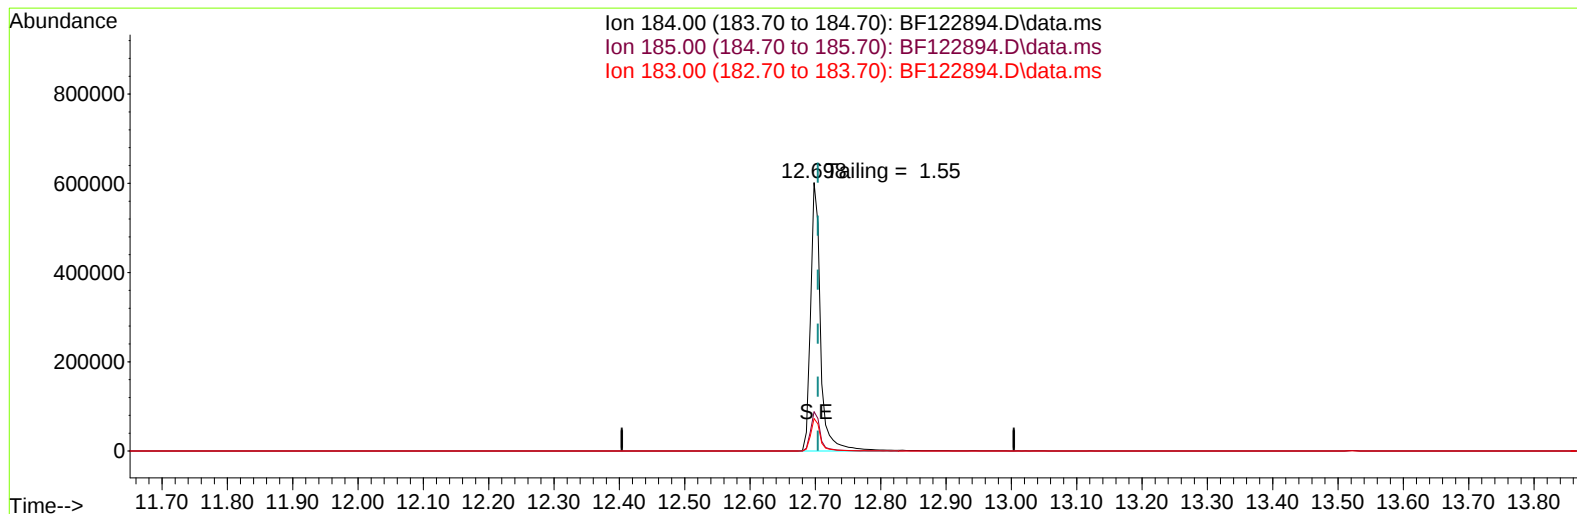

TIC: BF122894.D\data.ms

(77) Benzidine

12.698min (-0.006) 0.00 ng

response 639719

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.69
183.00	12.10	12.14
0.00	0.00	0.00