
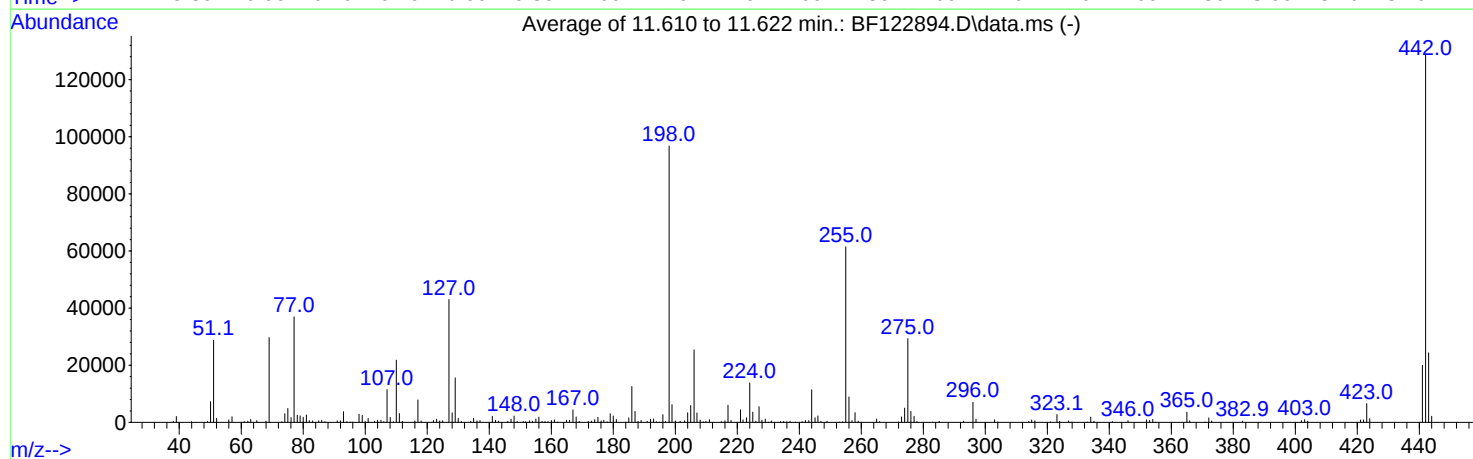


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123120\
 Data File : BF122894.D
 Acq On : 31 Dec 2020 13:18
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 31 15:53:00 2020

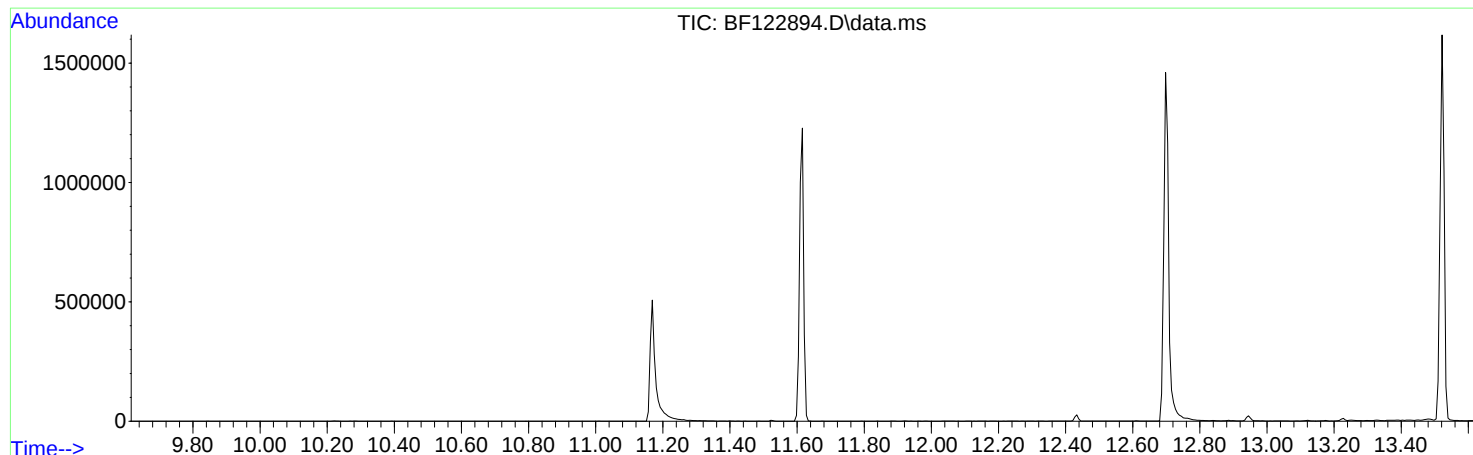

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	28715	PASS
68	69	0.00	2	1.6	469	PASS
69	198	0.00	100	30.7	29696	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.5	43019	PASS
197	198	0.00	2	0.3	269	PASS
198	198	100	100	100.0	96755	PASS
199	198	5	9	6.5	6241	PASS
275	198	10	60	30.3	29317	PASS
365	198	1	100	3.7	3580	PASS
441	198	0.01	100	20.6	19921	PASS
442	442	100	100	100.0	128792	PASS
443	442	15	24	18.9	24384	PASS