


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010623\
Data File : BF131934.D
Acq On : 06 Jan 2023 10:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 06 23:58:27 2023

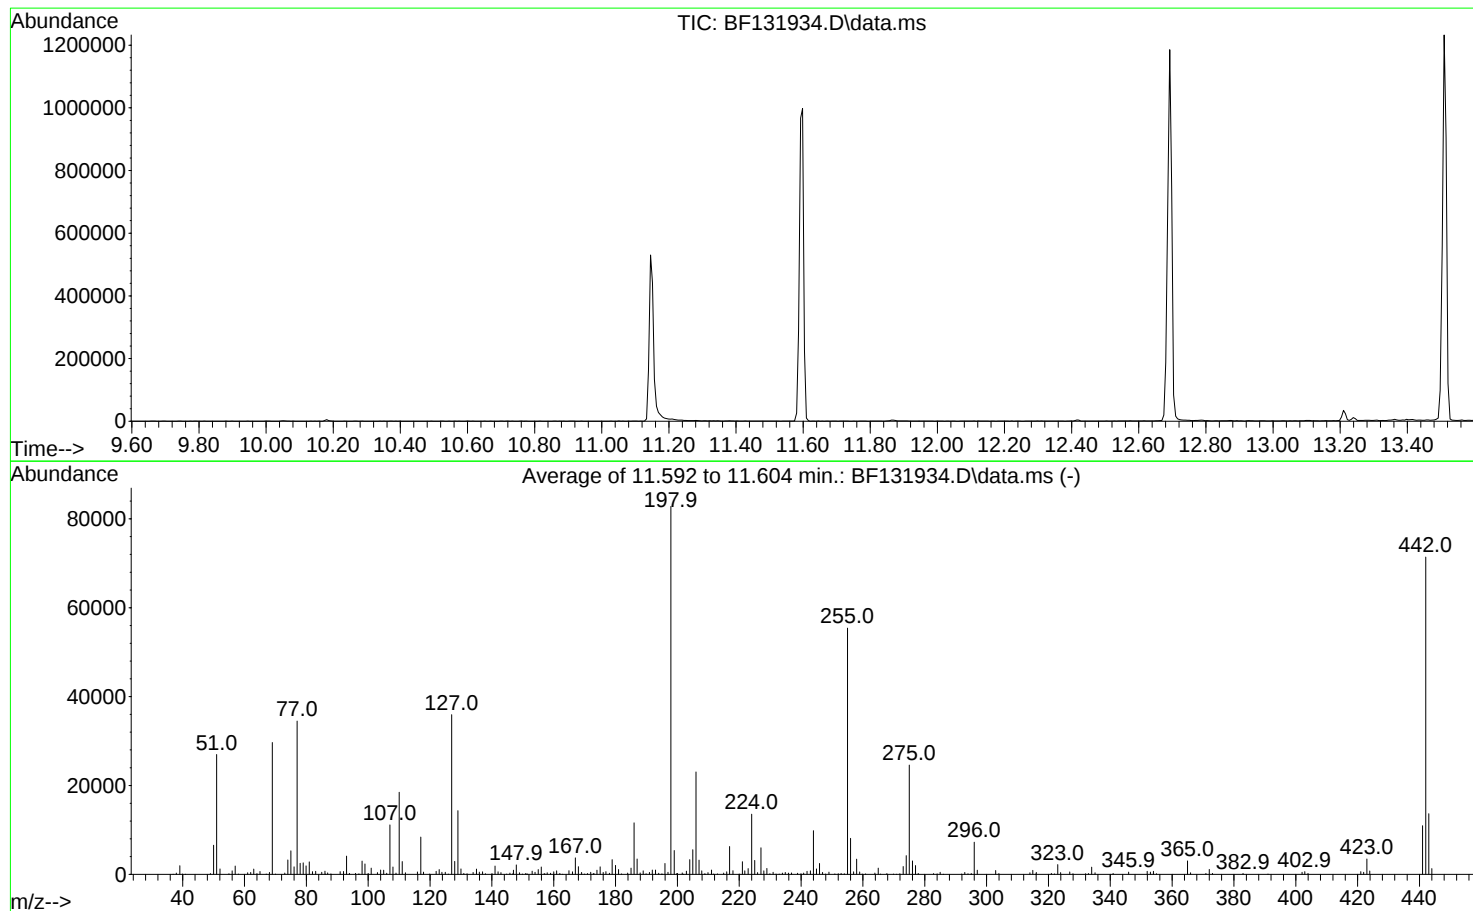




AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	26984	PASS
68	69	0.00	2	1.5	447	PASS
69	198	0.00	100	35.8	29662	PASS
70	69	0.00	2	0.3	81	PASS
127	198	10	80	43.4	35933	PASS
197	198	0.00	2	0.6	475	PASS
198	198	100	100	100.0	82787	PASS
199	198	5	9	6.5	5370	PASS
275	198	10	60	29.7	24600	PASS
365	198	1	100	3.6	3008	PASS
441	198	0.01	100	13.2	10945	PASS
442	442	50	100	100.0	71411	PASS
443	442	15	24	19.1	13658	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010623\
Data File : BF131934.D
Acq On : 06 Jan 2023 10:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 07 04:17:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 06 23:58:27 2023
Response via : Initial Calibration

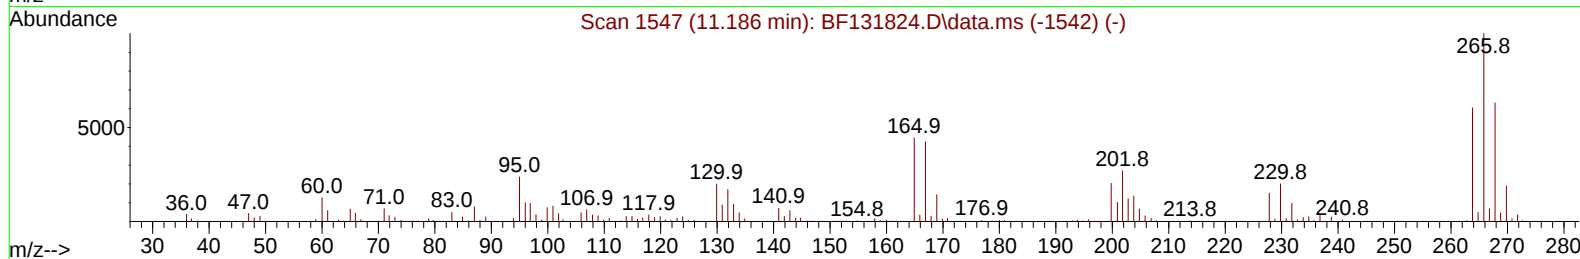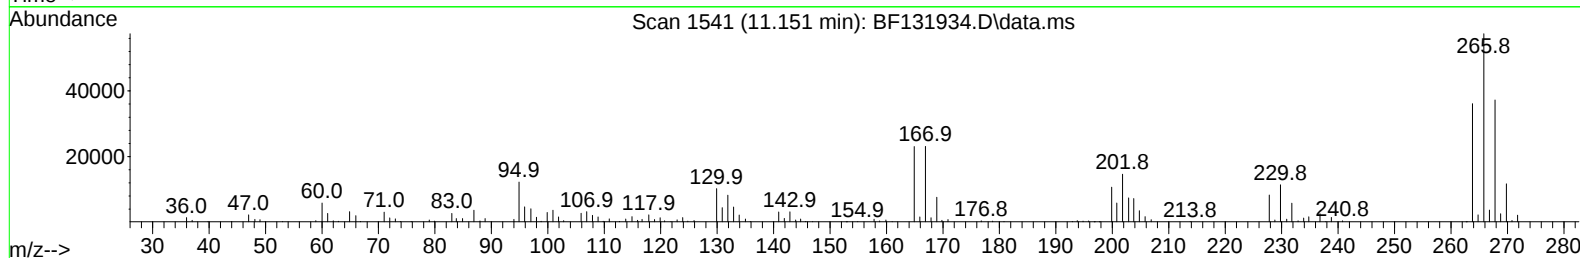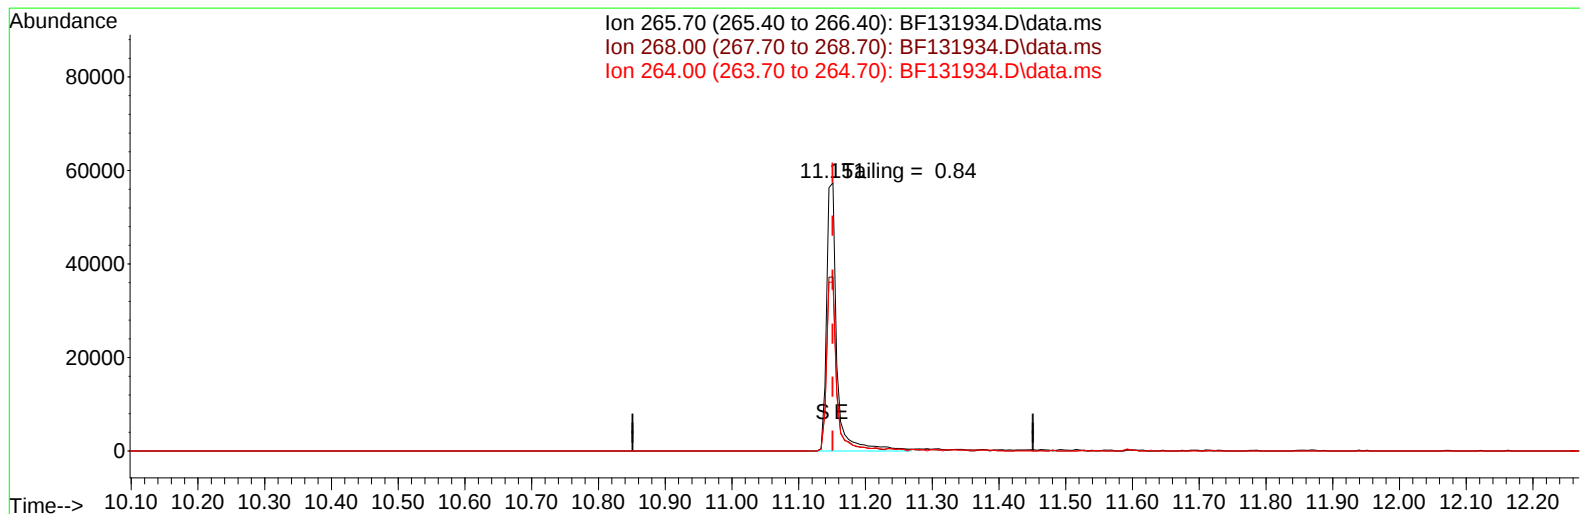

TIC: BF131934.D\data.ms

(70) Pentachlorophenol (C)

11.151min (+ 0.000) 22684.54 ng




response 61310

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.86
264.00	60.40	62.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010623\
Data File : BF131934.D
Acq On : 06 Jan 2023 10:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 07 04:17:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 06 23:58:27 2023
Response via : Initial Calibration

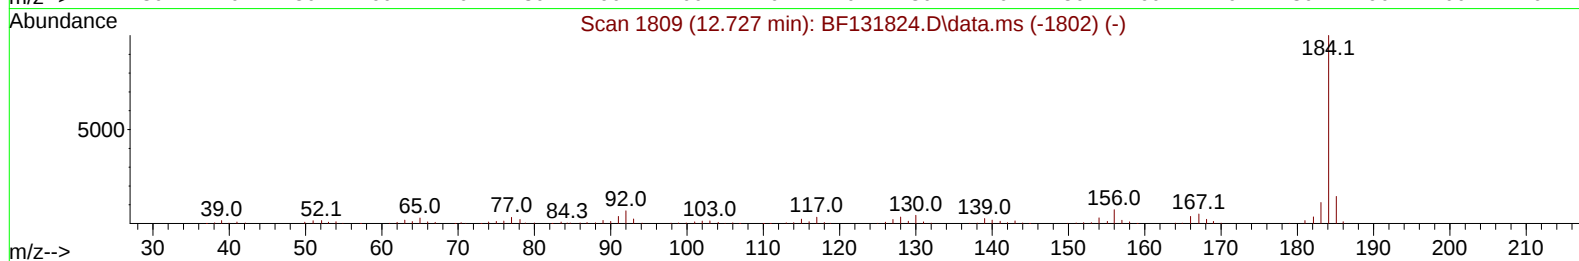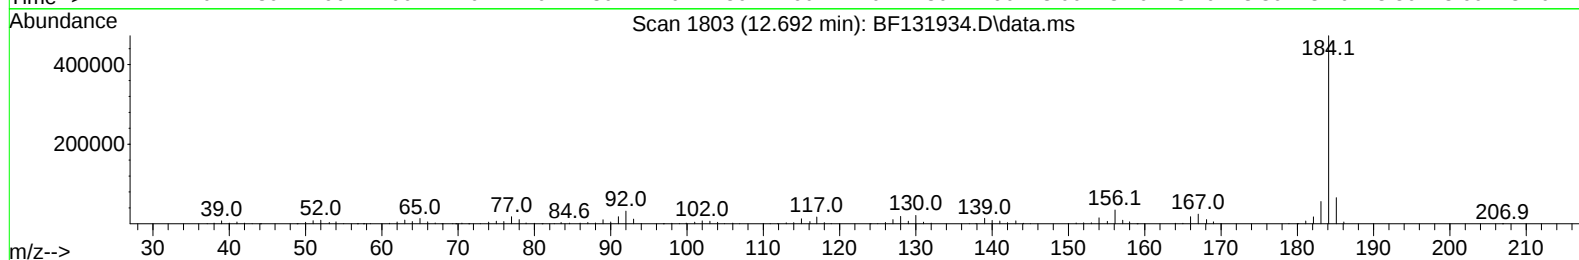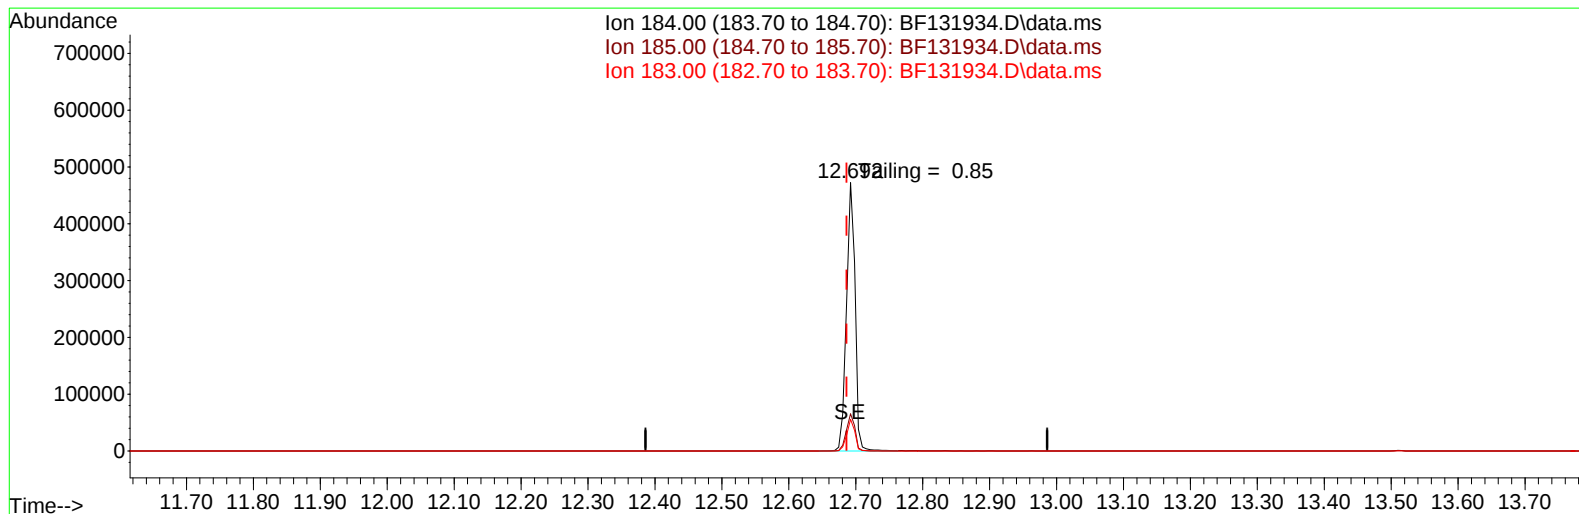

TIC: BF131934.D\data.ms

(77) Benzidine

12.692min (+ 0.006) 0.00 ng

response 423743

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.93
183.00	11.20	11.85
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/6/2023	BNA_F	<u>BF131934.D</u>
Compound Name	Response	Retention Time
DDT	202831	13.51
DDD	7416	13.21
DDE	329	12.875
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7745	210576	3.68

Instrument :
BNA_F
ClientSampleId :
DFTPP