




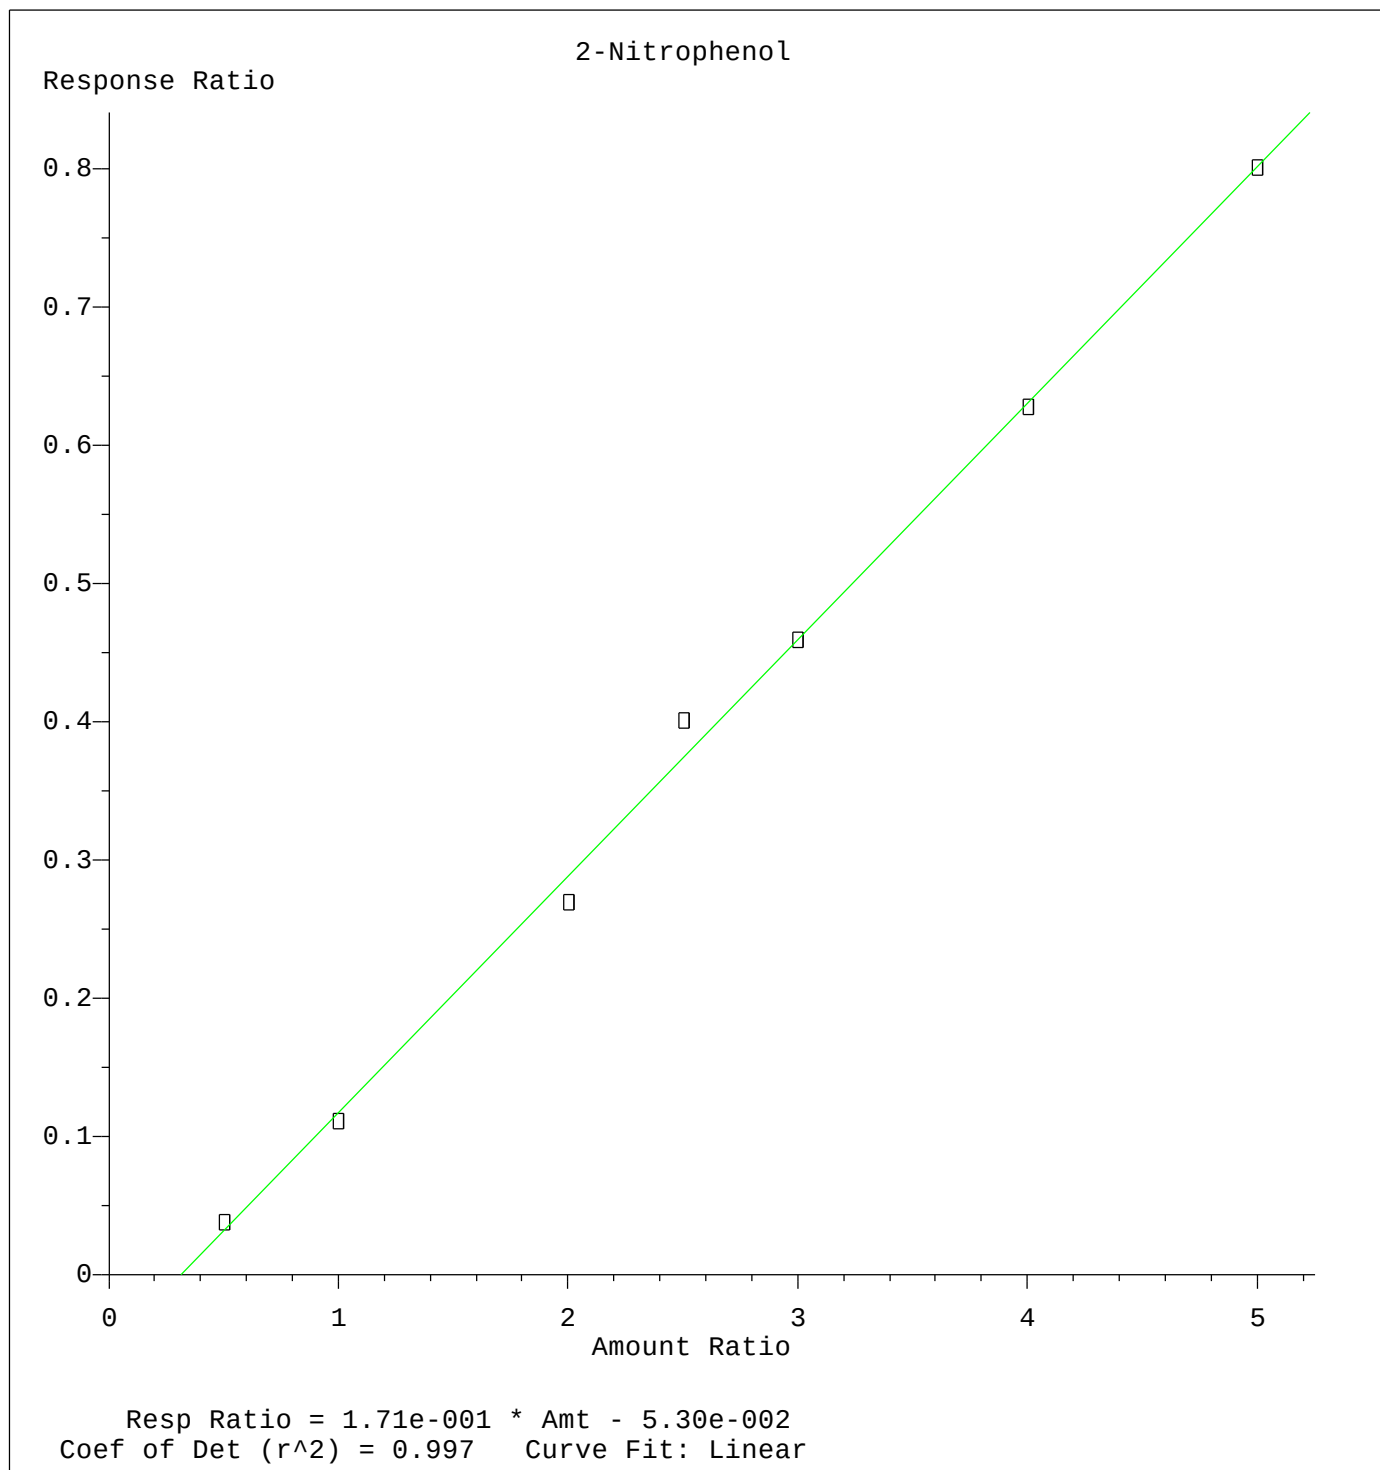

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011720.M
Calibration Table Last Updated: Fri Jan 17 15:49:53 2020

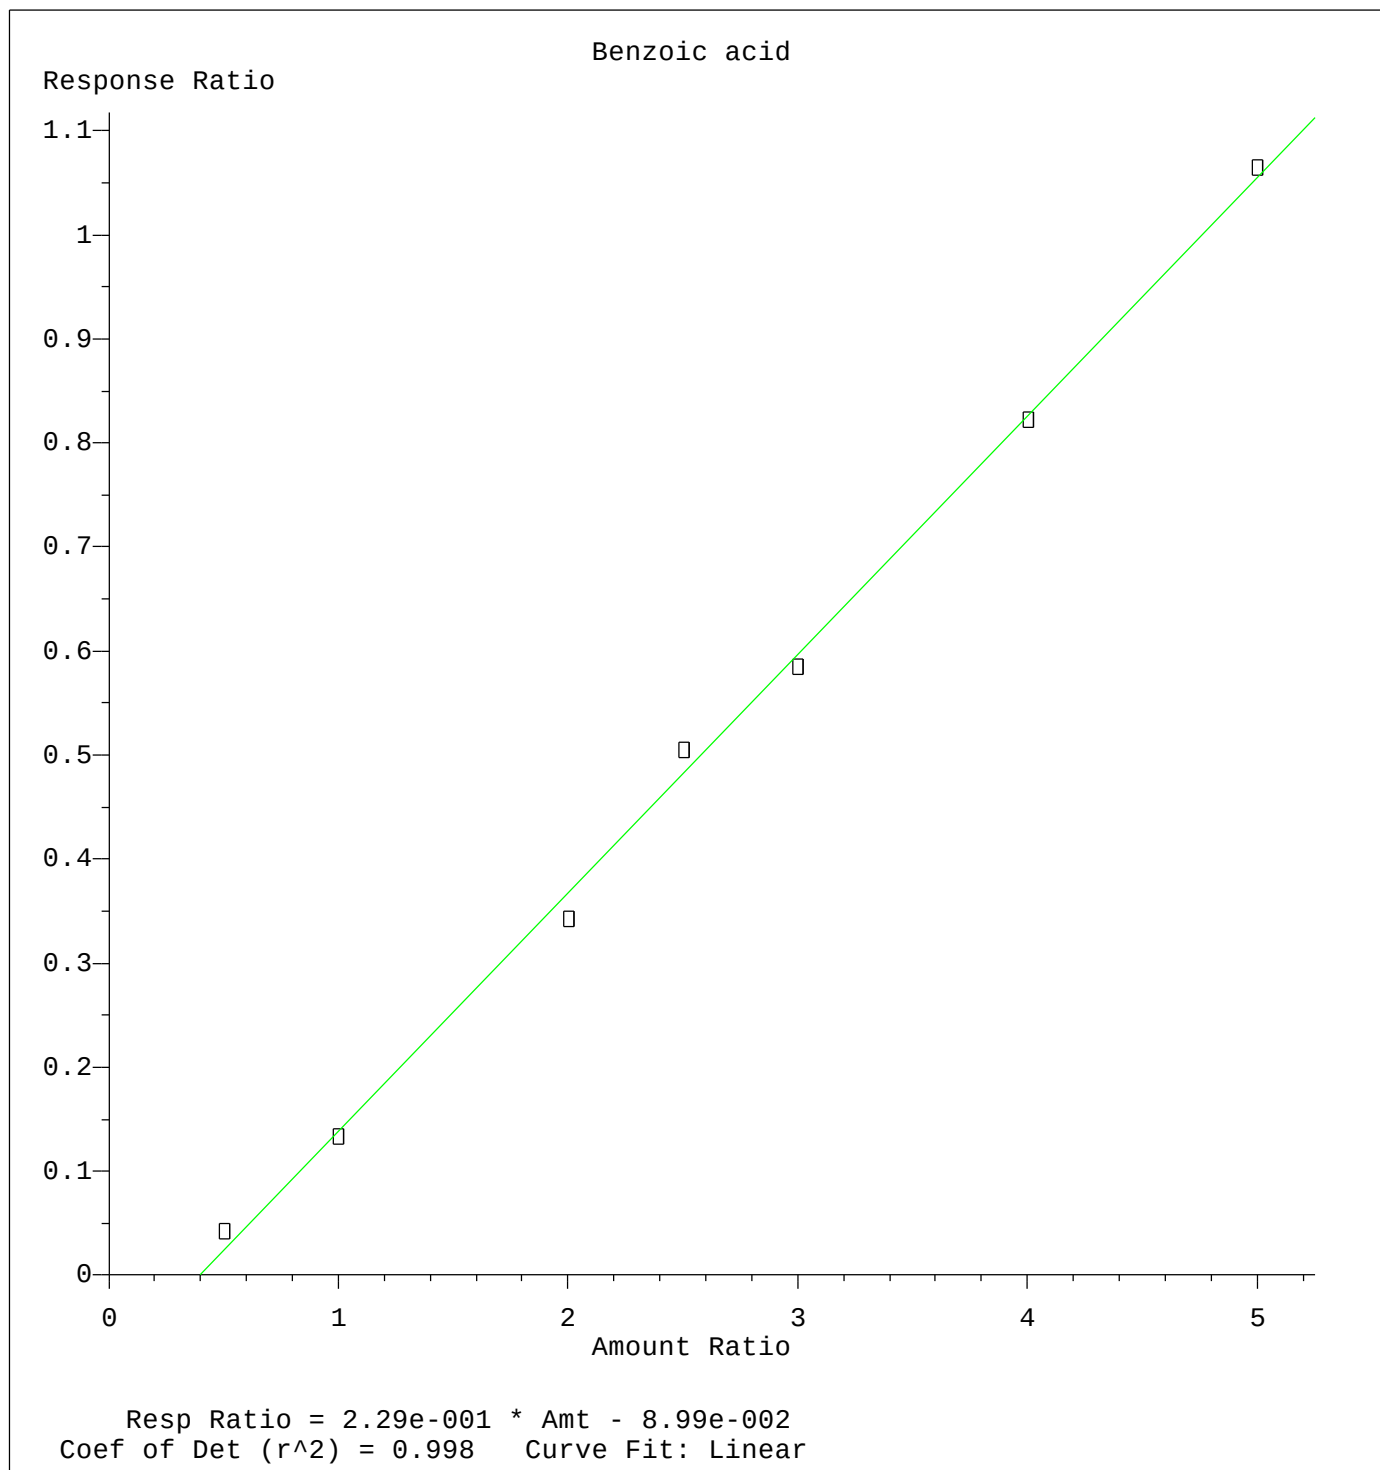


Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011720.M
Calibration Table Last Updated: Fri Jan 17 15:49:53 2020

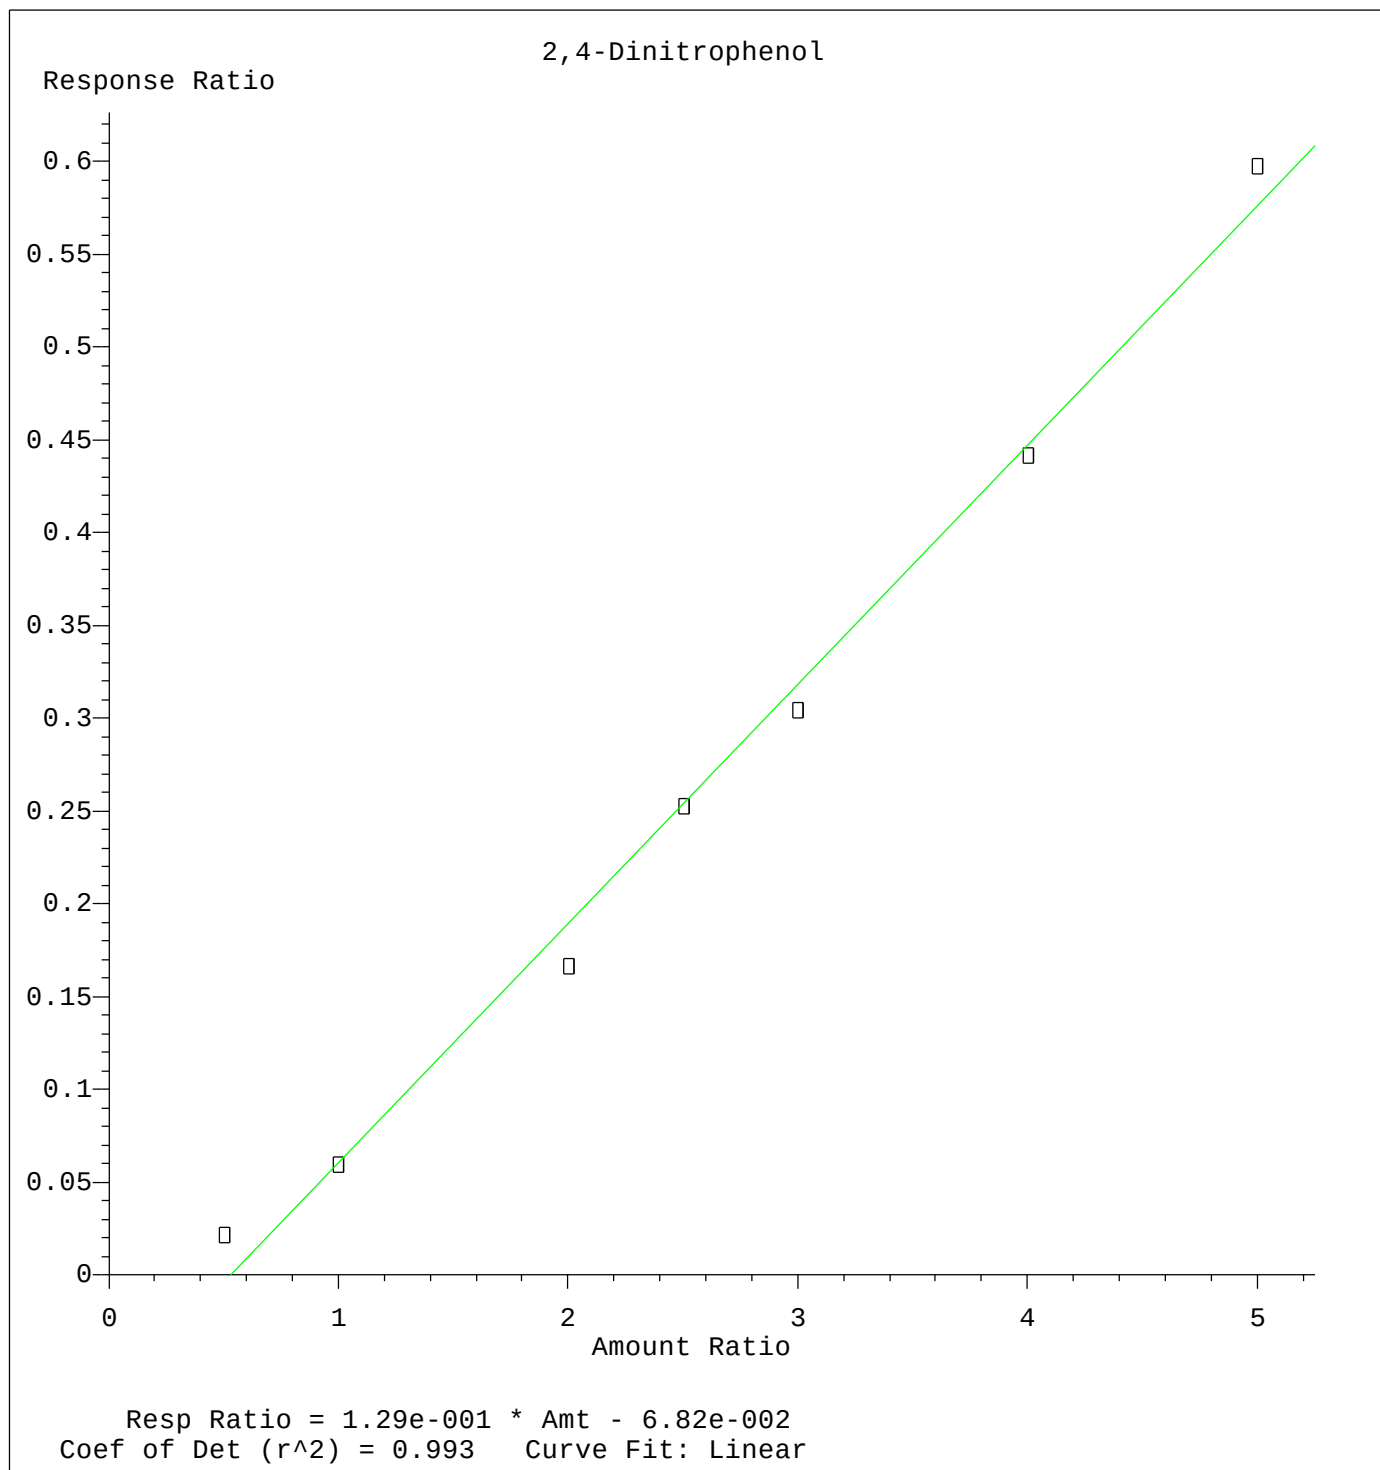

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011720.M
Calibration Table Last Updated: Fri Jan 17 15:49:53 2020


2,4-Dinitrotoluene

Response Ratio

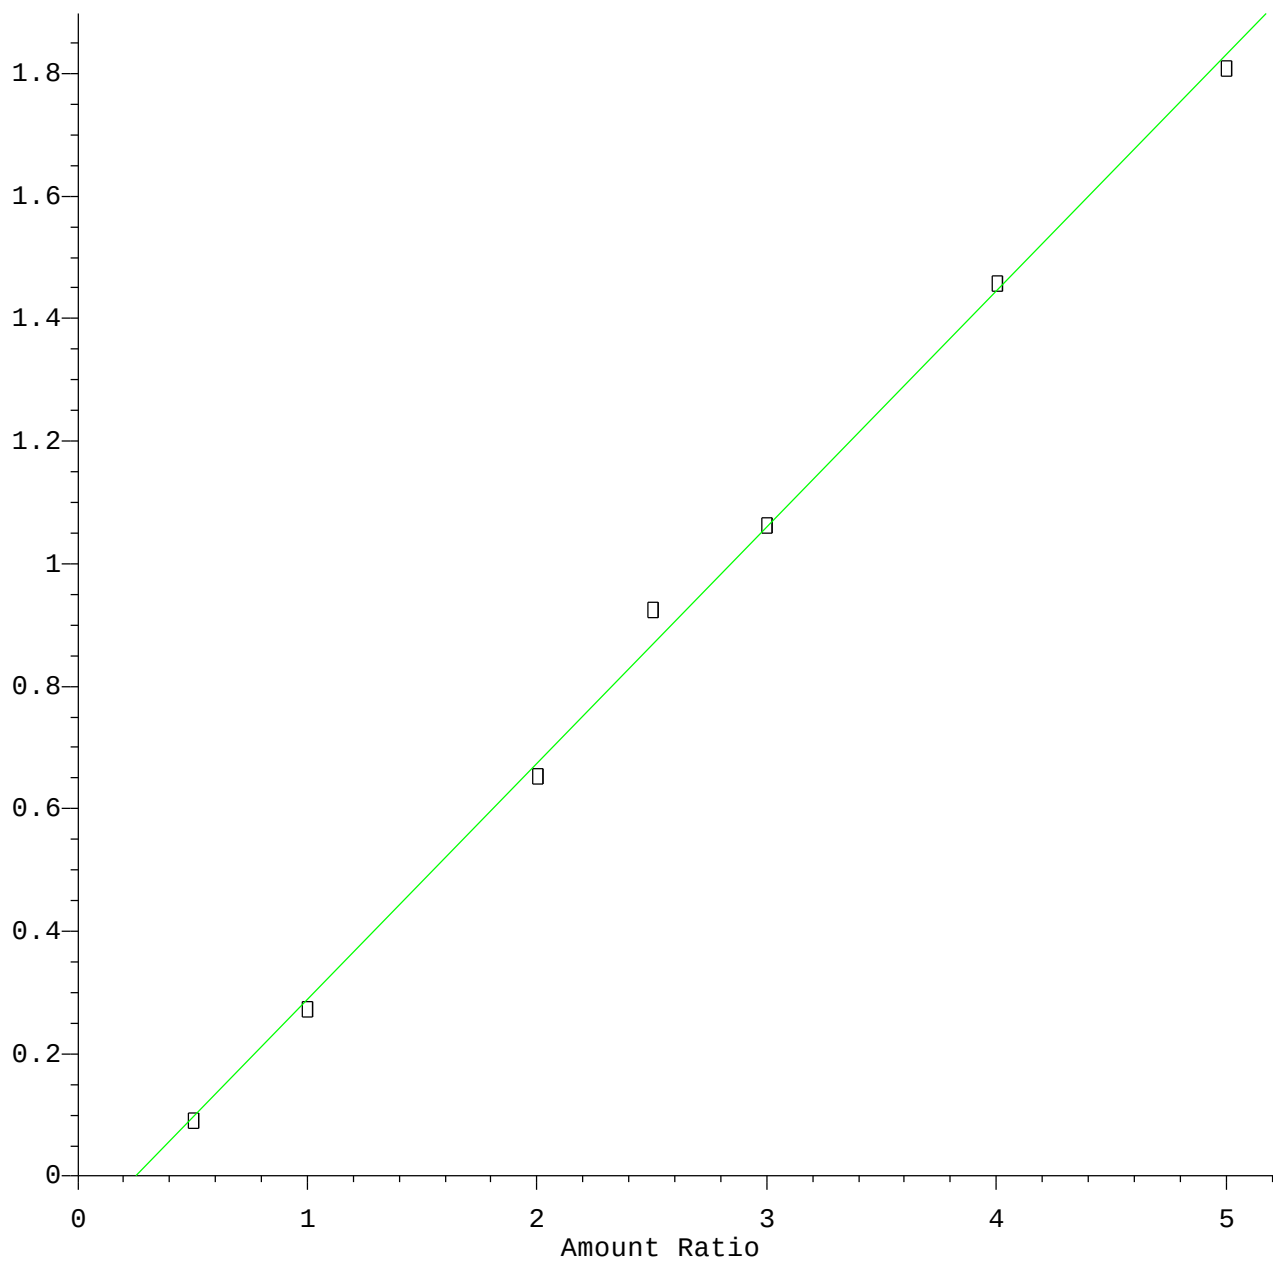

Resp Ratio = $3.86 \times 10^{-1} \times \text{Amt} - 9.72 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011720.M
Calibration Table Last Updated: Fri Jan 17 15:49:53 2020

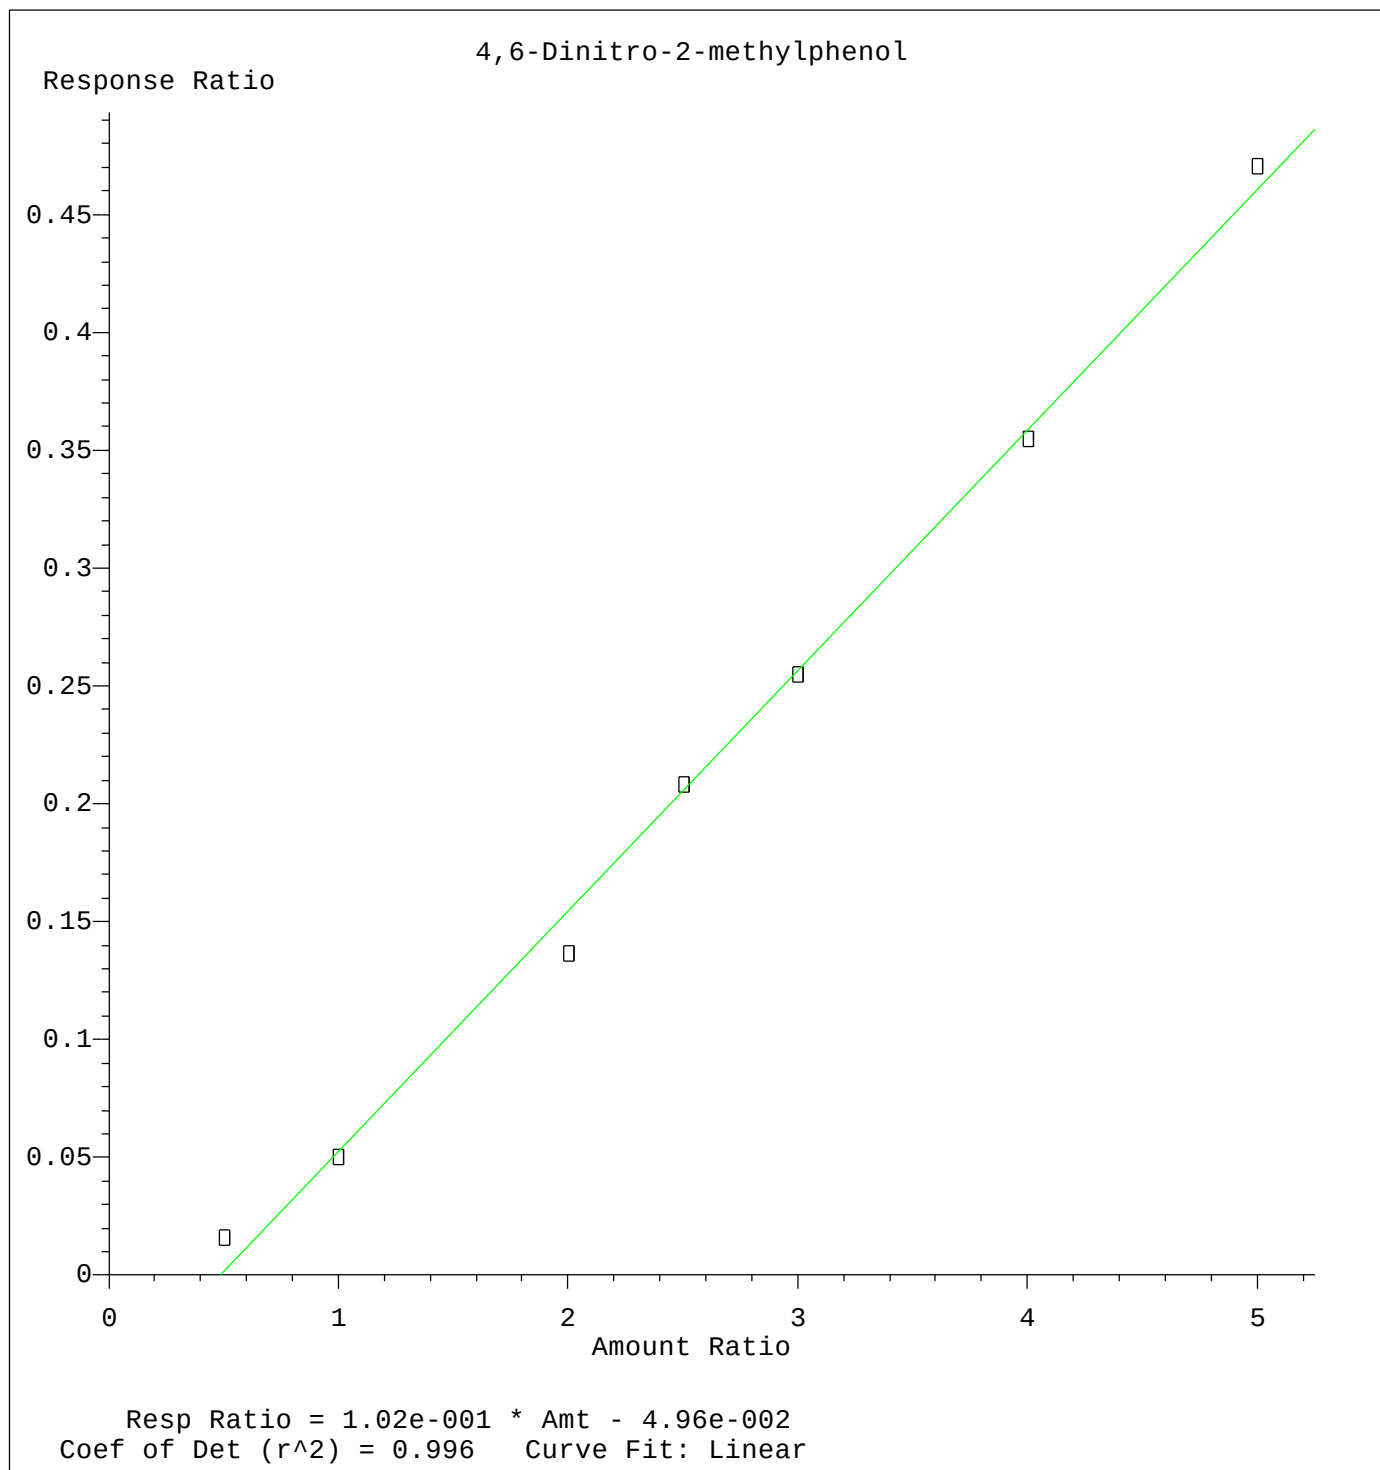

Method Name: Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011720.M
Calibration Table Last Updated: Fri Jan 17 15:49:53 2020