
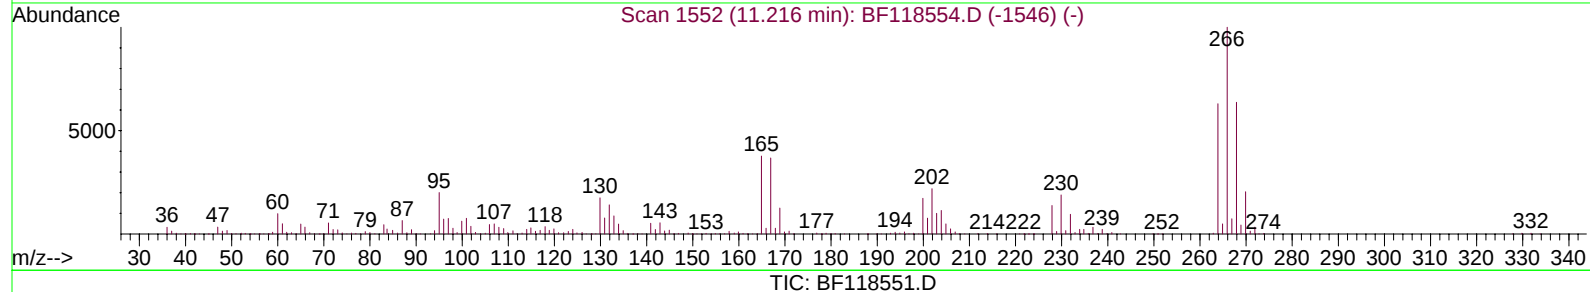
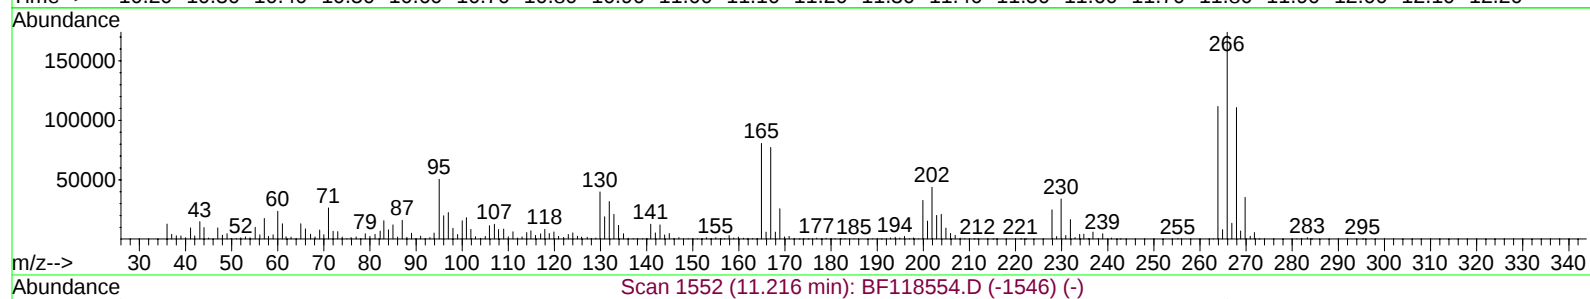


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF011720\
Data File : BF118551.D
Acq On : 17 Jan 2020 10:11
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 18:00:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF011720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 17 15:49:53 2020
Response via : Initial Calibration

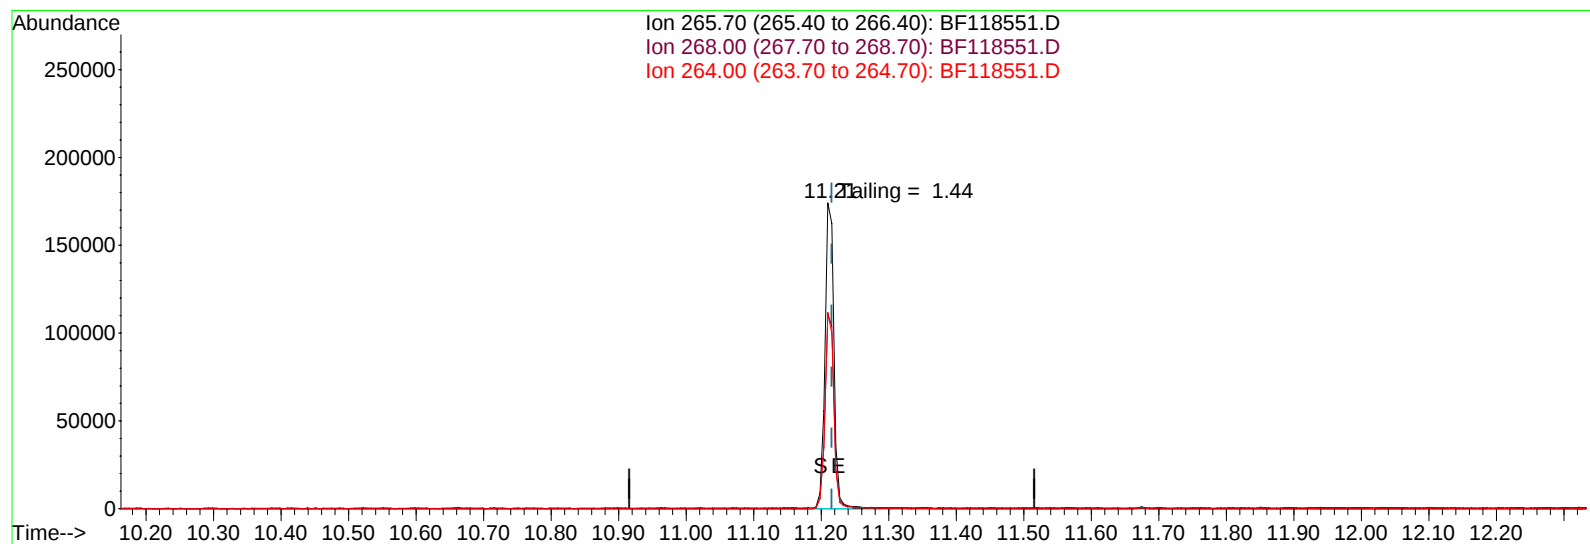

(70) Pentachlorophenol (C)




11.210min (-0.006) 14088.00ng

response 161761

Ion	Exp%	Act%
265.70	100	100
268.00	63.70	63.58
264.00	63.10	64.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF011720\
Data File : BF118551.D
Acq On : 17 Jan 2020 10:11
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 18:00:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF011720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 17 15:49:53 2020
Response via : Initial Calibration

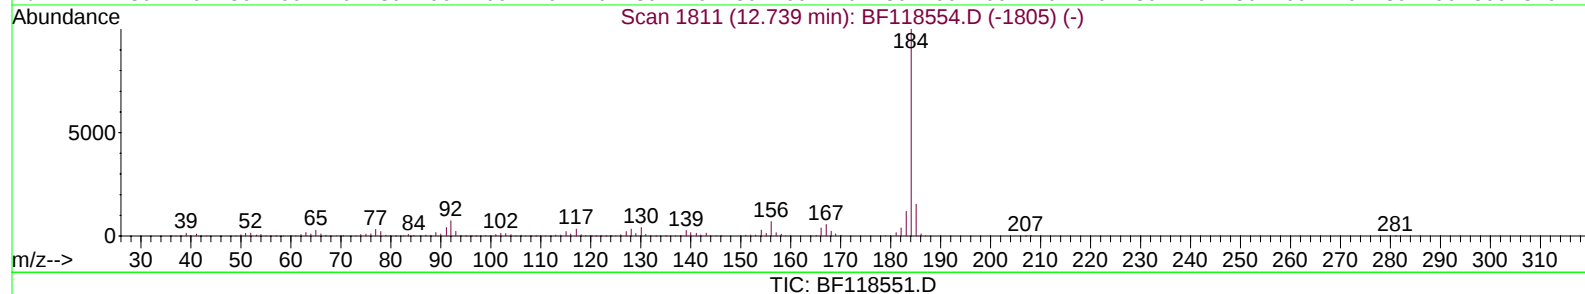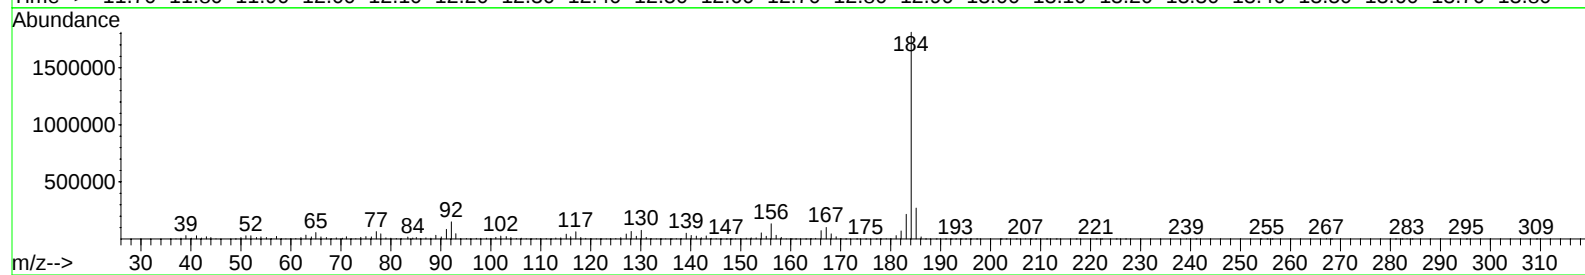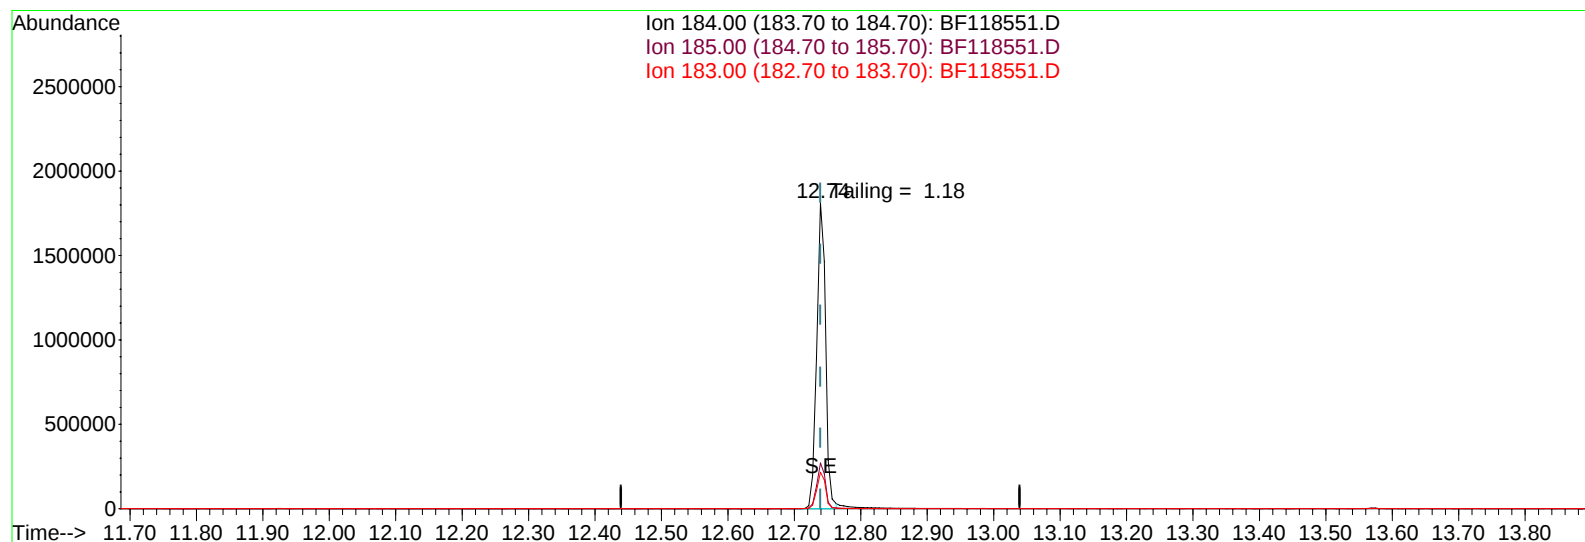

(77) Benzidine

12.739min (+0.000) 353890.96ng

response 1728244

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	14.99
183.00	11.90	11.92
0.00	0.00	0.00