
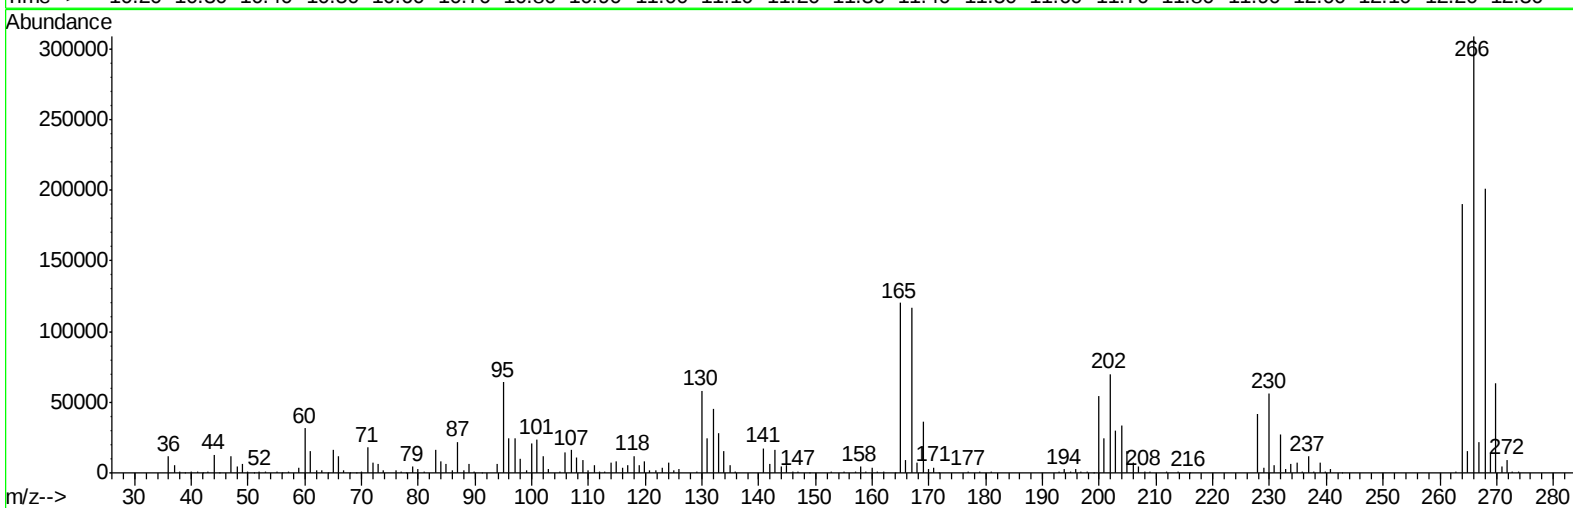


Data File : BF118560.D
Acq On : 17 Jan 2020 16:02
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 02:02:35 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 17 15:49:53 2020
Response via : Initial Calibration

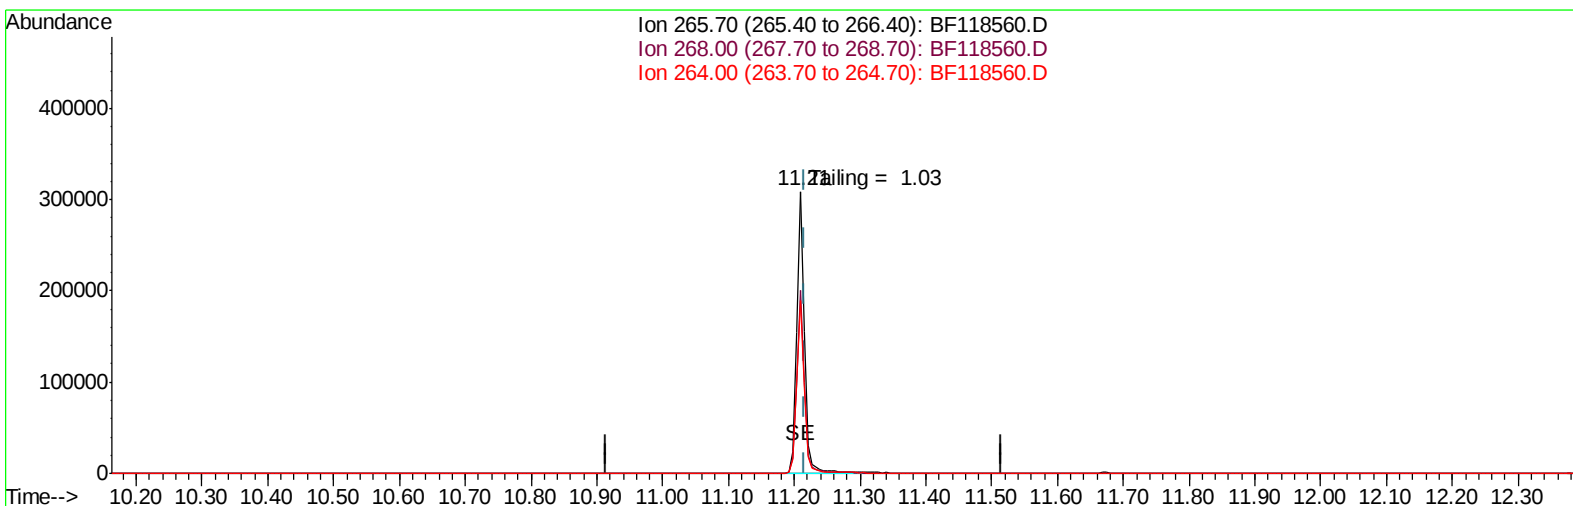

TIC: BF118560.D

(70) Pentachlorophenol (C)



11.210min (-0.006) 246921.46ng

response 257418

Ion	Exp%	Act%
265.70	100	100
268.00	63.70	65.18
264.00	63.10	61.51
0.00	0.00	0.00

Data File : BF118560.D
Acq On : 17 Jan 2020 16:02
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 02:02:35 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 17 15:49:53 2020
Response via : Initial Calibration

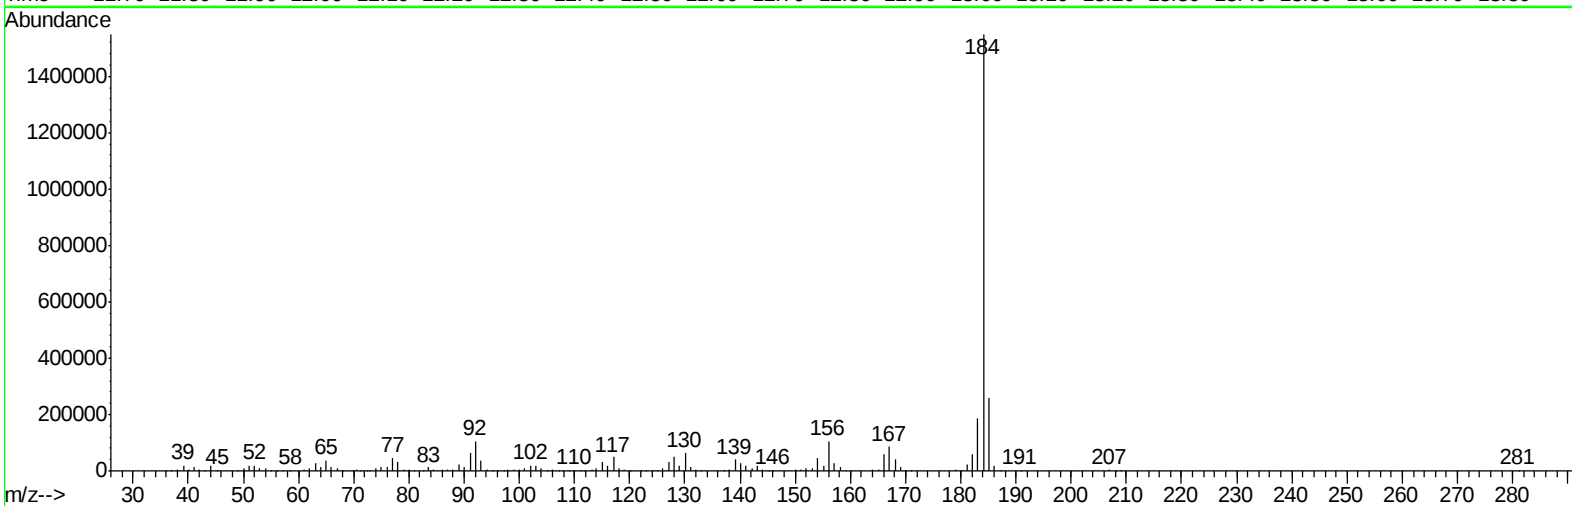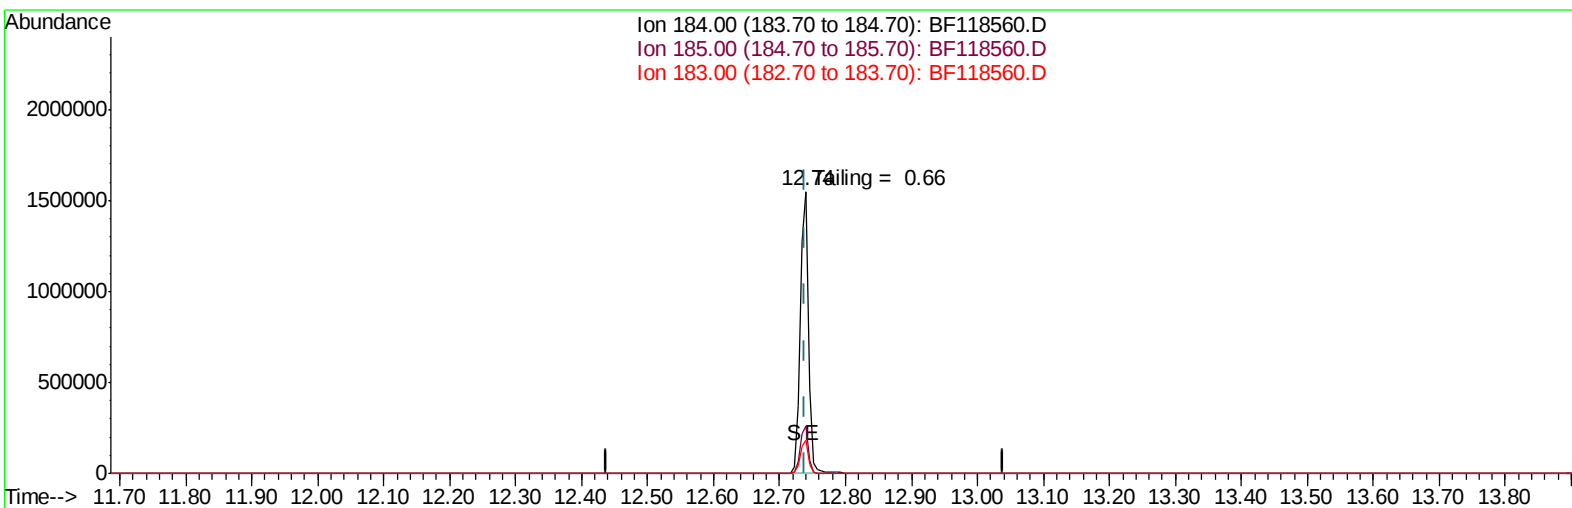

TIC: BF118560.D

(77) Benzidine

12.739min (+0.000) 487423.97ng

response 1361897

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	16.77
183.00	11.90	12.02
0.00	0.00	0.00