

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF011720\
 Data File : BF118570.D
 Acq On : 17 Jan 2020 20:55
 Operator : JU
 Sample : L1010-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OK-02-011620

Quant Time: Jan 18 01:38:30 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF011720.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 17 15:49:53 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	318067	20.00	ng	0.00
21) Naphthalene-d8	8.17	136	1158016	20.00	ng	0.00
39) Acenaphthene-d10	9.92	164	638177	20.00	ng	-0.01
64) Phenanthrene-d10	11.41	188	1186087	20.00	ng	0.00
76) Chrysene-d12	14.04	240	997506	20.00	ng	-0.01
87) Perylene-d12	15.52	264	1019866	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.52	112	2401330	139.50	ng	0.01
7) Phenol-d6	6.52	99	2911980	129.10	ng	0.00
23) Nitrobenzene-d5	7.45	82	1963588	104.73	ng	-0.01
42) 2,4,6-Tribromophenol	10.71	330	1103257	156.38	ng	0.00
45) 2-Fluorobiphenyl	9.25	172	3648570	103.21	ng	0.00
79) Terphenyl-d14	13.00	244	4528481	89.66	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF011720\
Data File : BF118570.D
Acq On : 17 Jan 2020 20:55
Operator : JU
Sample : L1010-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-02-011620

Quant Time: Jan 18 01:38:30 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF011720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 17 15:49:53 2020
Response via : Initial Calibration

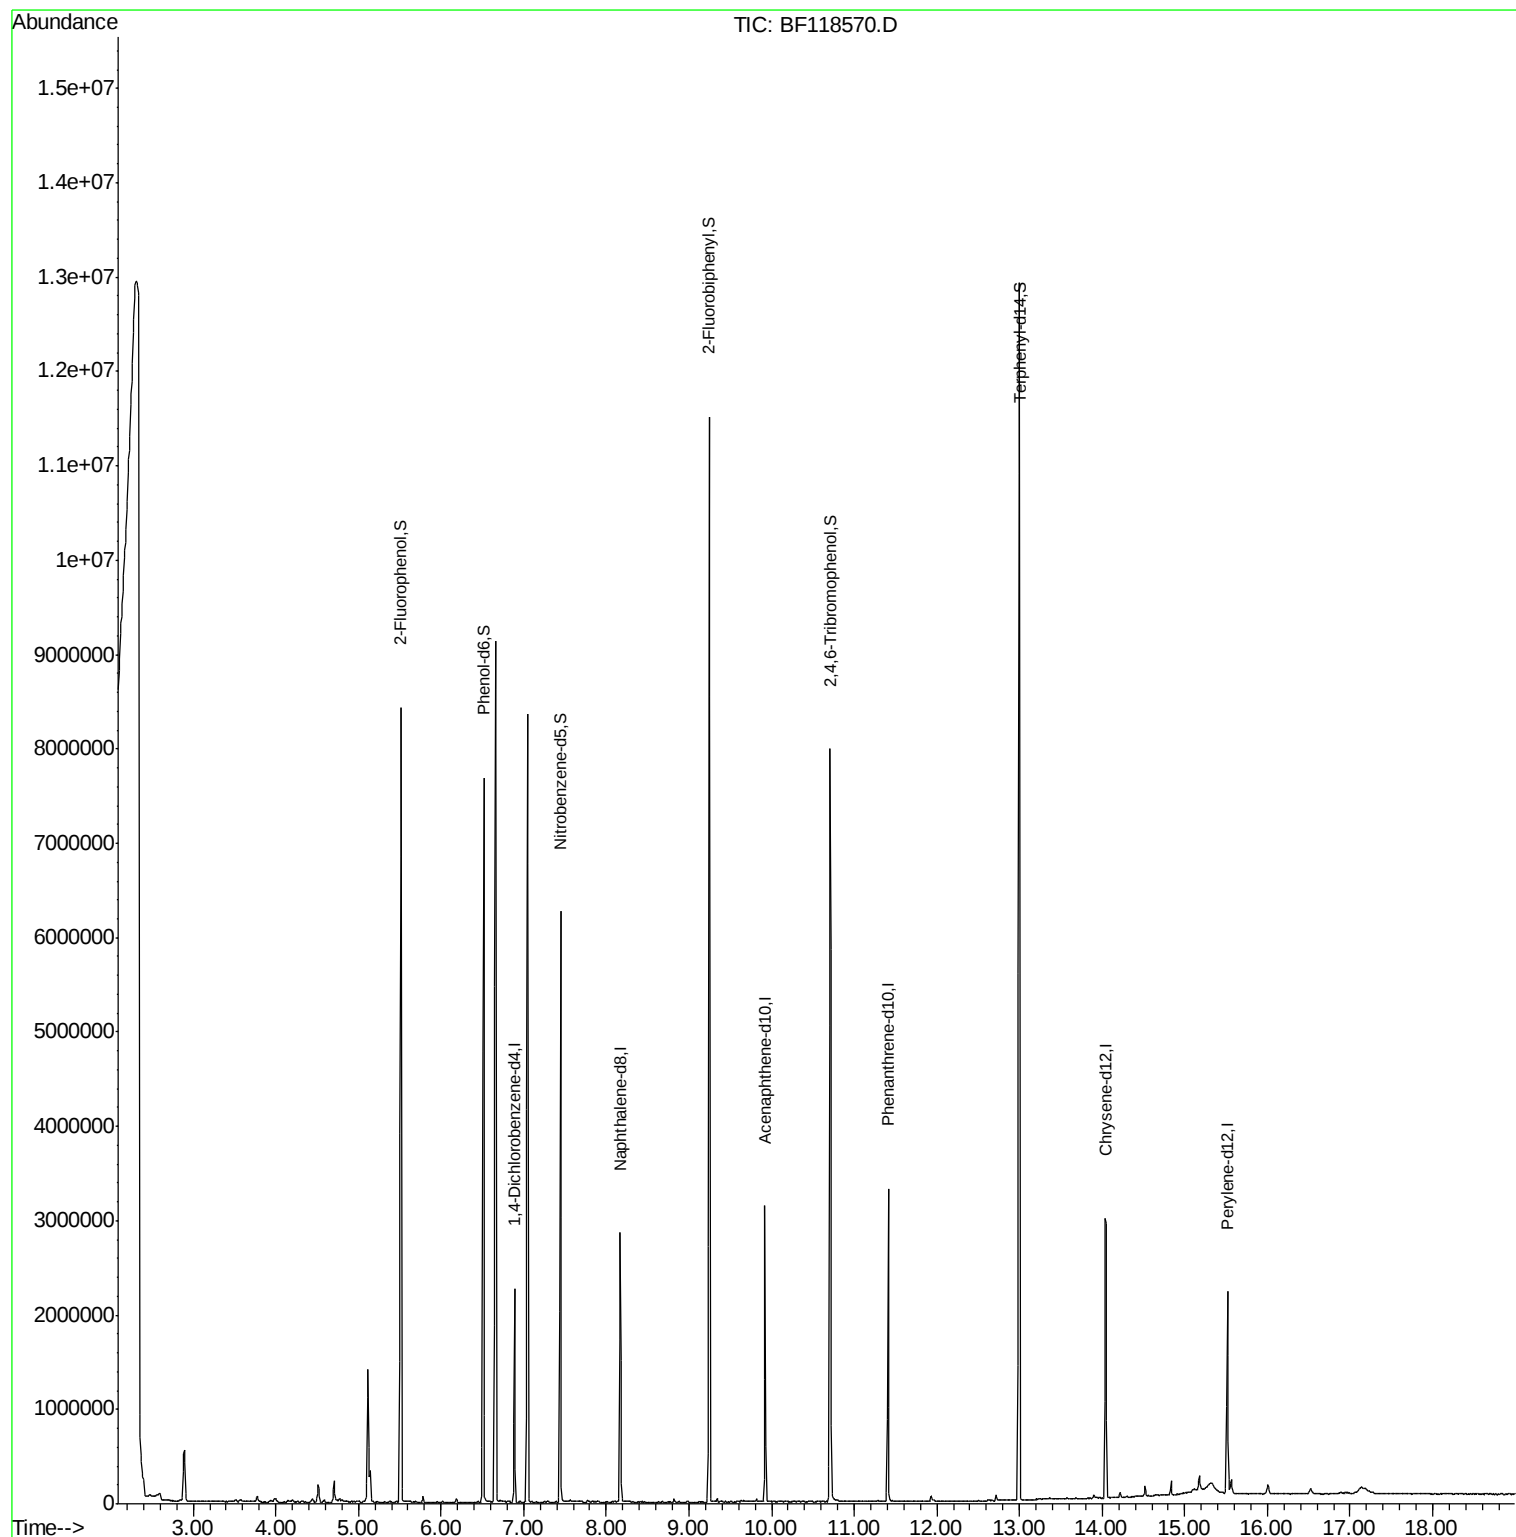

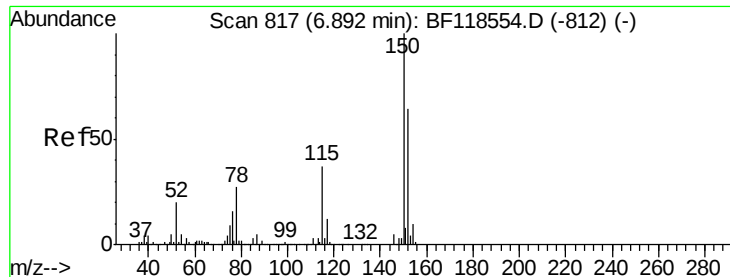


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.89 min Scan# 816
Delta R.T. -0.01 min
Lab File: BF118570.D
Acq: 17 Jan 2020 20:55

Instrument :
BNA_F
ClientSampleId :
OK-02-011620

Tot Ion	Ratio	Lower	Upper
152	100		
150	156.9	124.9	187.3
115	60.6	45.8	68.6

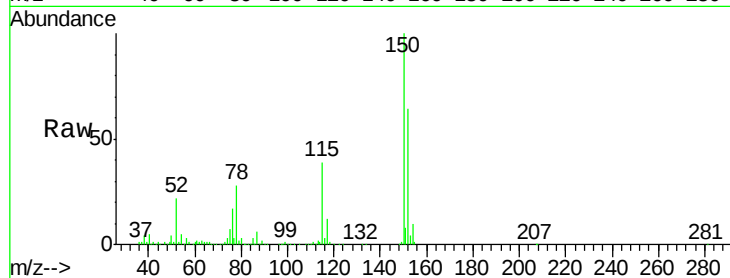


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

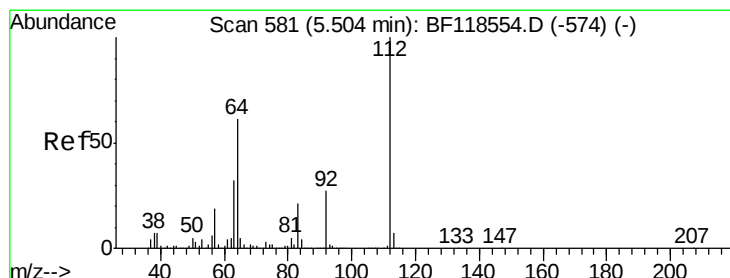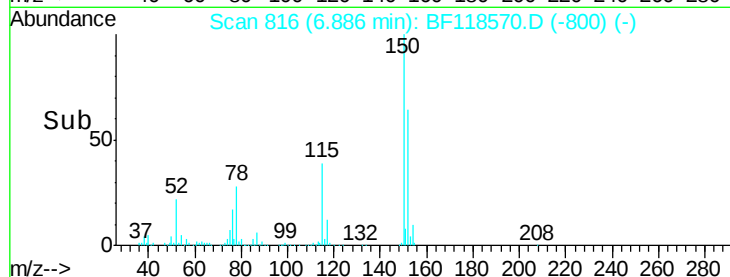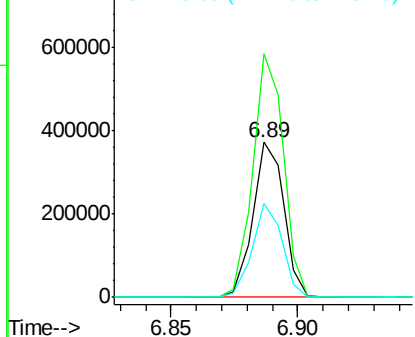



#5


2-Fluorophenol
Concen: 139.499 ng
RT: 5.52 min Scan# 583
Delta R.T. 0.01 min
Lab File: BF118570.D
Acq: 17 Jan 2020 20:55

Tgt Ion	Ratio	Lower	Upper
112	100		
64	59.7	49.1	73.7
63	32.1	25.8	38.8

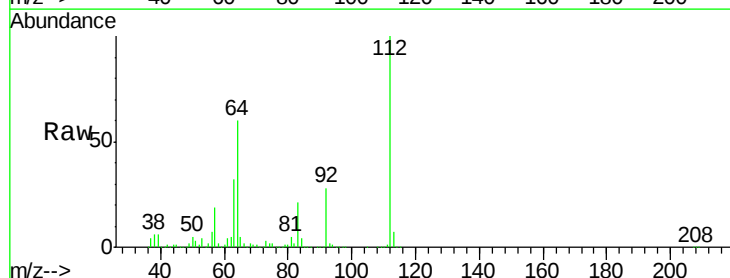

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

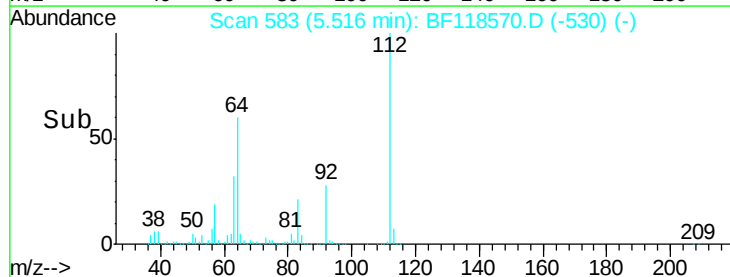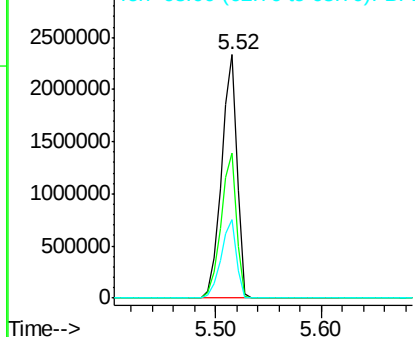

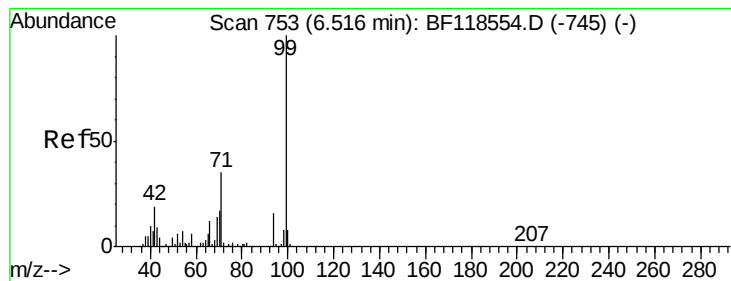

#7

Phenol-d6

Concen: 129.102 ng

RT: 6.52 min Scan# 753

Delta R.T. -0.00 min

Lab File: BF118570.D

Acq: 17 Jan 2020 20:55

Instrument :

BNA_F

ClientSampleId :

OK-02-011620


Tot Ion: 99 Resp: 2911980

Ion Ratio Lower Upper

99 100

42 17.9 14.9 22.3




71 35.3 28.3 42.5

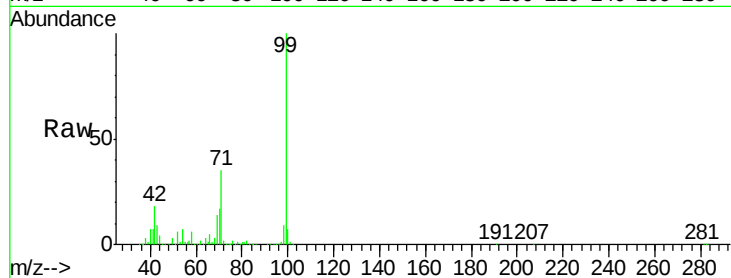

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

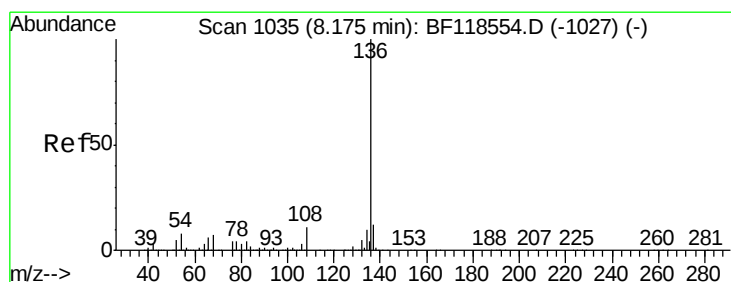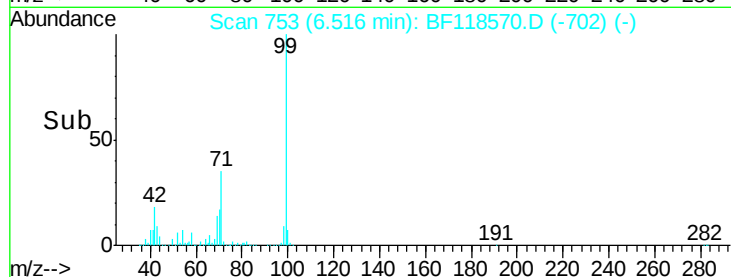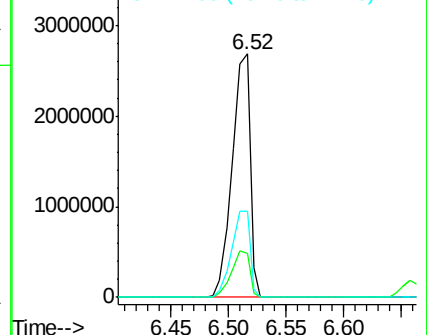

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.17 min Scan# 1034

Delta R.T. -0.01 min

Lab File: BF118570.D

Acq: 17 Jan 2020 20:55

Tgt Ion: 136 Resp: 1158016


Ion Ratio Lower Upper

136 100

137 11.1 9.4 14.0

54 7.4 6.2 9.2

68 6.4 5.4 8.0


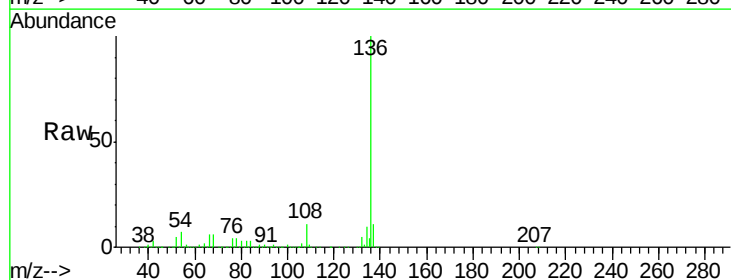



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1



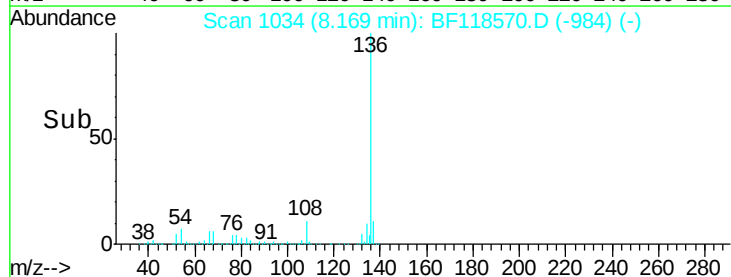
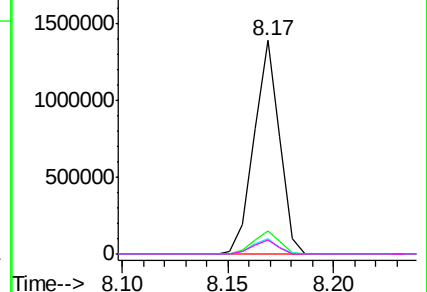


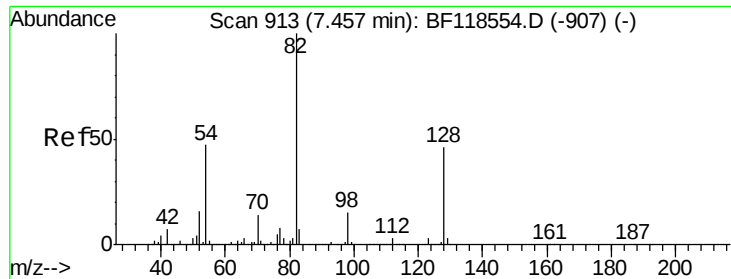

#23
Nitrobenzene-d5
Concen: 104.726 ng
RT: 7.45 min Scan# 911
Delta R.T. -0.01 min
Lab File: BF118570.D
Acq: 17 Jan 2020 20:55




Instrument :
BNA_F
ClientSampled :
OK-02-011620


Tot Ion: 82 Resp: 1963588
Ion Ratio Lower Upper
82 100
128 45.2 37.0 55.4
54 48.2 37.4 56.0

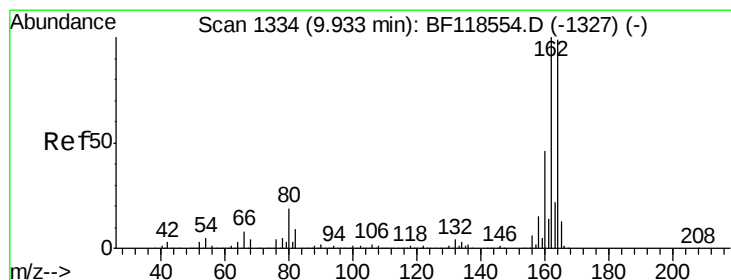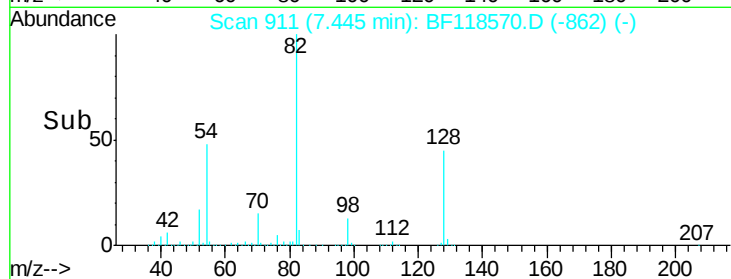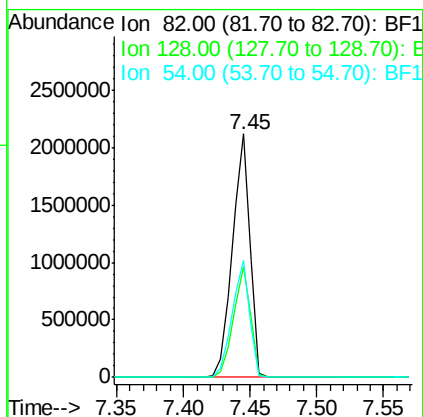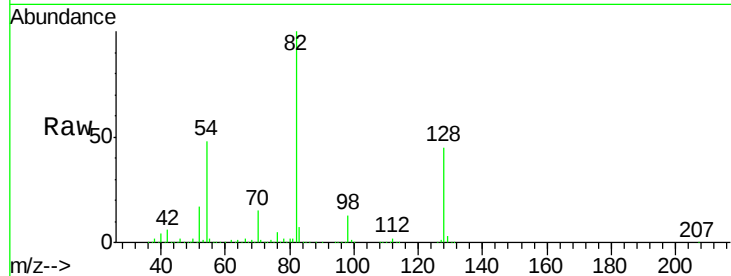

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.92 min Scan# 1332
Delta R.T. -0.01 min
Lab File: BF118570.D
Acq: 17 Jan 2020 20:55

Tgt Ion:164 Resp: 638177
Ion Ratio Lower Upper
164 100
162 100.8 80.6 120.8
160 45.9 36.7 55.1

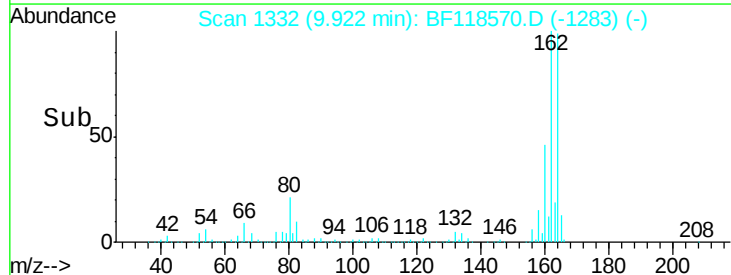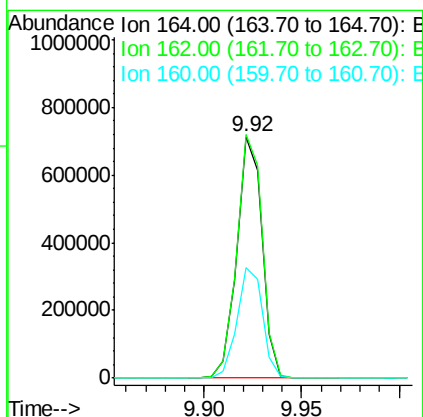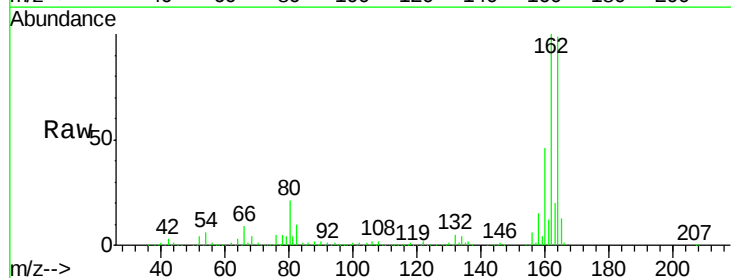


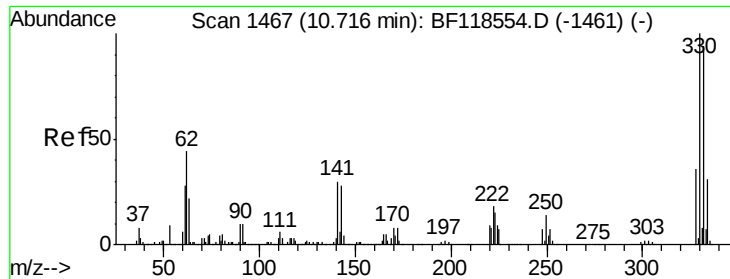




#42
 2,4,6-Tribromophenol
 Concen: 156.381 ng
 RT: 10.71 min Scan# 1466
 Delta R.T. -0.01 min
 Lab File: BF118570.D
 Acq: 17 Jan 2020 20:55

Instrument :
 BNA_F
 ClientSampleId :
 OK-02-011620

Tot Ion:330 Resp: 1103257
 Ion Ratio Lower Upper
 330 100
 332 95.2 76.4 114.6
 141 28.8 23.4 35.2

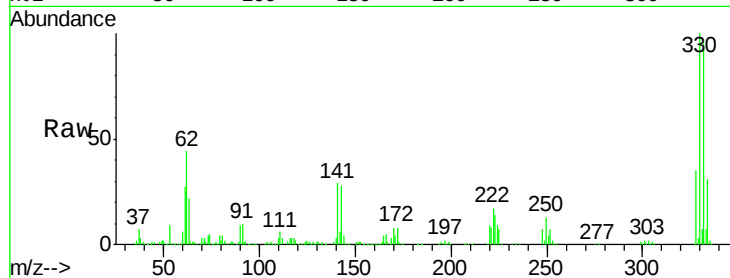


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

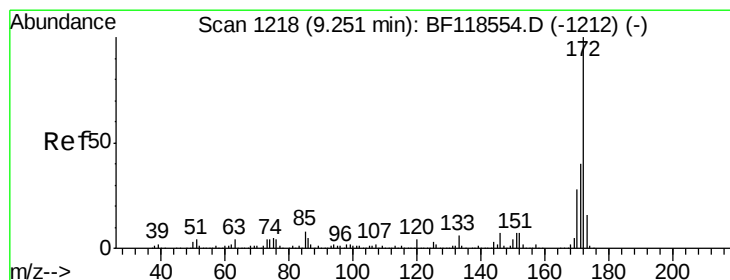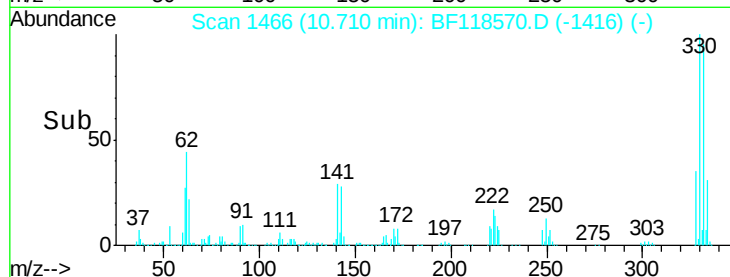
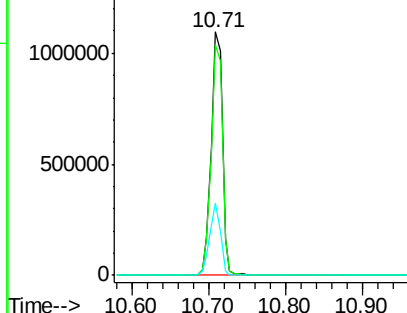



#45
 2-Fluorobiphenyl
 Concen: 103.212 ng
 RT: 9.25 min Scan# 1217
 Delta R.T. -0.01 min
 Lab File: BF118570.D
 Acq: 17 Jan 2020 20:55

Tgt Ion:172 Resp: 3648570
 Ion Ratio Lower Upper
 172 100
 171 39.8 32.4 48.6
 170 27.4 22.5 33.7

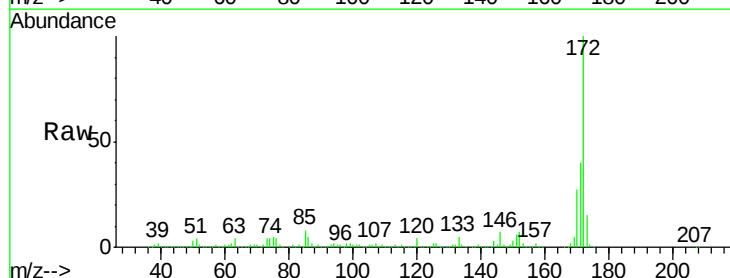

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



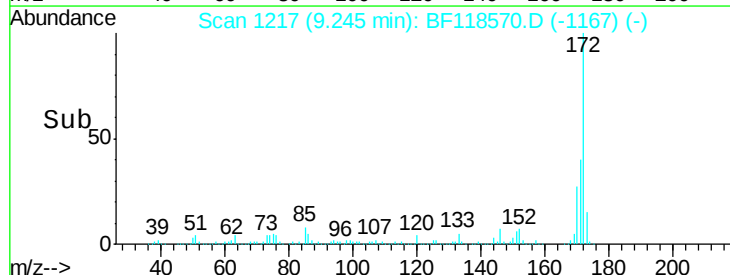
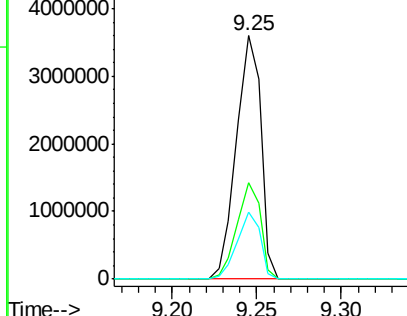


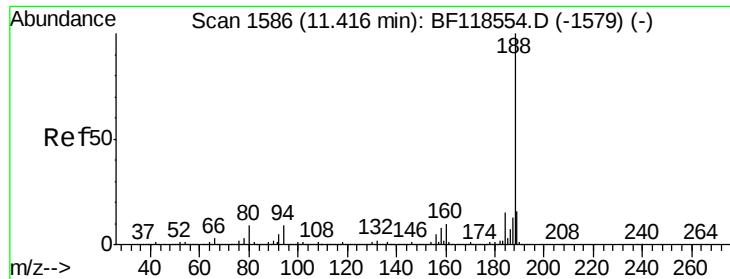

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.41 min Scan# 1585
Delta R.T. -0.01 min
Lab File: BF118570.D
Acq: 17 Jan 2020 20:55




Instrument :
BNA_F
ClientSampleId :
OK-02-011620


Tot Ion:188 Resp: 1186087
Ion Ratio Lower Upper
188 100
94 8.2 7.0 10.4
80 9.0 7.4 11.2

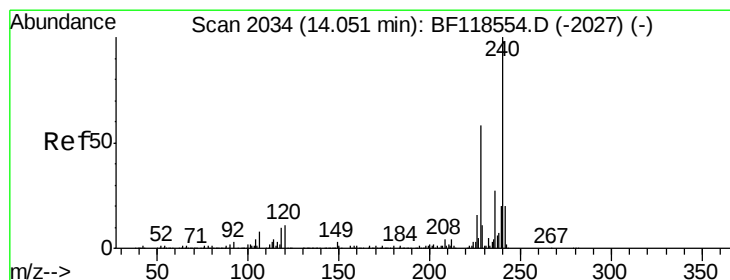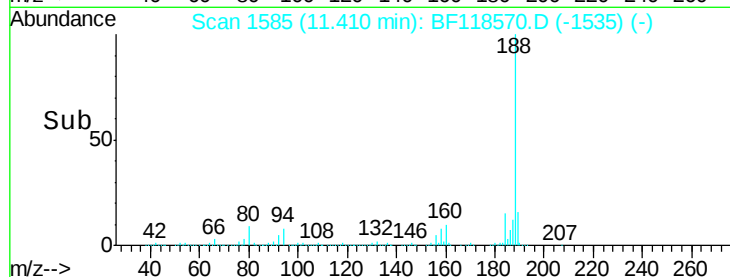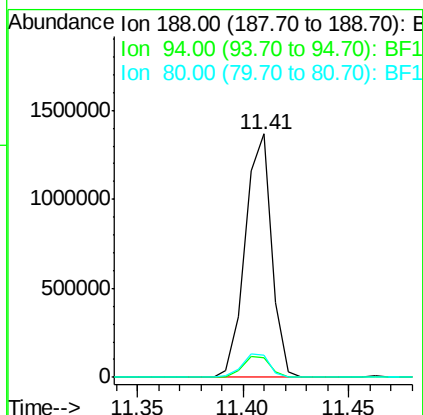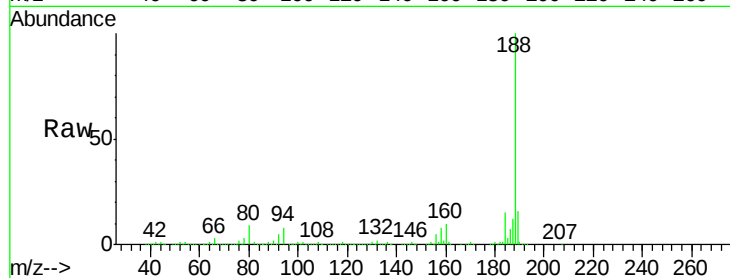

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.04 min Scan# 2032
Delta R.T. -0.01 min
Lab File: BF118570.D
Acq: 17 Jan 2020 20:55

Tgt Ion:240 Resp: 997506
Ion Ratio Lower Upper
240 100
120 11.2 8.7 13.1
236 26.3 21.8 32.8

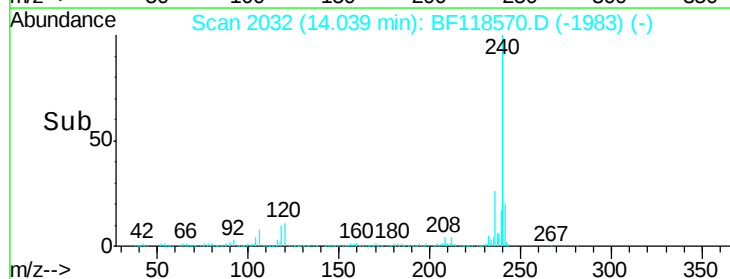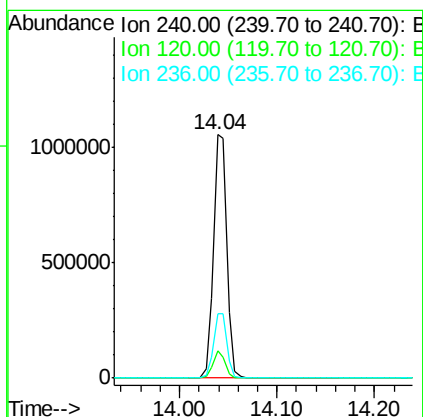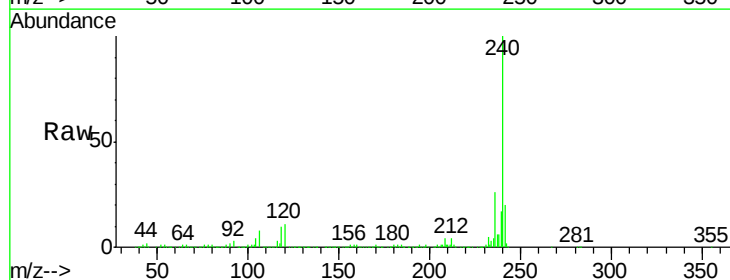

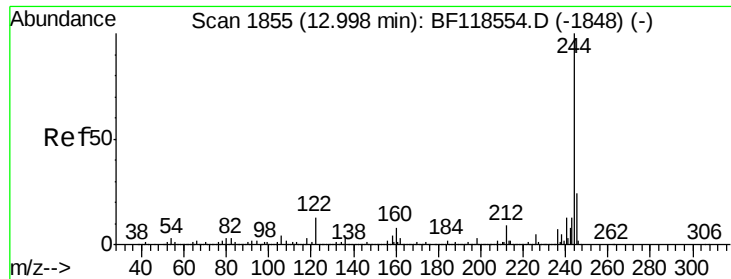

#79

Terphenyl-d14

Concen: 89.658 ng

RT: 13.00 min Scan# 1855

Delta R.T. -0.00 min

Lab File: BF118570.D

Acq: 17 Jan 2020 20:55

Instrument :

BNA_F

ClientSampleId :

OK-02-011620


Tot Ion:244 Resp: 4528481

Ion Ratio Lower Upper

244 100

212 8.7 7.0 10.4




122 12.4 10.4 15.6

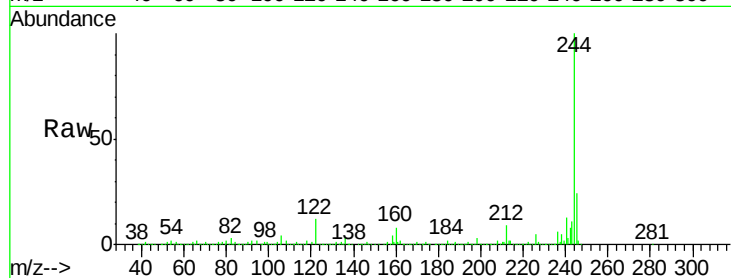

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

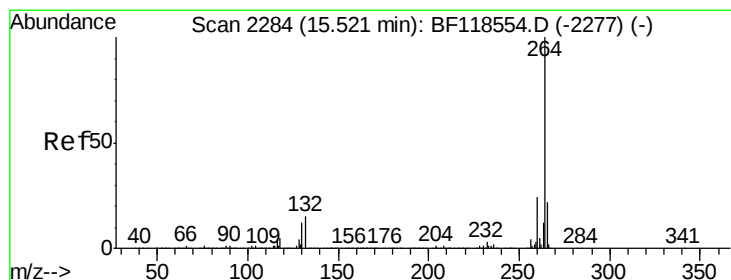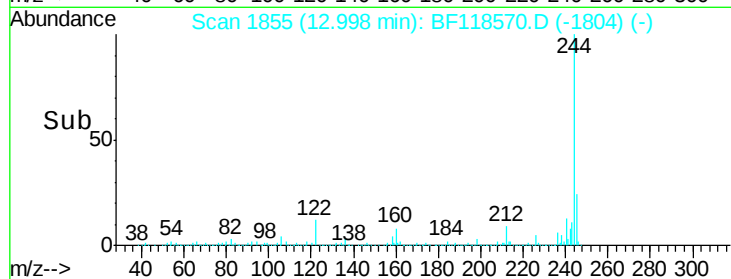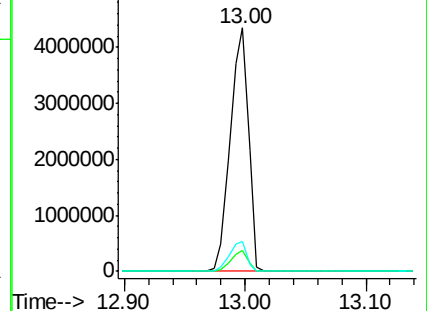

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.52 min Scan# 2283

Delta R.T. -0.01 min

Lab File: BF118570.D

Acq: 17 Jan 2020 20:55


Tgt Ion:264 Resp: 1019866

Ion Ratio Lower Upper

264 100

260 24.4 19.0 28.6

265 22.1 17.6 26.4

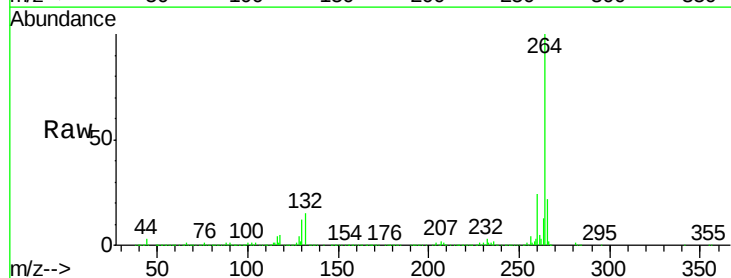

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

