


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF011720\
 Data File : BF118551.D
 Acq On : 17 Jan 2020 10:11
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 17 15:49:53 2020

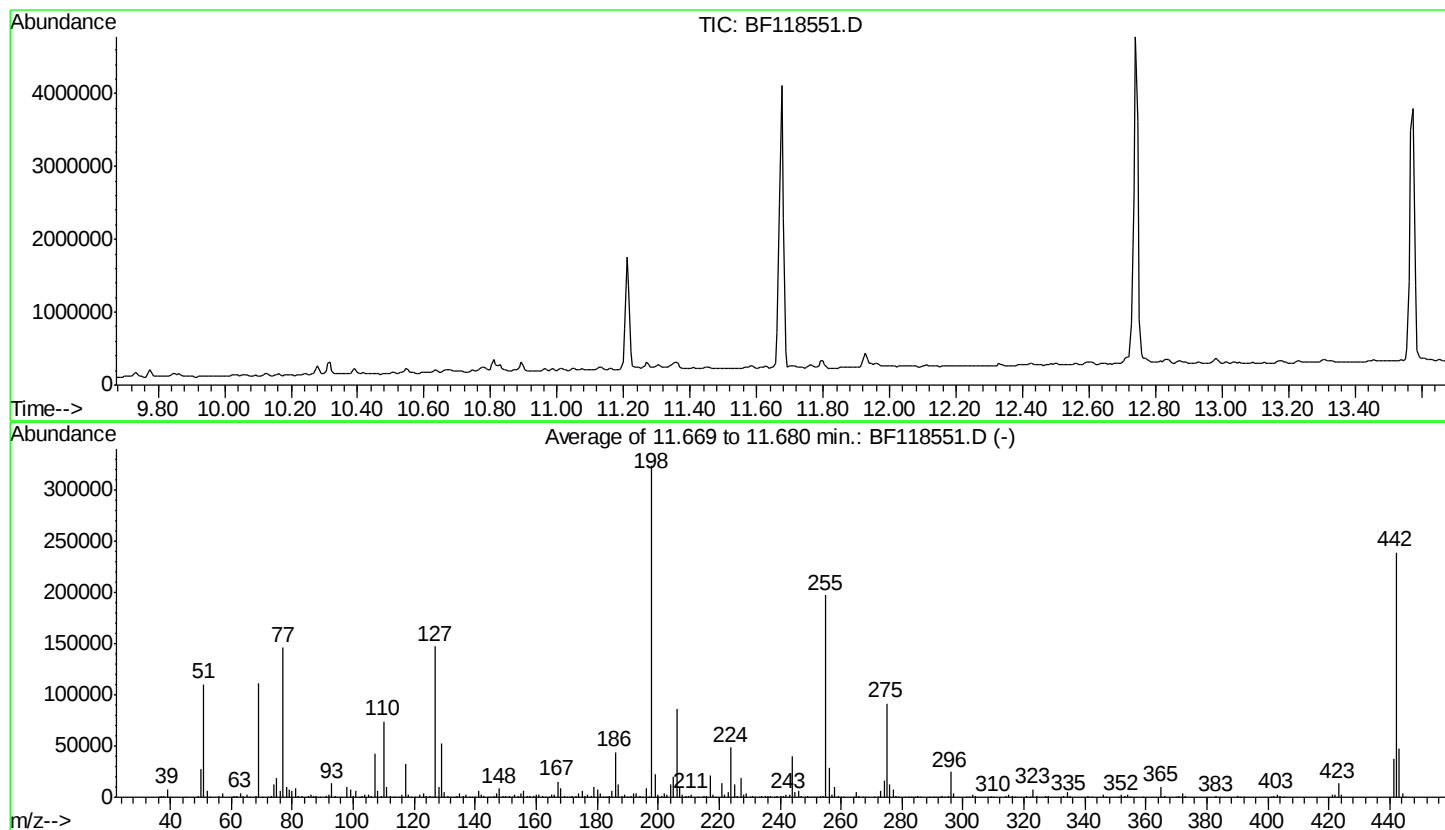

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1623

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	110498	PASS
68	69	0.00	2	1.5	1644	PASS
69	198	0.00	100	34.3	110925	PASS
70	69	0.00	2	0.1	72	PASS
127	198	10	80	45.5	147315	PASS
197	198	0.00	2	0.2	597	PASS
198	198	100	100	100.0	323712	PASS
199	198	5	9	6.9	22433	PASS
275	198	10	60	28.3	91544	PASS
365	198	1	100	3.2	10280	PASS
441	198	0.01	100	11.5	37349	PASS
442	198	50	100	73.9	239309	PASS
443	442	15	24	19.8	47426	PASS