


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF011720\
 Data File : BF118560.D
 Acq On : 17 Jan 2020 16:02
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 17 15:49:53 2020

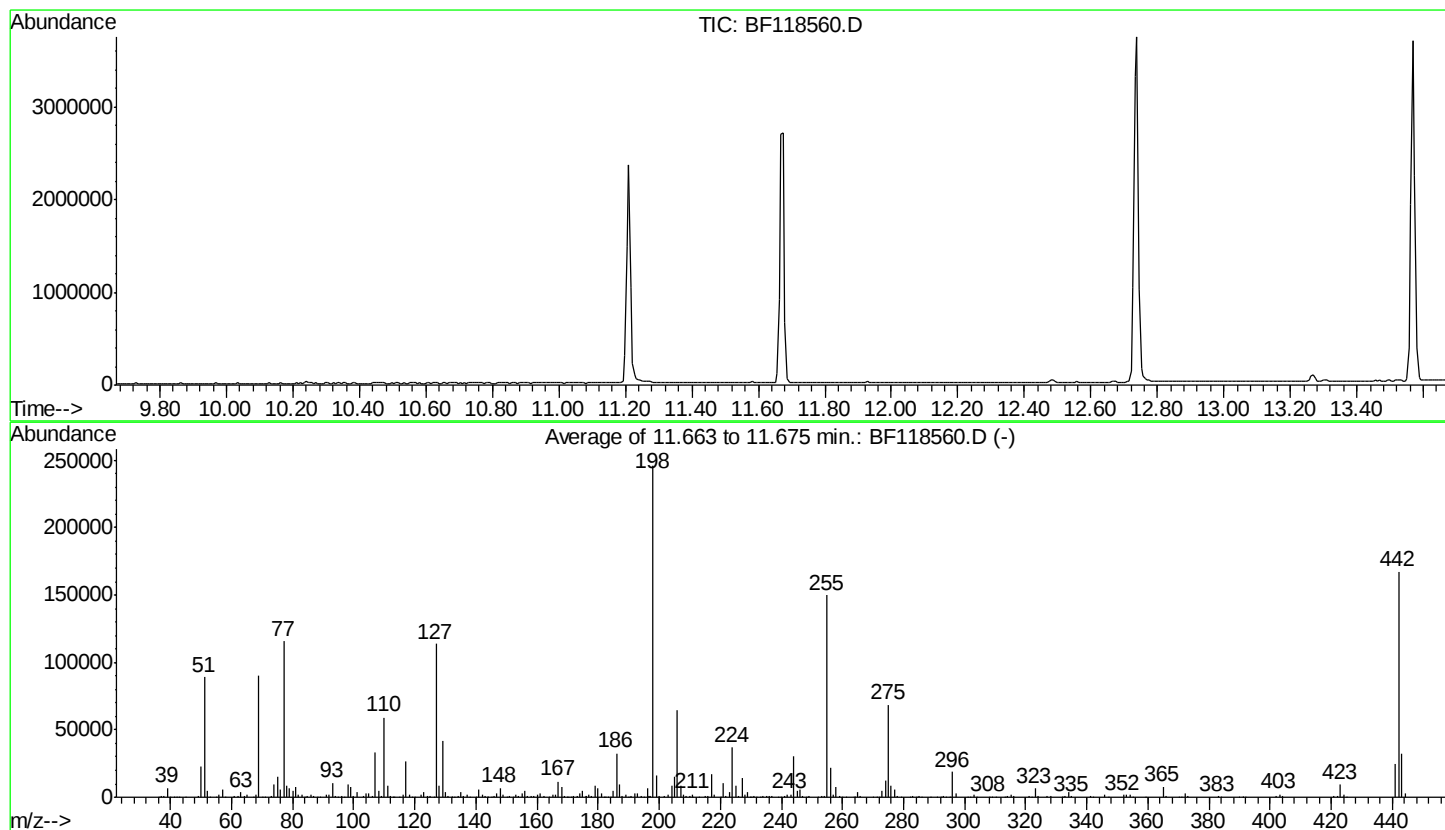

AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1623

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	88906	PASS
68	69	0.00	2	1.8	1589	PASS
69	198	0.00	100	36.5	89892	PASS
70	69	0.00	2	0.4	367	PASS
127	198	10	80	46.2	113754	PASS
197	198	0.00	2	0.3	673	PASS
198	198	100	100	100.0	246010	PASS
199	198	5	9	6.6	16345	PASS
275	198	10	60	28.0	68864	PASS
365	198	1	100	3.1	7737	PASS
441	198	0.01	100	10.1	24870	PASS
442	198	50	100	68.0	167248	PASS
443	442	15	24	19.3	32196	PASS