

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011823\
 Data File : BF132122.D
 Acq On : 18 Jan 2023 17:11
 Operator : CG\JU
 Sample : PB150317BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB150317BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF132122.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.366	423	430	443	rVB	1956502	3065576	36.76%	6.031%
2	5.737	487	493	496	rBV	4901706	6219598	74.59%	12.236%
3	6.713	652	659	662	rBV	4691048	6341638	76.05%	12.476%
4	7.095	720	724	727	rBV	1642899	1300519	15.60%	2.559%
5	7.660	813	820	823	rBV	3568230	4361882	52.31%	8.581%
6	8.383	937	943	946	rBV	1978622	1683449	20.19%	3.312%
7	9.460	1119	1126	1130	rBV	6461948	7212727	86.50%	14.190%
8	10.148	1236	1243	1246	rBV	2418147	2013476	24.15%	3.961%
9	10.942	1373	1378	1381	rBV	5137869	5366747	64.36%	10.558%
10	11.648	1494	1498	1501	rVB	2521093	2258970	27.09%	4.444%
11	13.248	1764	1770	1773	rBV	7443902	8338683	100.00%	16.405%
12	14.307	1946	1950	1954	rBV	1824339	1642803	19.70%	3.232%
13	15.906	2216	2222	2235	rBV	767566	1024808	12.29%	2.016%




Sum of corrected areas: 50830876

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011823\
Data File : BF132122.D
Acq On : 18 Jan 2023 17:11
Operator : CG\JU
Sample : PB150317BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB150317BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

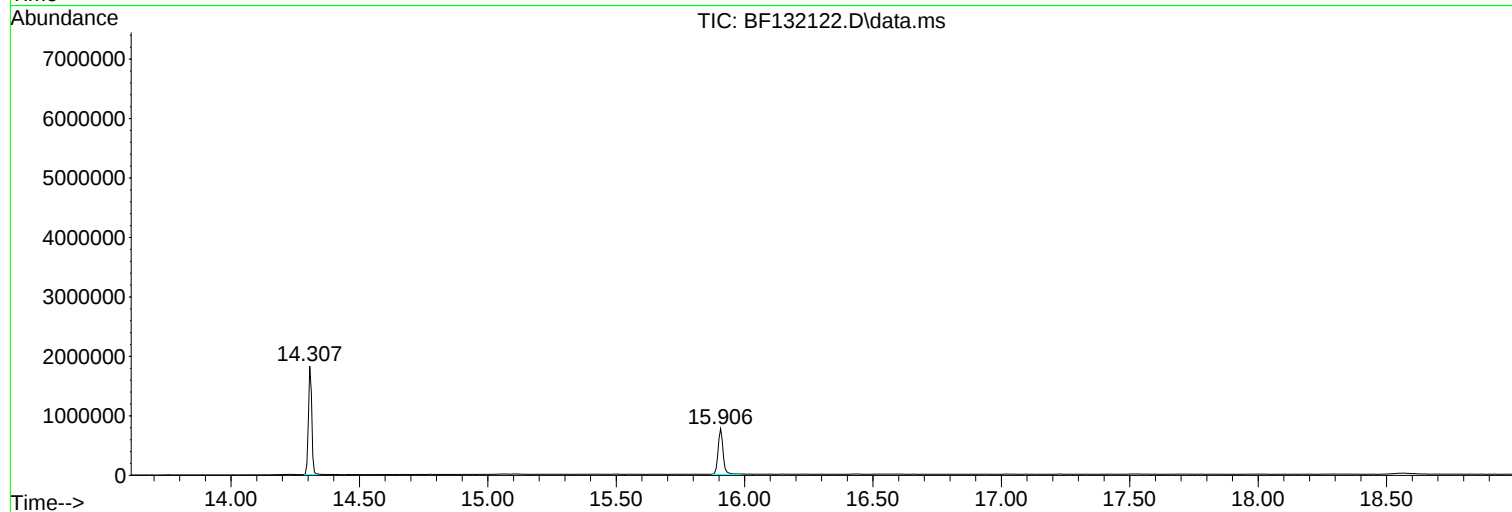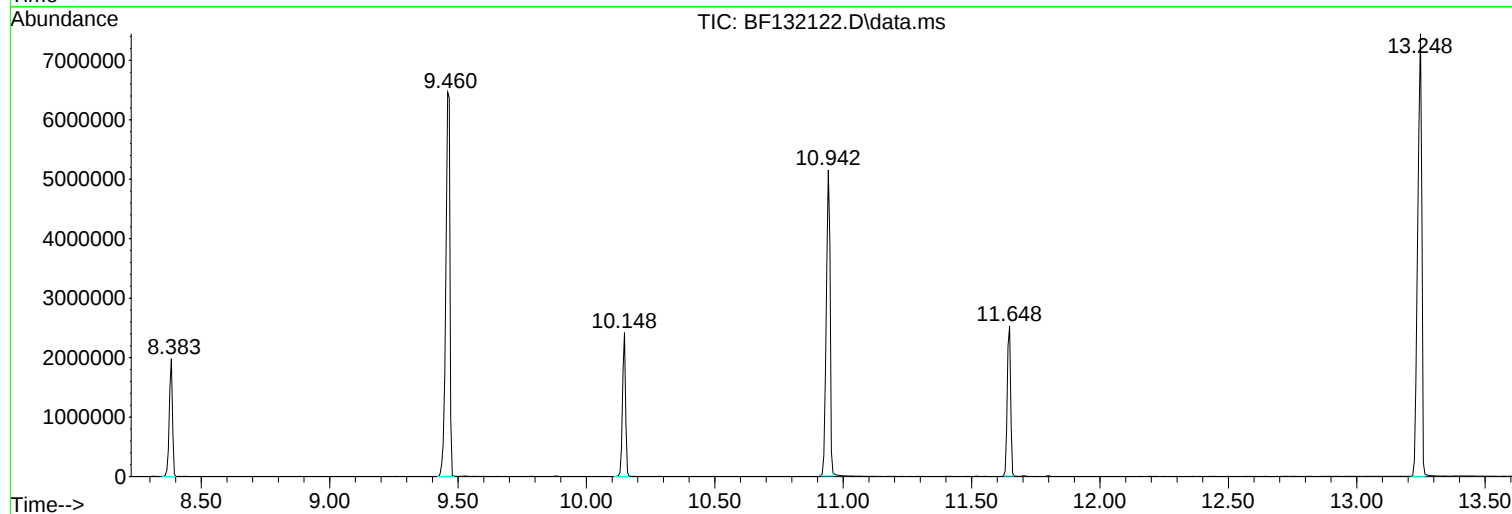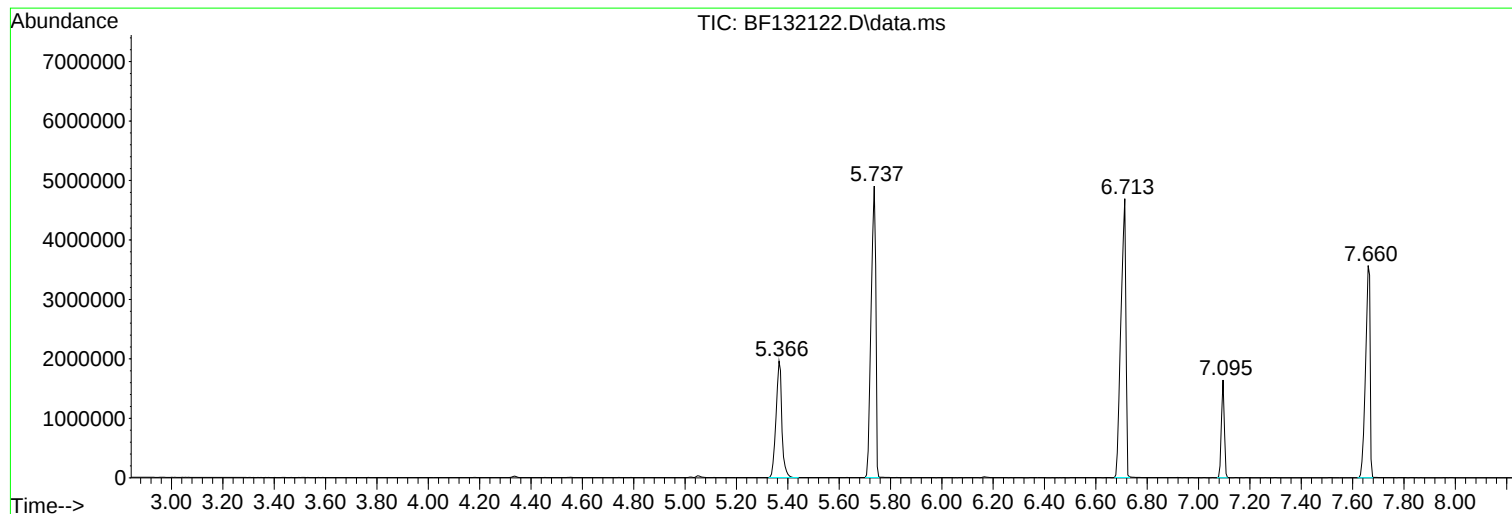

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011823\
Data File : BF132122.D
Acq On : 18 Jan 2023 17:11
Operator : CG\JU
Sample : PB150317BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB150317BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.366	47.14 ng	3065580	1,4-Dichlorobenzene-d4	7.095

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59		
2	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	27		
3	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23		
4	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	17		
5	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	12		

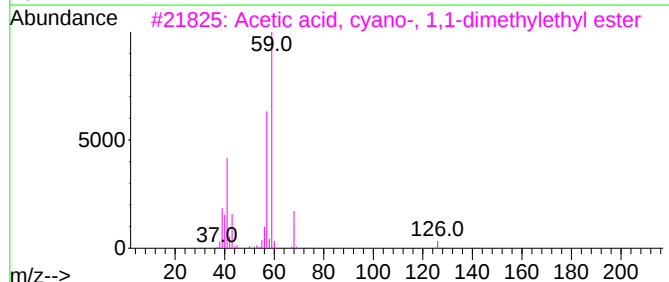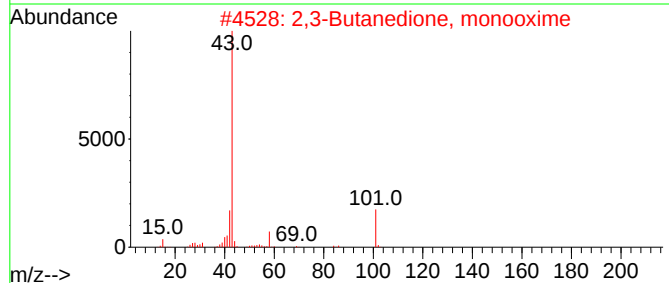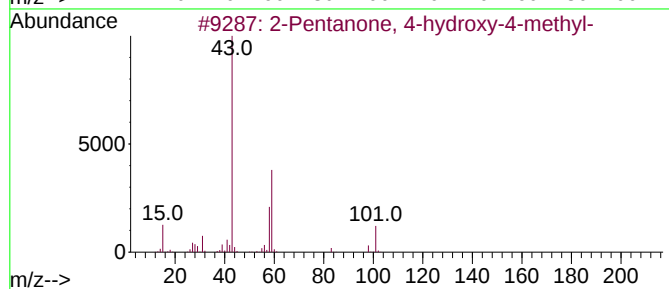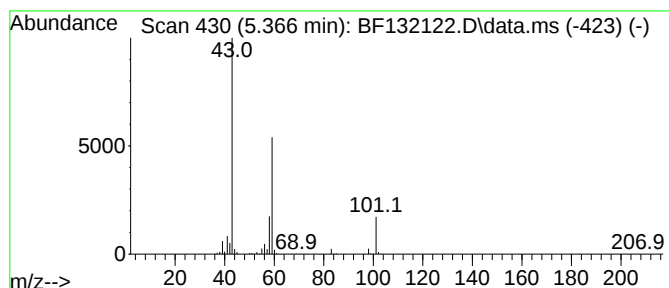

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011823\
Data File : BF132122.D
Acq On : 18 Jan 2023 17:11
Operator : CG\JU
Sample : PB150317BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB150317BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.366	47.1	ng	3065580	1	7.095	1300520	20.0