


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011823\
Data File : BF132109.D
Acq On : 18 Jan 2023 09:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 19 00:42:19 2023

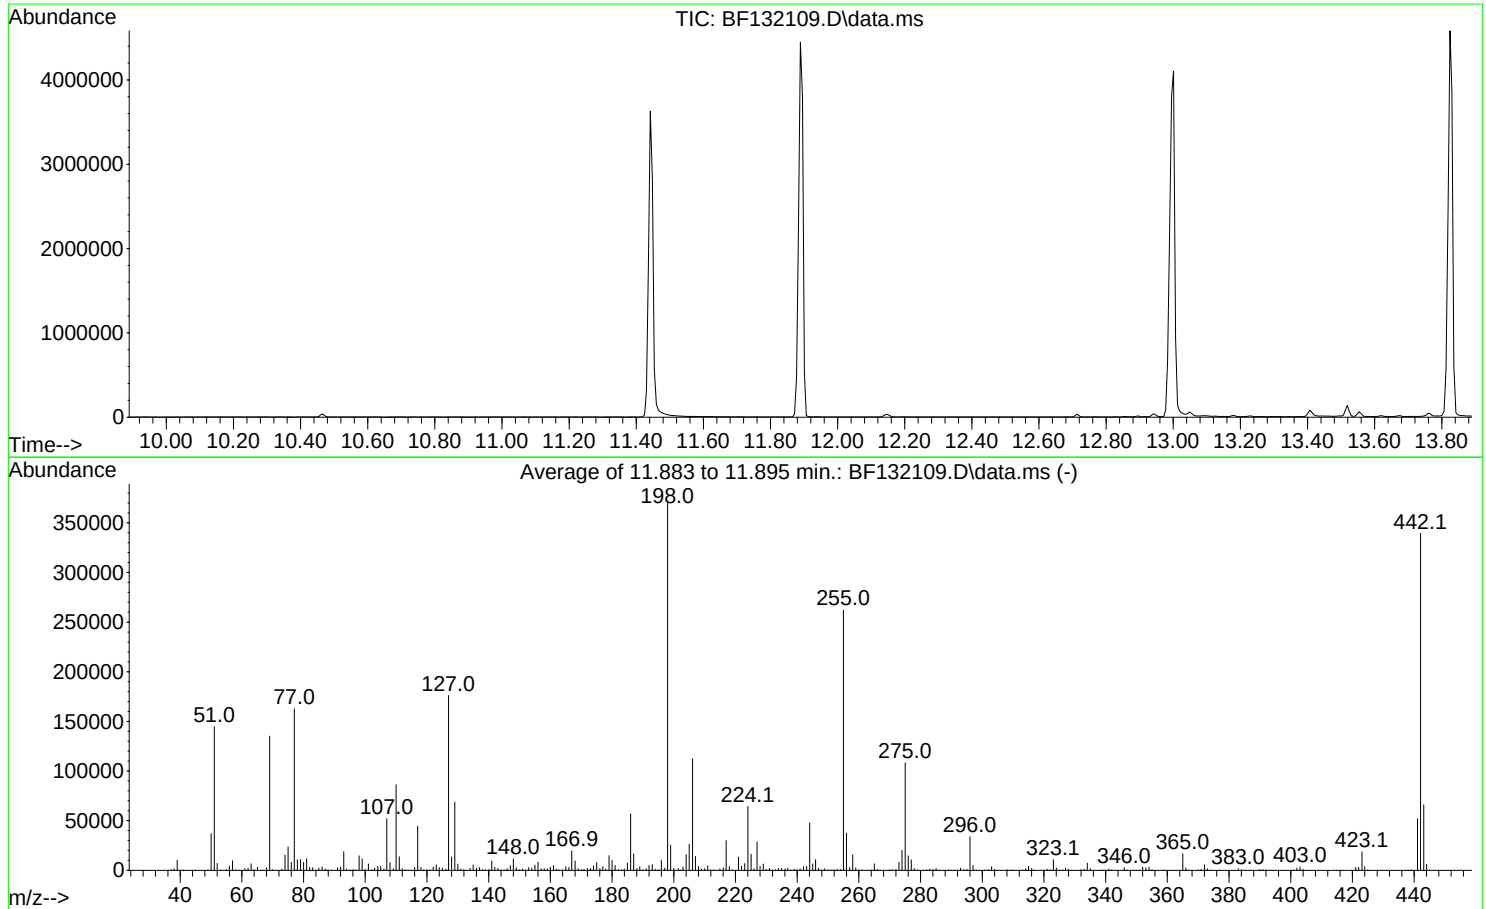




AutoFind: Scans 1538, 1539, 1540; Background Corrected with Scan 1532

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	144744	PASS
68	69	0.00	2	1.9	2579	PASS
69	198	0.00	100	36.5	135088	PASS
70	69	0.00	2	0.5	739	PASS
127	198	10	80	47.5	176107	PASS
197	198	0.00	2	0.6	2115	PASS
198	198	100	100	100.0	370581	PASS
199	198	5	9	6.8	25259	PASS
275	198	10	60	29.2	108208	PASS
365	198	1	100	4.5	16733	PASS
441	198	0.01	100	14.0	52000	PASS
442	442	50	100	100.0	339315	PASS
443	442	15	24	19.4	65984	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011823\
 Data File : BF132109.D
 Acq On : 18 Jan 2023 09:30
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jan 19 07:34:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 19 00:42:19 2023
 Response via : Initial Calibration

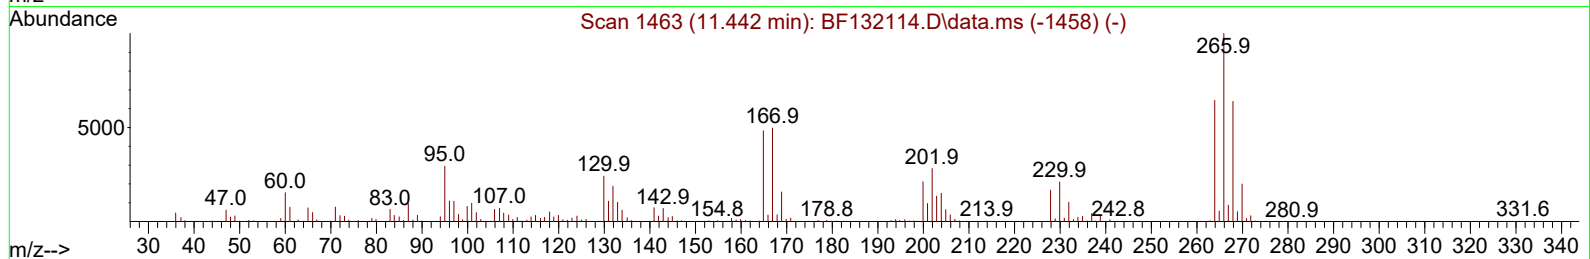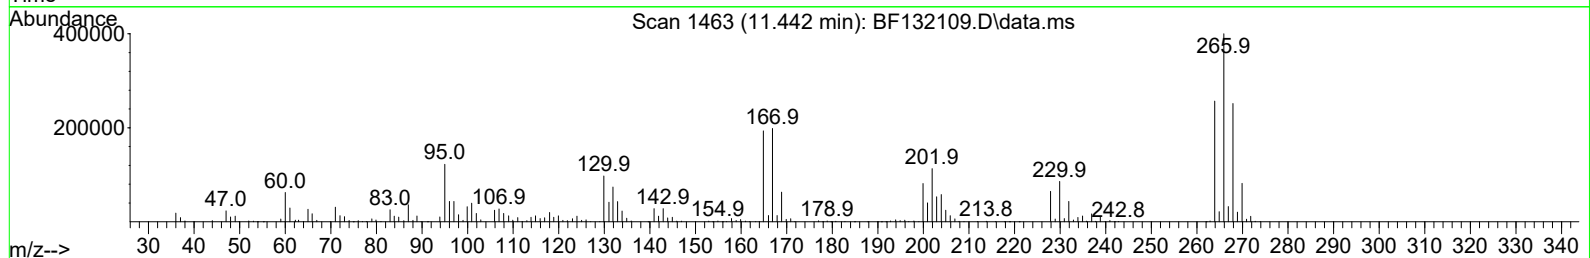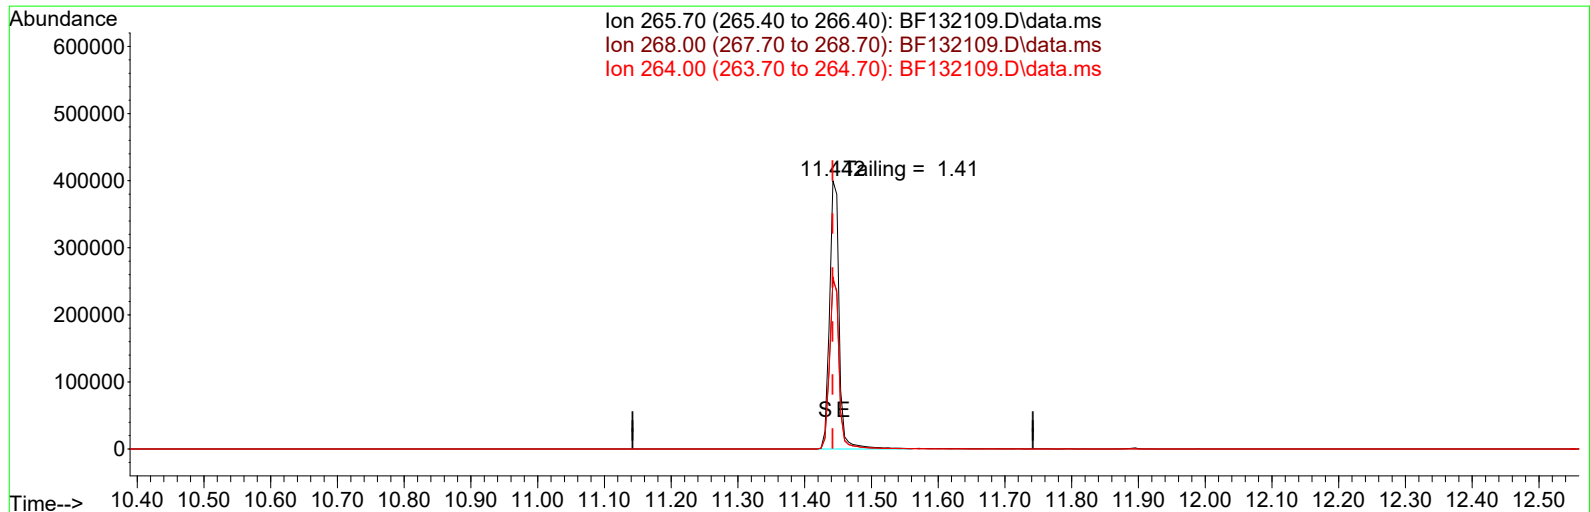

TIC: BF132109.D\data.ms

(70) Pentachlorophenol (C)

11.442min (+ 0.000) 53761.67 ng




response 402290

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.95
264.00	64.50	64.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011823\
Data File : BF132109.D
Acq On : 18 Jan 2023 09:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 19 07:34:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 00:42:19 2023
Response via : Initial Calibration

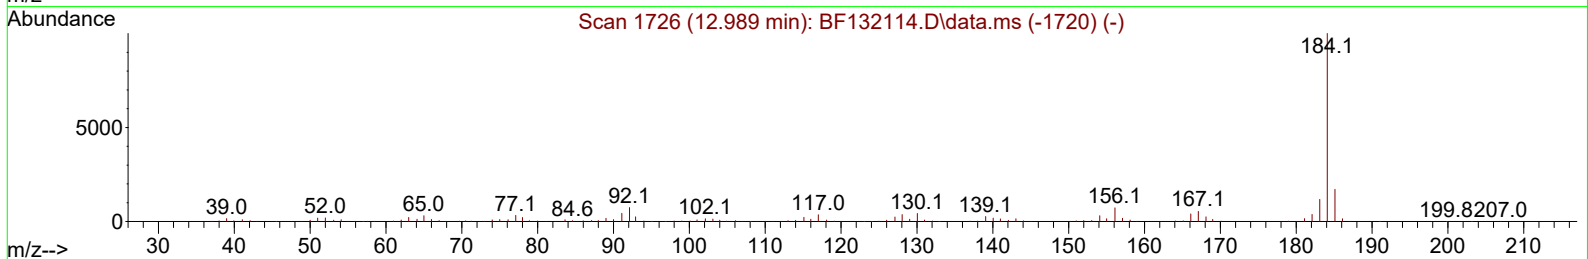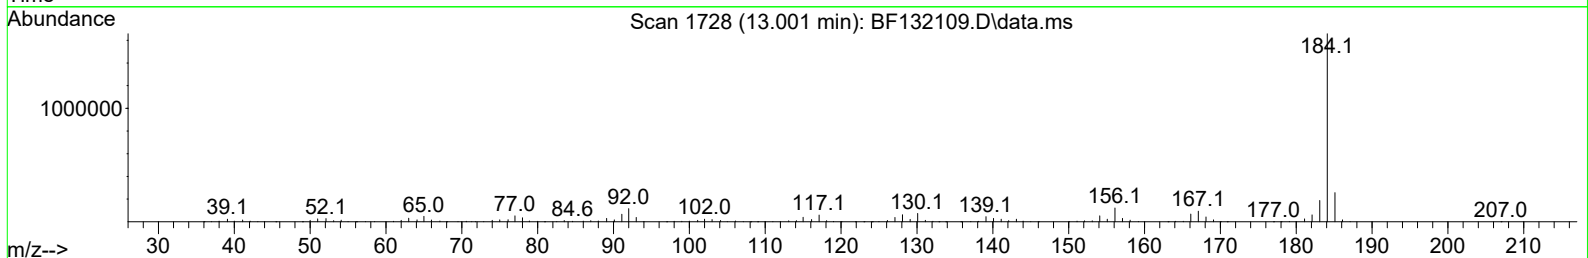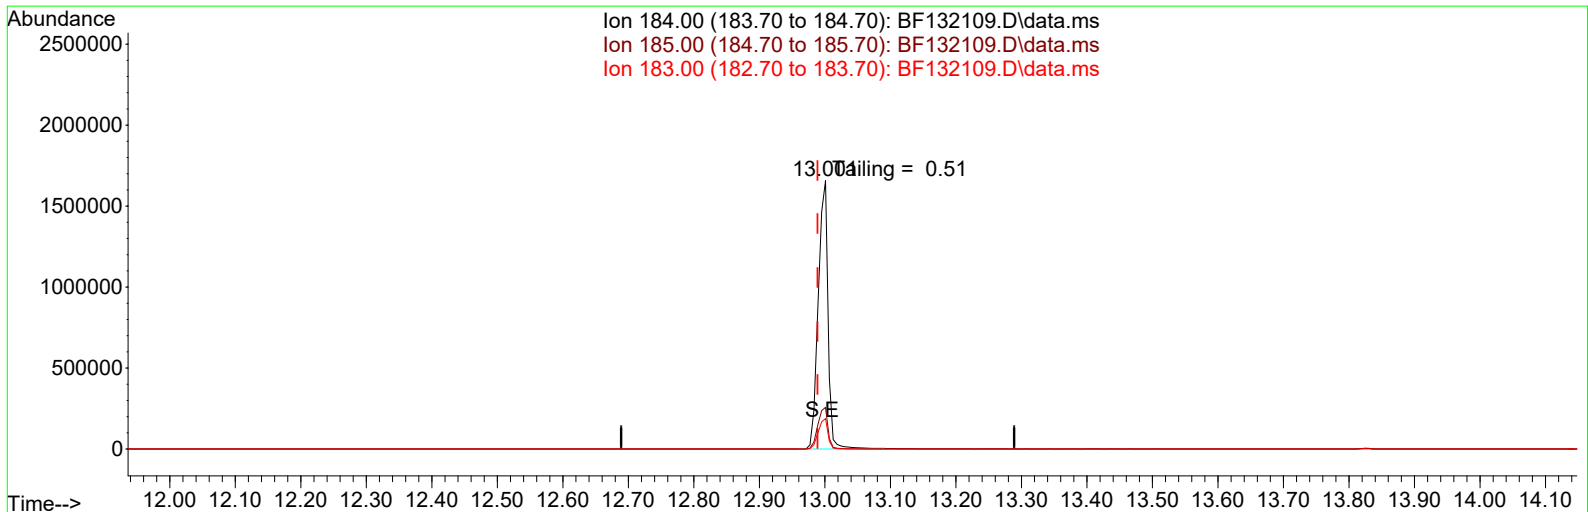

TIC: BF132109.D\data.ms

(77) Benzidine

13.001min (+ 0.012) 80715.69 ng

response 1732290

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	17.10	15.49
183.00	11.70	11.33
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/18/2023	BNA_F	<u>BF132109.D</u>
Compound Name	Response	Retention Time
DDT	790278	13.824
DDD	27051	13.519
DDE	1796	13.177
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28847	819125	3.52

Instrument :
BNA_F
ClientSampleId :
DFTPP