
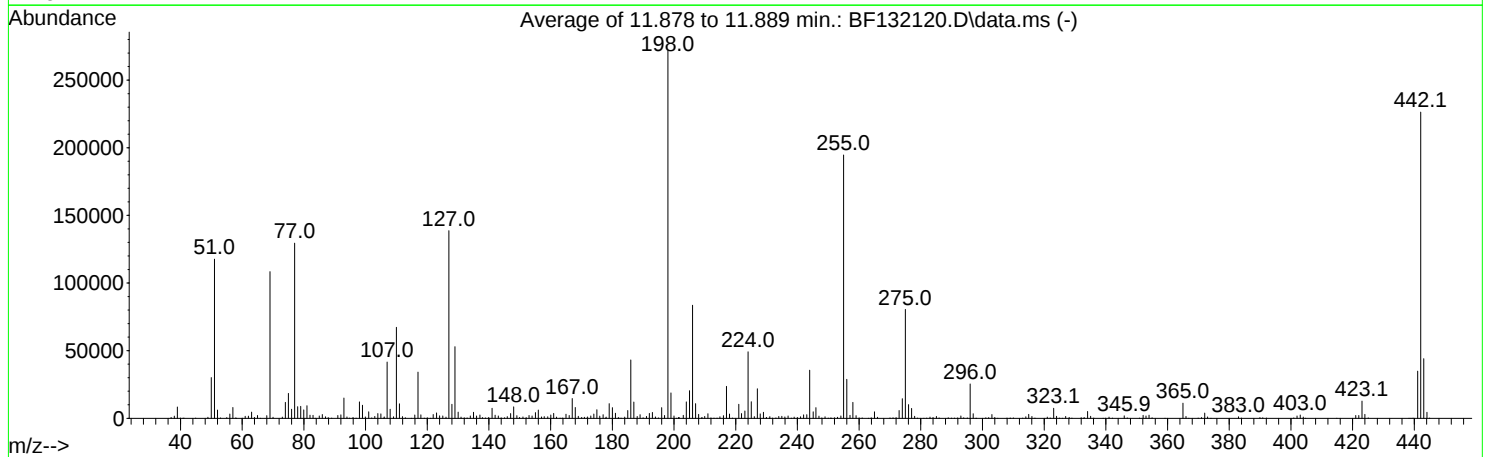


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011823\
Data File : BF132120.D
Acq On : 18 Jan 2023 16:03
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 19 00:42:19 2023

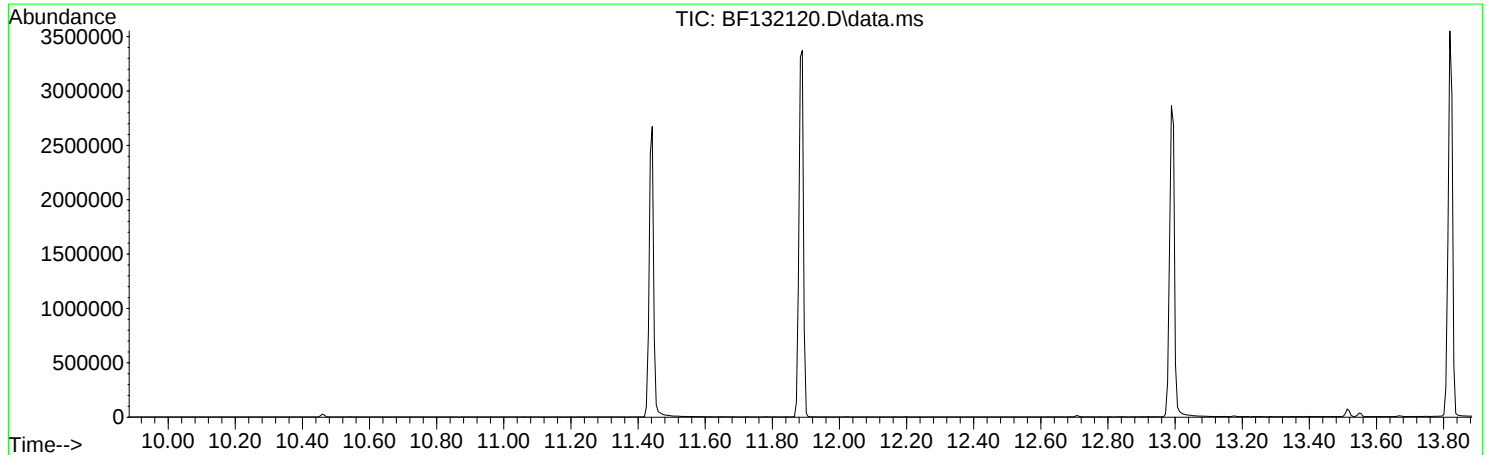




AutoFind: Scans 1537, 1538, 1539; Background Corrected with Scan 1532

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.3	117675	PASS
68	69	0.00	2	1.8	1990	PASS
69	198	0.00	100	39.8	108360	PASS
70	69	0.00	2	0.7	762	PASS
127	198	10	80	51.0	138691	PASS
197	198	0.00	2	0.8	2113	PASS
198	198	100	100	100.0	271939	PASS
199	198	5	9	6.9	18750	PASS
275	198	10	60	29.6	80467	PASS
365	198	1	100	4.1	11232	PASS
441	198	0.01	100	12.8	34868	PASS
442	442	50	100	100.0	226323	PASS
443	442	15	24	19.5	44057	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011823\
Data File : BF132120.D
Acq On : 18 Jan 2023 16:03
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 19 08:57:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 00:42:19 2023
Response via : Initial Calibration

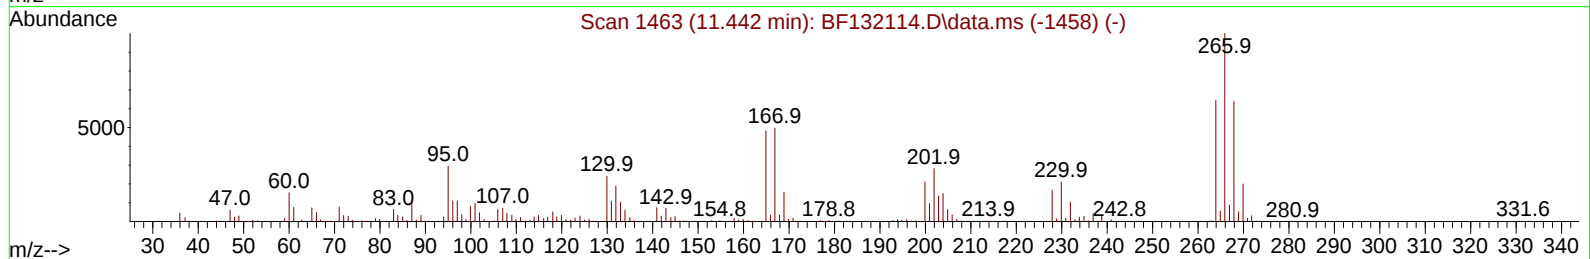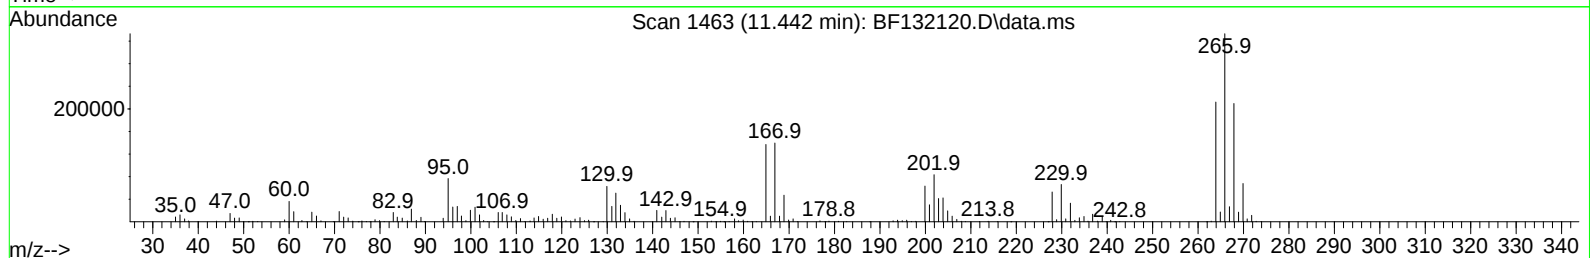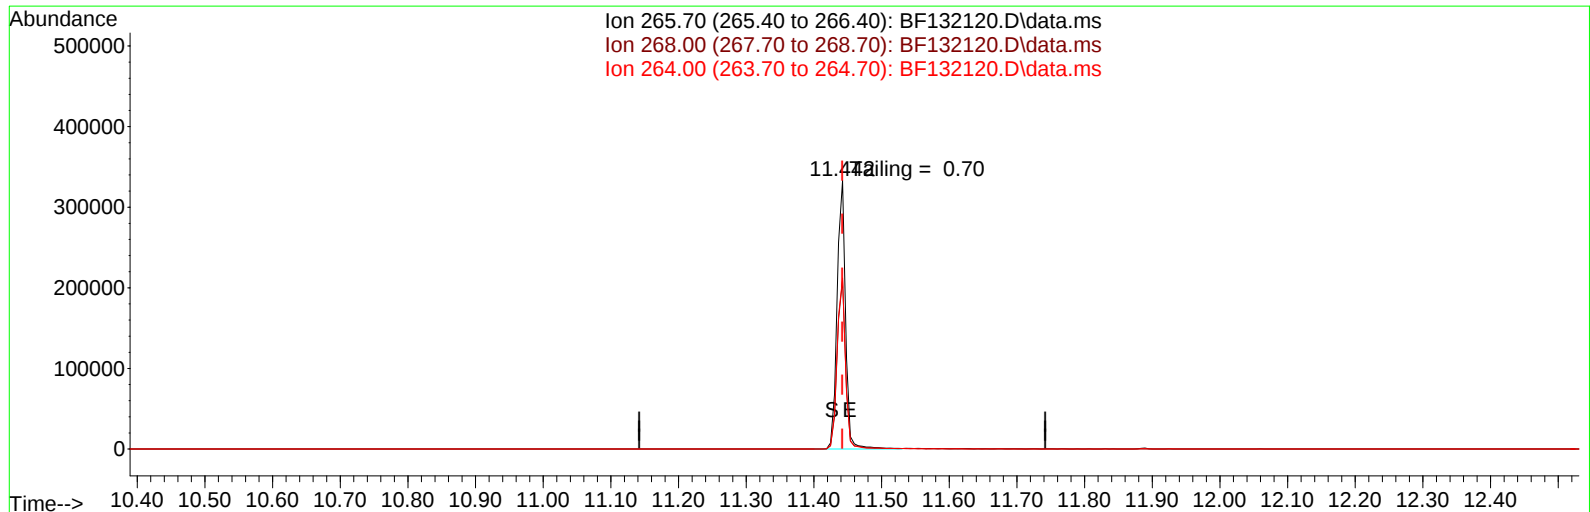

TIC: BF132120.D\data.ms

(70) Pentachlorophenol (C)

11.442min (+ 0.000) 670829.63 ng




response 289700

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.93
264.00	64.50	63.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011823\
Data File : BF132120.D
Acq On : 18 Jan 2023 16:03
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 19 08:57:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 00:42:19 2023
Response via : Initial Calibration

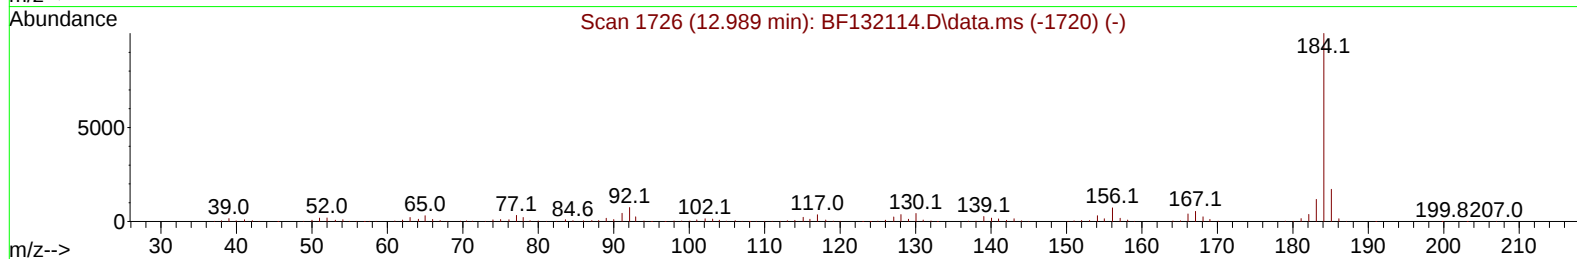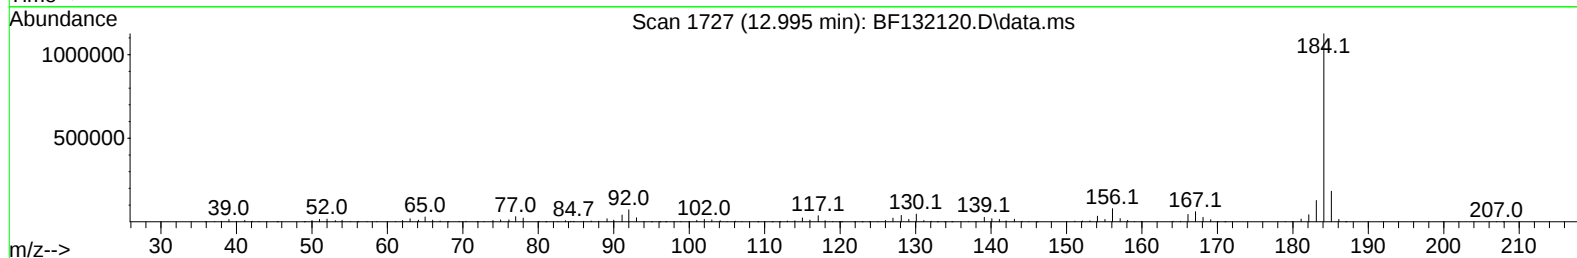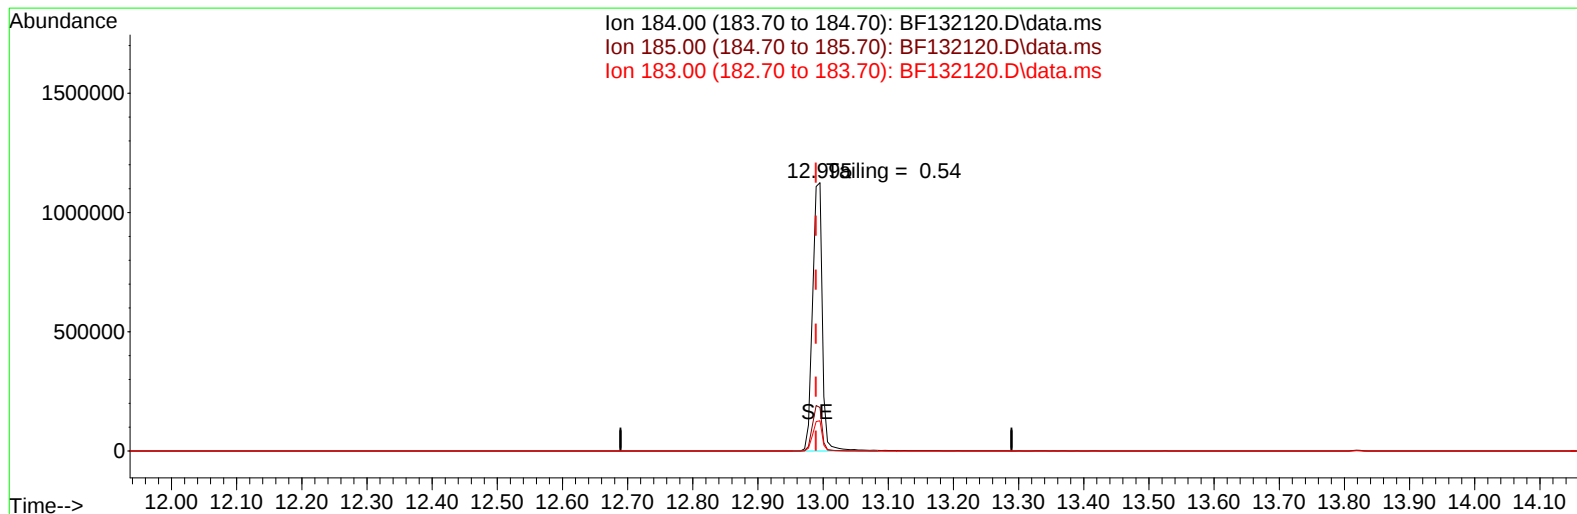

TIC: BF132120.D\data.ms

(77) Benzidine

12.995min (+ 0.006) 0.00 ng

response 1175467

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	17.10	16.25
183.00	11.70	11.31
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/18/2023	BNA_F	<u>BF132120.D</u>
Compound Name	Response	Retention Time
DDT	594023	13.819
DDD	16743	13.513
DDE	955	13.172
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17698	611721	2.89

Instrument :
BNA_F
ClientSampleId :
DFTPP