
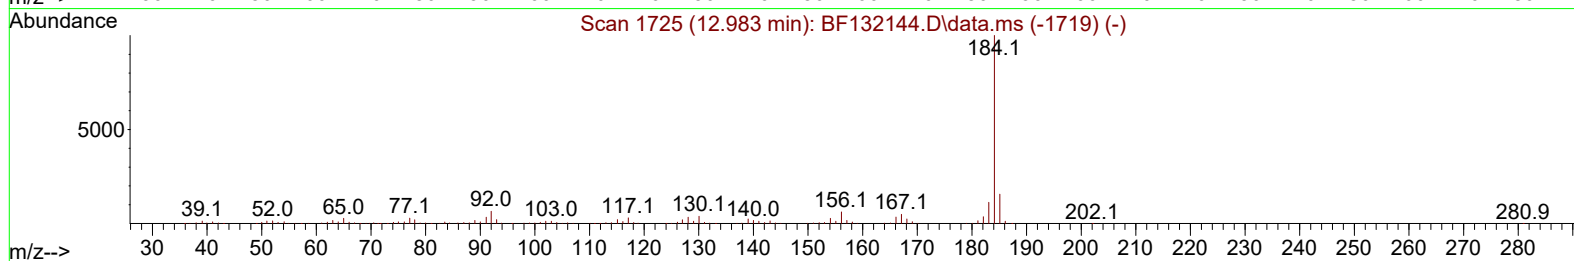
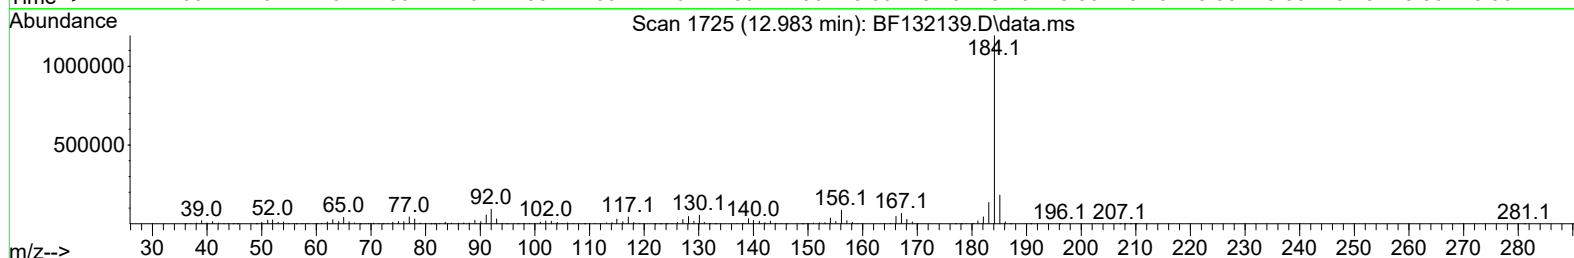


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011923\
 Data File : BF132139.D
 Acq On : 19 Jan 2023 10:46
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 20 05:07:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 20 00:50:42 2023
 Response via : Initial Calibration

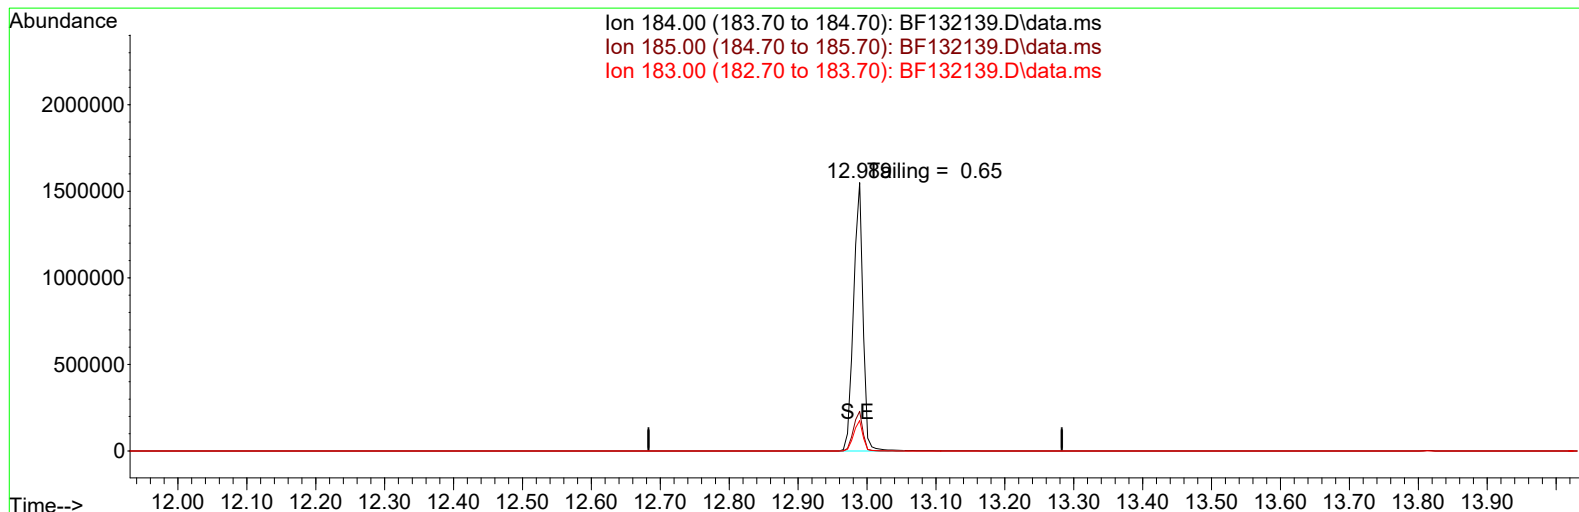

TIC: BF132139.D\data.ms

(77) Benzidine




12.983min (-12.983) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	15.60	0.00#
183.00	11.20	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011923\
 Data File : BF132139.D
 Acq On : 19 Jan 2023 10:46
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 20 05:07:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 20 00:50:42 2023
 Response via : Initial Calibration

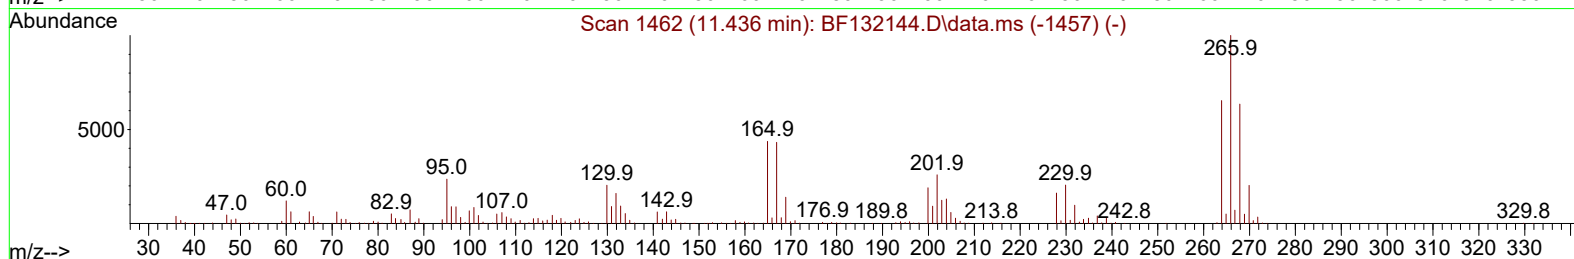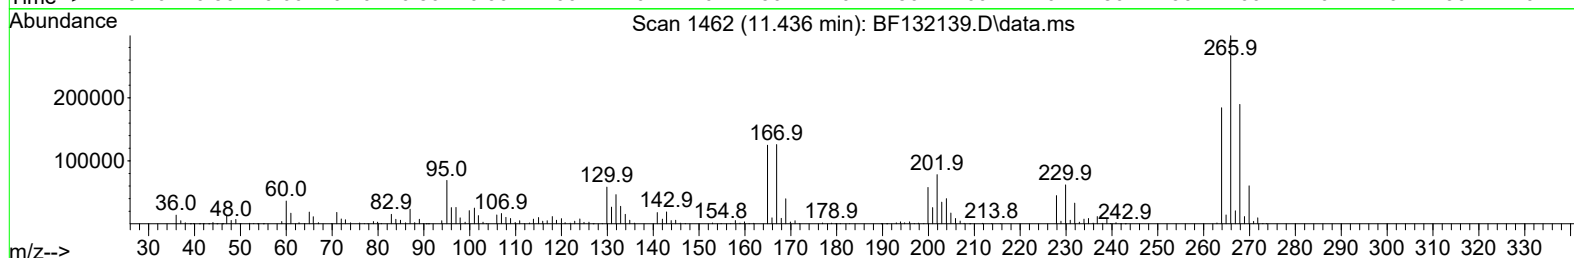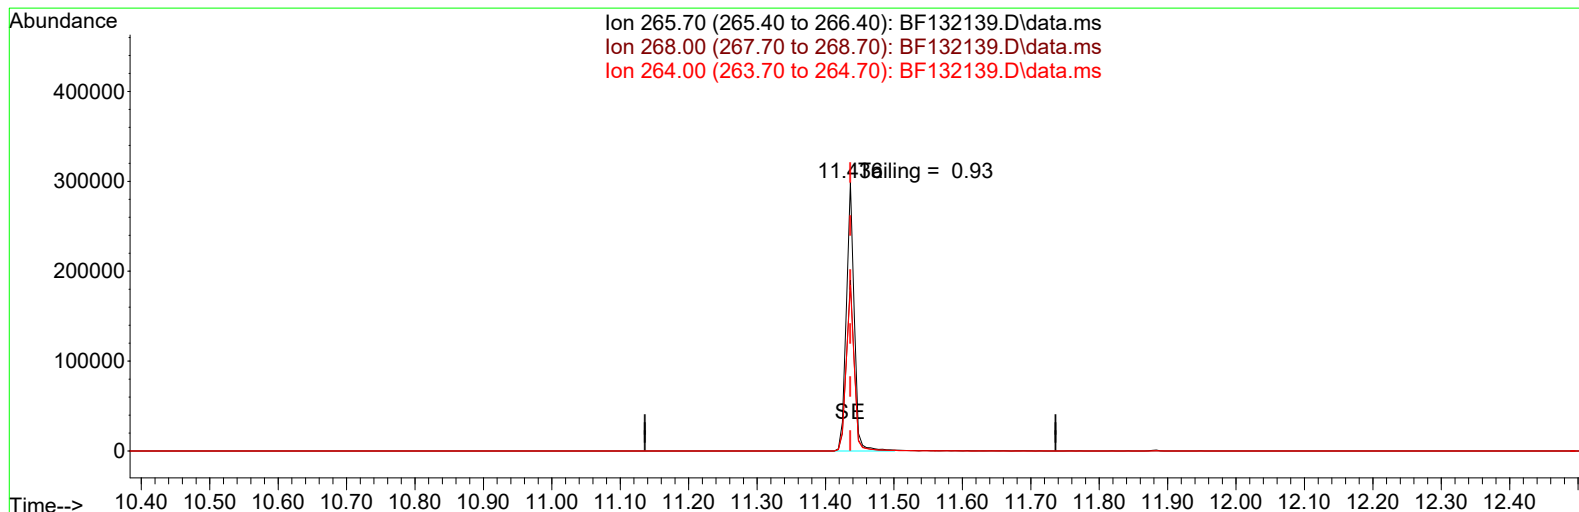

TIC: BF132139.D\data.ms

(70) Pentachlorophenol (C)

11.436min (+ 0.000) 469730.41 ng

response 241341

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	63.47
264.00	65.40	61.76
0.00	0.00	0.00