

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012422\
 Data File : BF126633.D
 Acq On : 24 Jan 2022 12:38
 Operator : CG/JU
 Sample : PB142183BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB142183BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126633.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.381	39	50	55	rBV	135081	189742	3.40%	0.553%
2	4.140	344	349	354	rVB	153326	183046	3.28%	0.534%
3	5.592	590	596	599	rBV	4223932	4670592	83.70%	13.623%
4	6.581	757	764	767	rBV	4195997	4779250	85.65%	13.940%
5	6.963	825	829	832	rBV	1124480	906701	16.25%	2.645%
6	7.528	919	925	928	rBV	2879539	3257995	58.39%	9.503%
7	8.245	1042	1047	1050	rBV	1279892	1205341	21.60%	3.516%
8	9.322	1224	1230	1233	rBV	4726525	5219098	93.53%	15.223%
9	10.004	1340	1346	1350	rBV	1612795	1385590	24.83%	4.041%
10	10.798	1474	1481	1484	rBV	3596660	3333006	59.73%	9.721%
11	11.498	1596	1600	1603	rBV	1751372	1416162	25.38%	4.131%
12	13.092	1866	1871	1874	rBV	5446522	5579880	100.00%	16.275%
13	14.145	2046	2050	2054	rBV	1289677	1215503	21.78%	3.545%
14	15.680	2305	2311	2315	rBV	753216	943219	16.90%	2.751%




Sum of corrected areas: 34285125

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012422\
Data File : BF126633.D
Acq On : 24 Jan 2022 12:38
Operator : CG/JU
Sample : PB142183BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142183BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

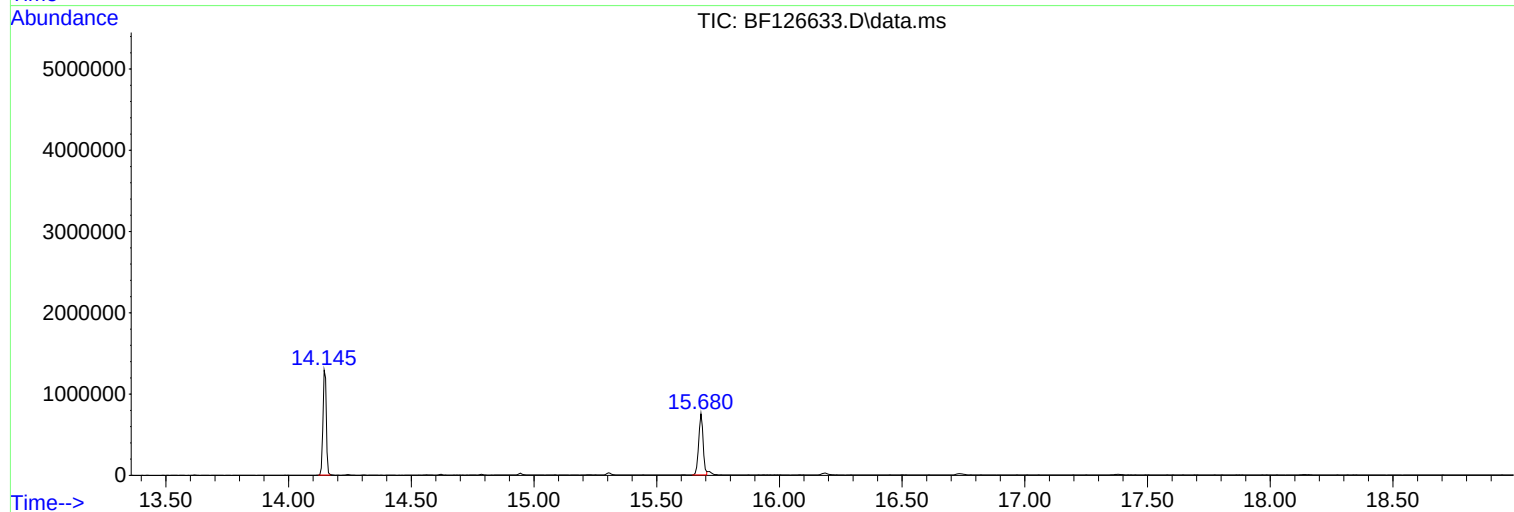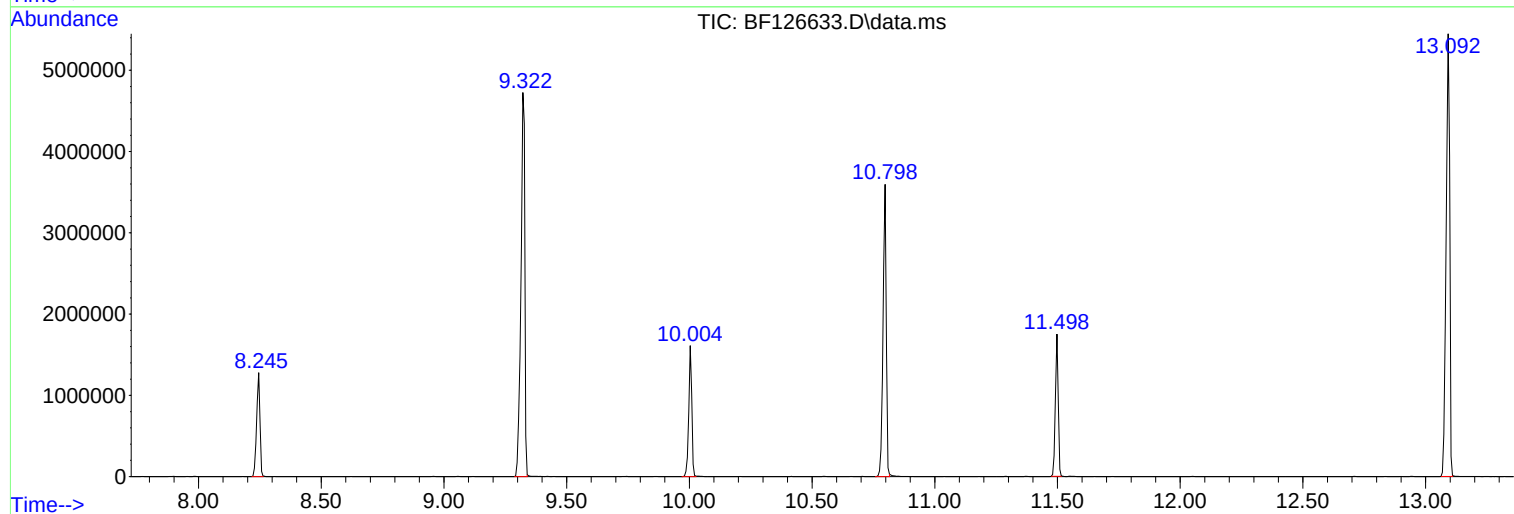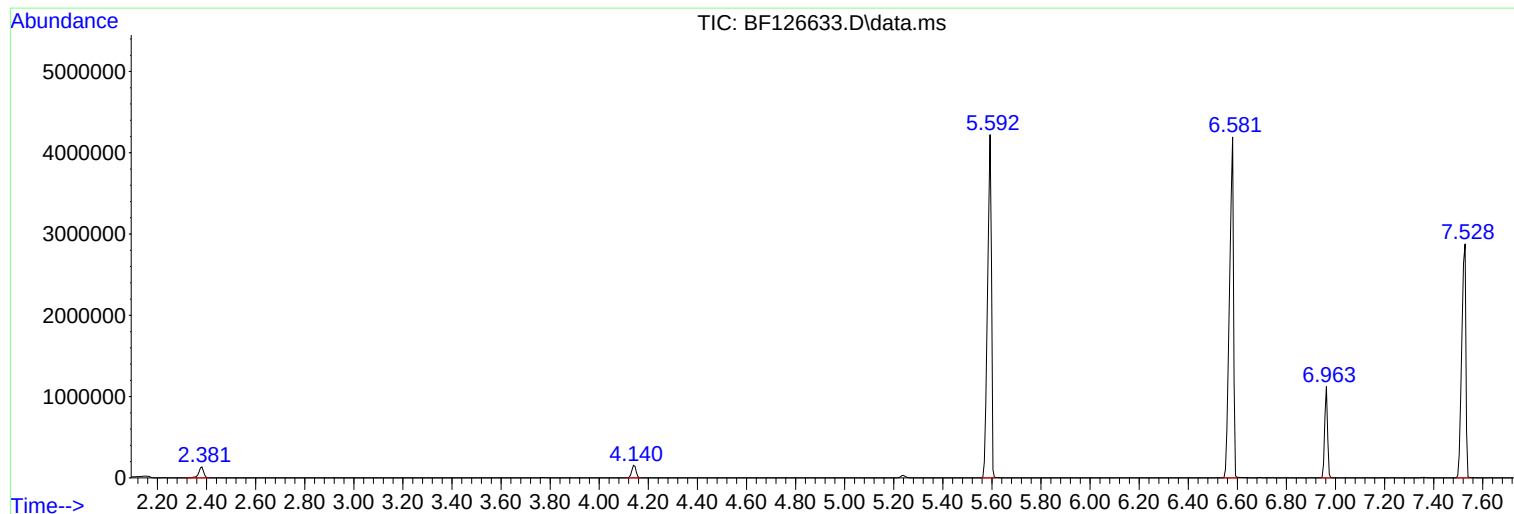

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012422\
Data File : BF126633.D
Acq On : 24 Jan 2022 12:38
Operator : CG/JU
Sample : PB142183BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142183BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.381	4.19 ng	189742	1,4-Dichlorobenzene-d4	6.963

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	43
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
4			N-Ethylformamide	73	C3H7NO	000627-45-2	9
5			Borane, dimethoxy-	74	C2H7BO2	004542-61-4	9

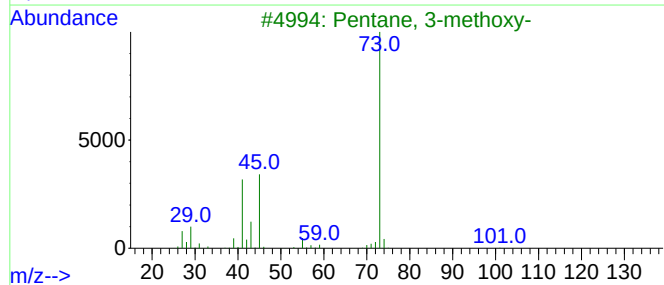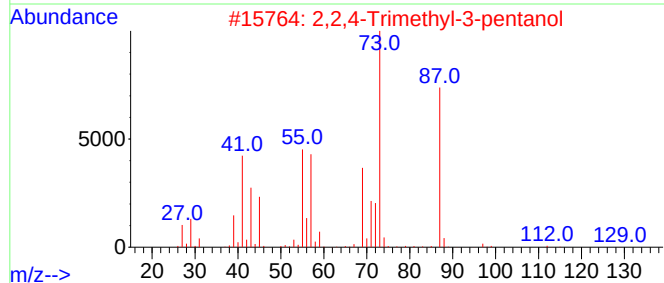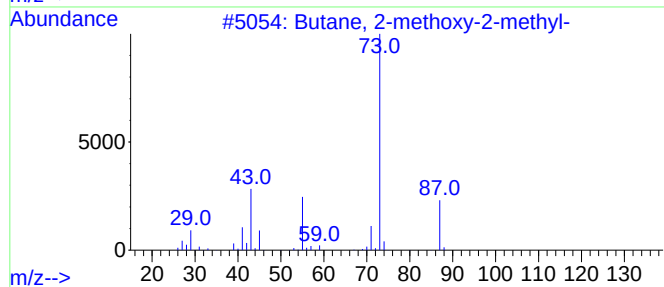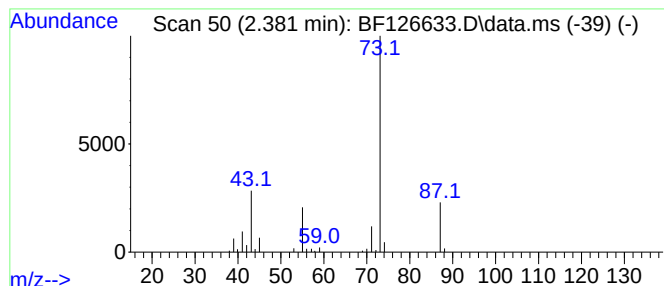

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012422\
Data File : BF126633.D
Acq On : 24 Jan 2022 12:38
Operator : CG/JU
Sample : PB142183BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142183BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.381	4.2	ng	189742	1	6.963	906701	20.0