

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012422\
 Data File : BF126635.D
 Acq On : 24 Jan 2022 13:32
 Operator : CG/JU
 Sample : PB142179BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB142179BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126635.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.369	36	48	56	rVB	131783	194985	3.63%	0.625%
2	4.134	343	348	353	rVB	139572	169662	3.16%	0.544%
3	5.593	590	596	599	rBV	3877564	4161921	77.50%	13.346%
4	6.581	757	764	766	rBV	3571041	4316994	80.39%	13.843%
5	6.963	825	829	832	rBB	1001682	808536	15.06%	2.593%
6	7.522	919	924	927	rBV	2490613	2845729	52.99%	9.125%
7	8.245	1042	1047	1050	rBV	1153767	1065308	19.84%	3.416%
8	9.322	1224	1230	1233	rBV	4424179	4612830	85.90%	14.792%
9	10.004	1341	1346	1349	rBV	1439570	1216284	22.65%	3.900%
10	10.798	1474	1481	1484	rBV	3147433	2943431	54.81%	9.439%
11	11.498	1596	1600	1603	rBV	1557594	1289496	24.01%	4.135%
12	13.092	1866	1871	1874	rBV	5463207	5370039	100.00%	17.220%
13	14.151	2046	2051	2054	rBV	1265405	1219330	22.71%	3.910%
14	15.686	2306	2312	2316	rBV	759630	970434	18.07%	3.112%




Sum of corrected areas: 31184979

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012422\
Data File : BF126635.D
Acq On : 24 Jan 2022 13:32
Operator : CG/JU
Sample : PB142179BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142179BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

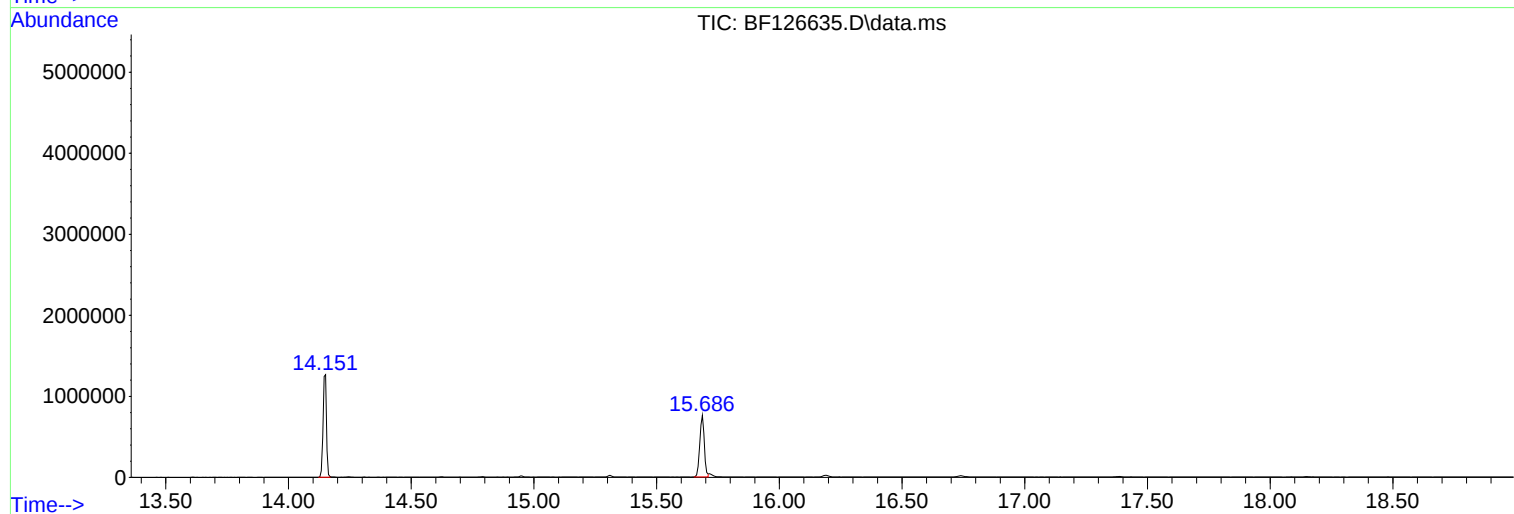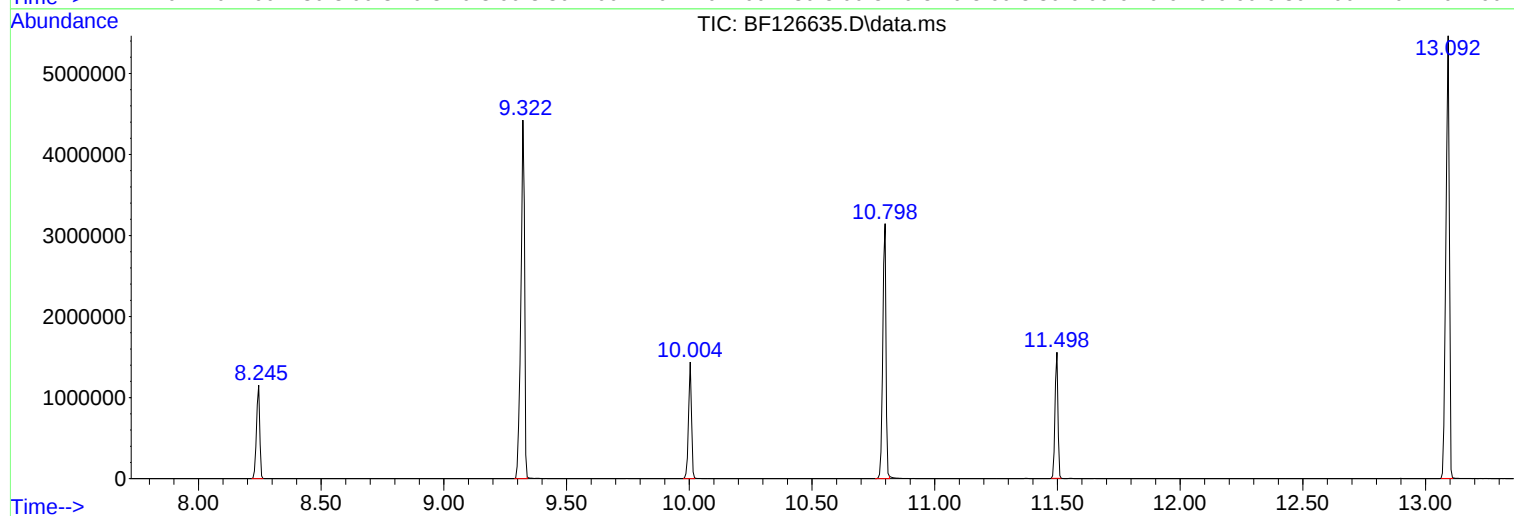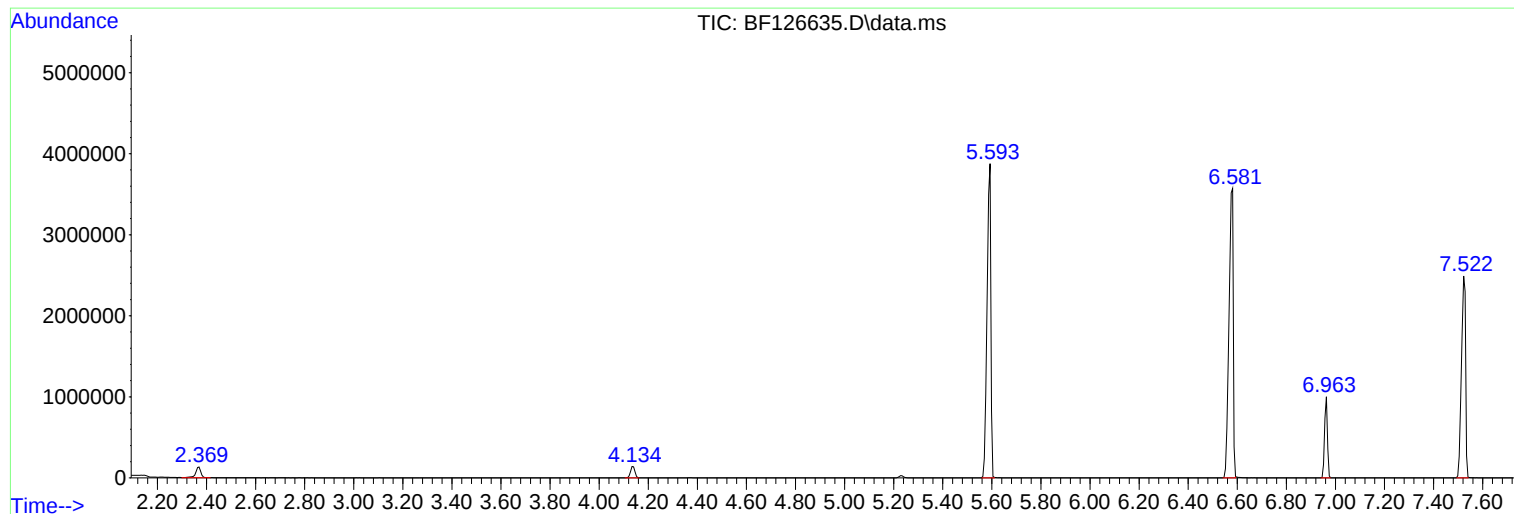

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012422\
Data File : BF126635.D
Acq On : 24 Jan 2022 13:32
Operator : CG/JU
Sample : PB142179BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142179BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.369	4.82 ng	194985	1,4-Dichlorobenzene-d4	6.963

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	43
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
4			N-Ethylformamide	73	C3H7NO	000627-45-2	9
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9

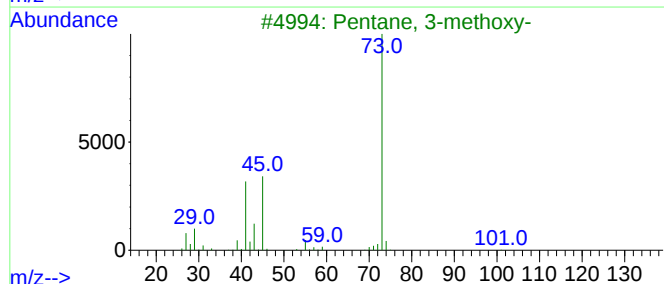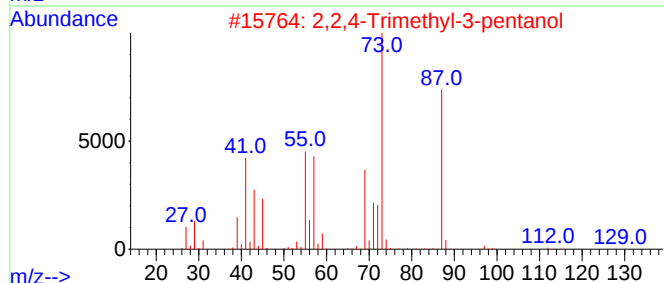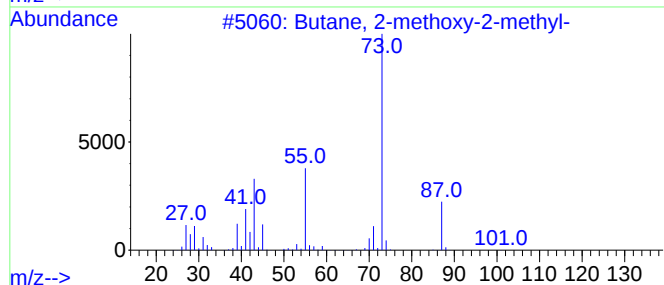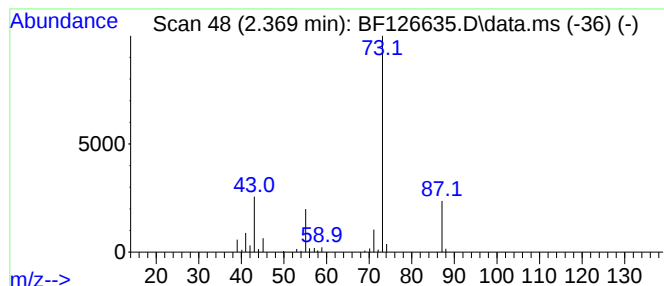

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012422\
Data File : BF126635.D
Acq On : 24 Jan 2022 13:32
Operator : CG/JU
Sample : PB142179BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142179BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.369	4.8	ng	194985	1	6.963	808536	20.0