


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012422\
 Data File : BF126627.D
 Acq On : 24 Jan 2022 09:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 27 03:09:40 2022

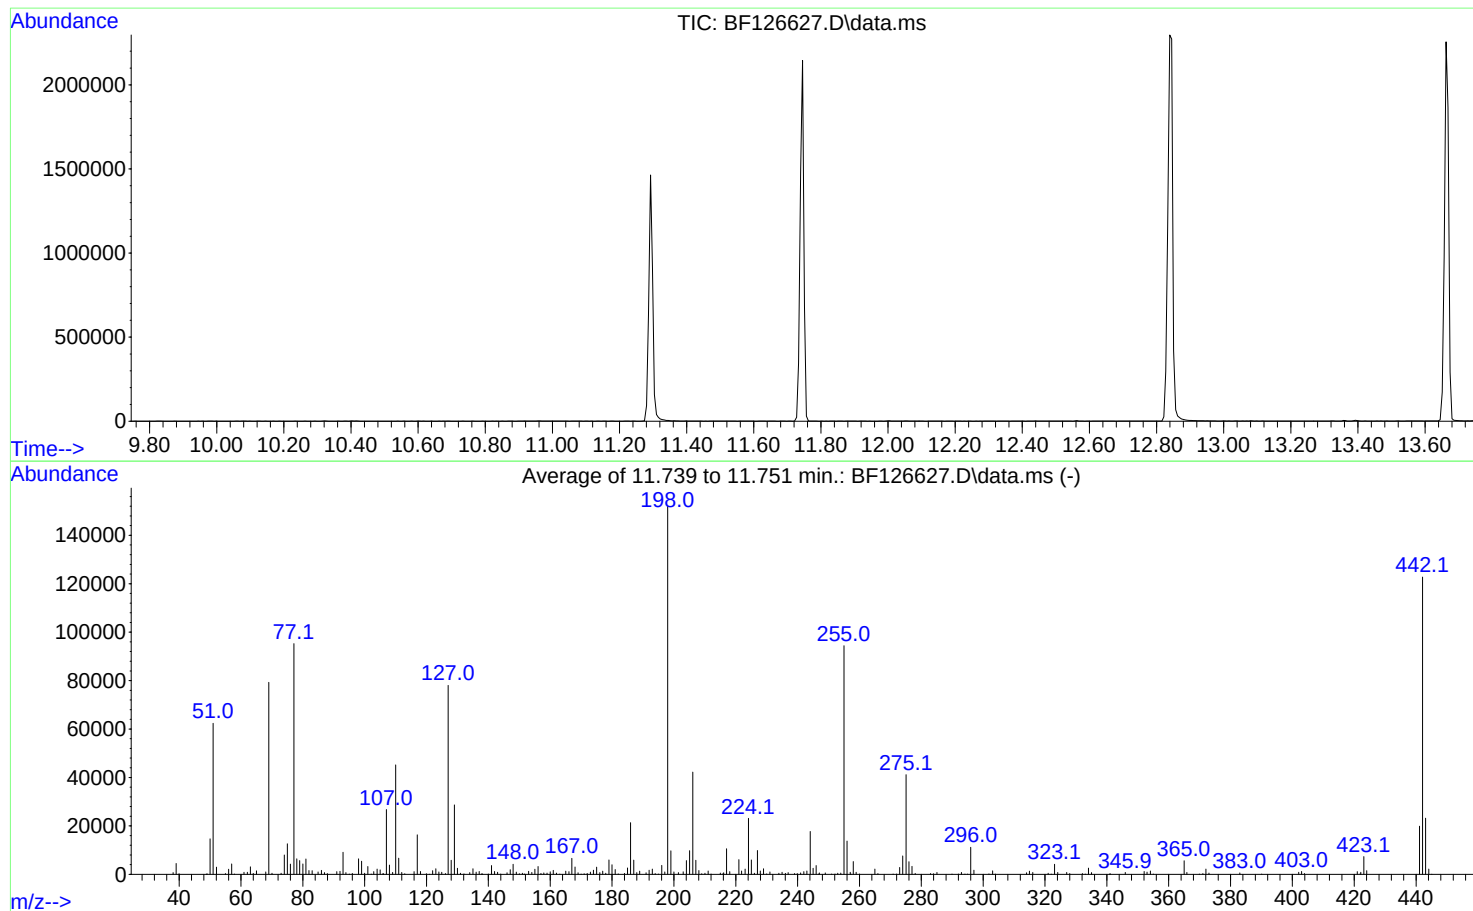




AutoFind: Scans 1641, 1642, 1643; Background Corrected with Scan 1636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	62395	PASS
68	69	0.00	2	1.3	1012	PASS
69	198	0.00	100	52.2	79264	PASS
70	69	0.00	2	0.6	477	PASS
127	198	10	80	51.4	78053	PASS
197	198	0.00	2	0.7	1012	PASS
198	198	100	100	100.0	151891	PASS
199	198	5	9	6.4	9751	PASS
275	198	10	60	27.1	41189	PASS
365	198	1	100	3.7	5638	PASS
441	198	0.01	100	13.1	19926	PASS
442	442	50	100	100.0	122760	PASS
443	442	15	24	18.9	23193	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012422\
Data File : BF126627.D
Acq On : 24 Jan 2022 09:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 24 13:18:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 19 07:04:14 2022
Response via : Initial Calibration

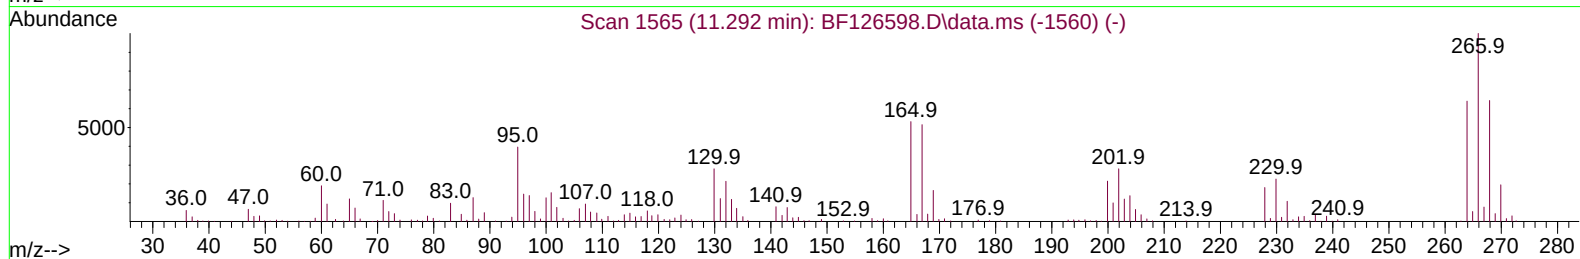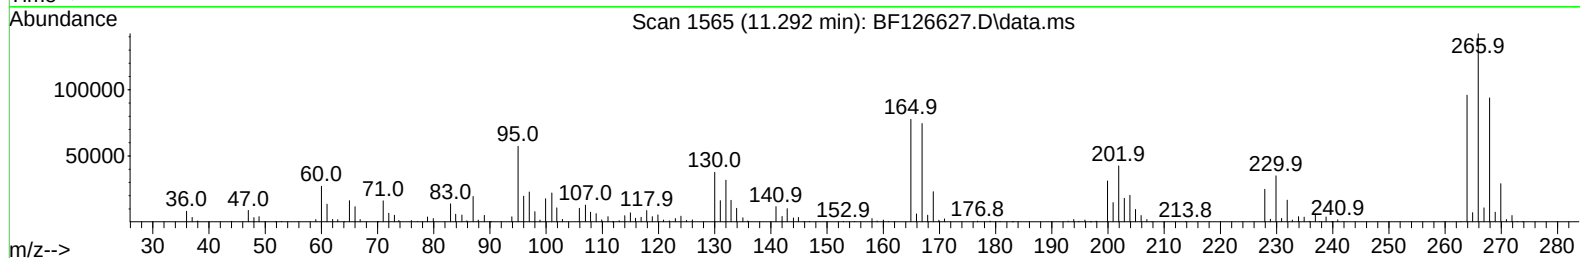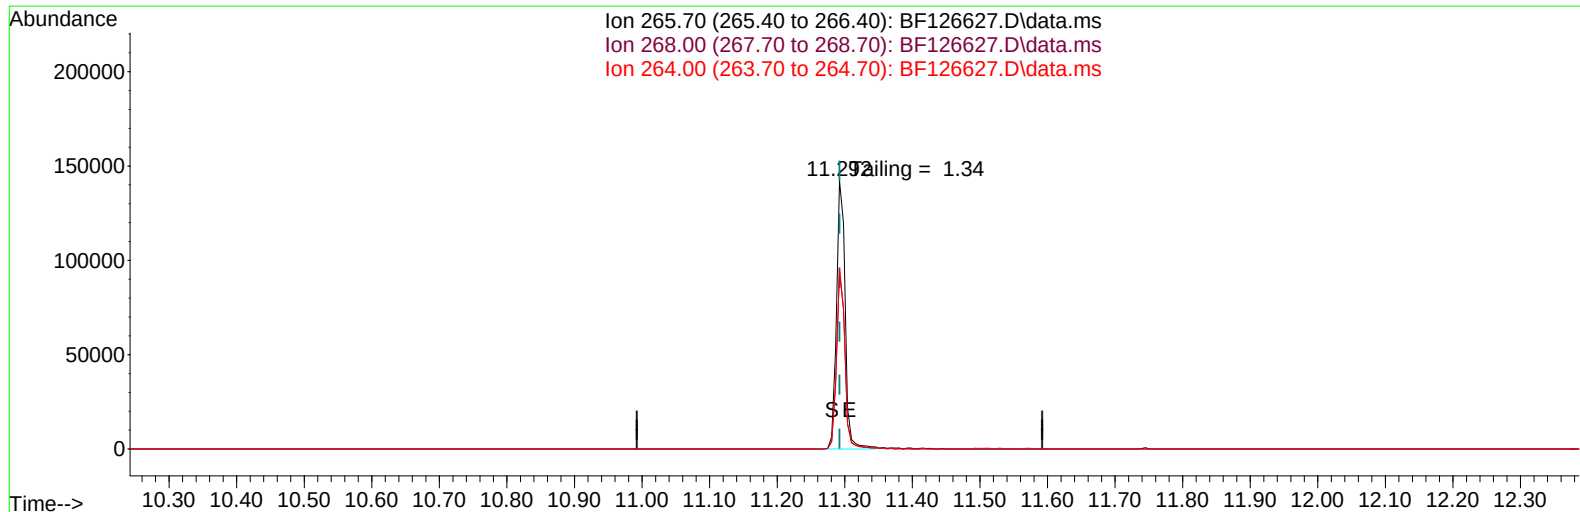

TIC: BF126627.D\data.ms

(70) Pentachlorophenol (C)

11.292min (0.000) 22965.27 ng




response 127262

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	65.96
264.00	63.00	67.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012422\
Data File : BF126627.D
Acq On : 24 Jan 2022 09:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 24 13:18:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 19 07:04:14 2022
Response via : Initial Calibration

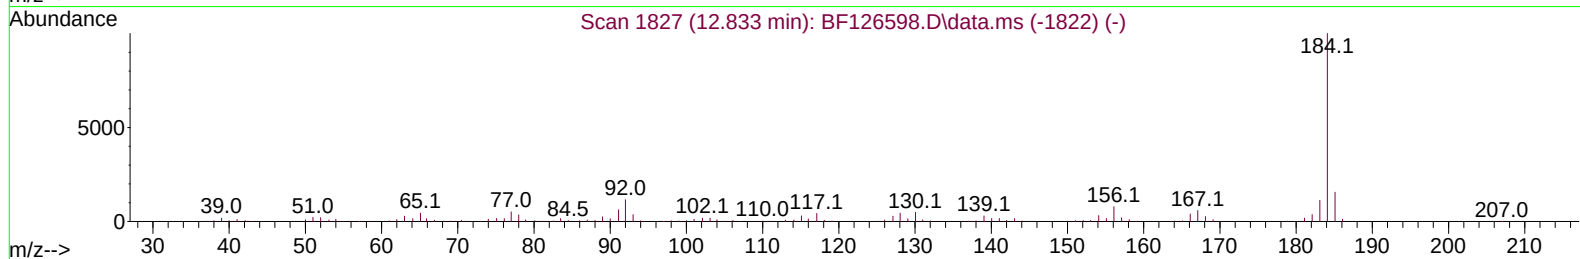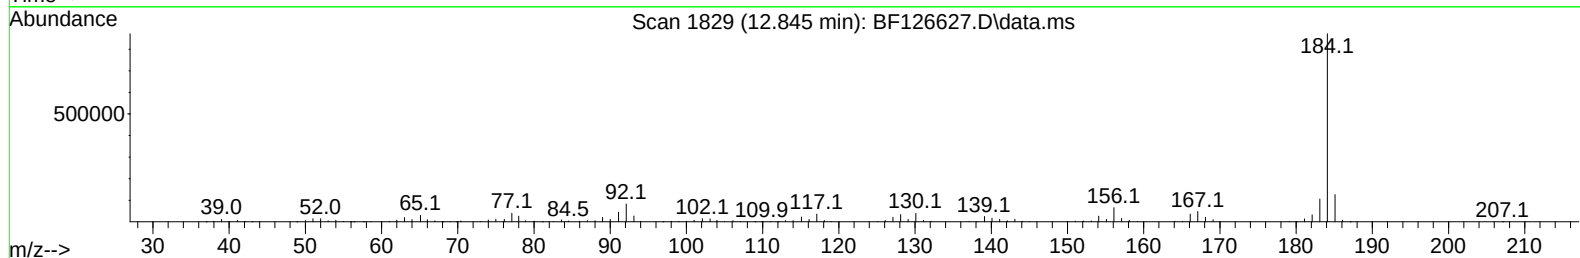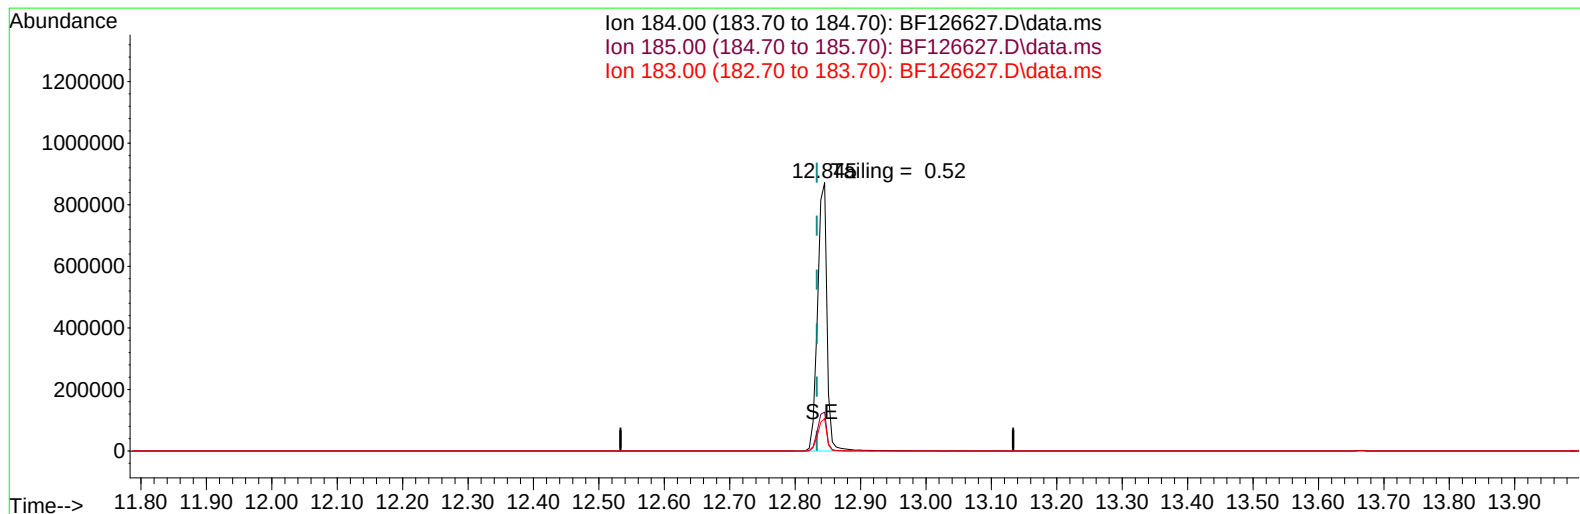

TIC: BF126627.D\data.ms

(77) Benzidine

12.845min (+ 0.012) 0.00 ng

response 875880

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.52
183.00	10.20	12.10
0.00	0.00	0.00

Instrument :

BNA_F

ClientSampleId :

DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/24/2022	BNA_F	<u>BF126627.D</u>
Compound Name	Response	Retention Time
DDT	340799	13.66
DDD	947	13.35
DDE	115	13.02
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1062	341861	0.31