
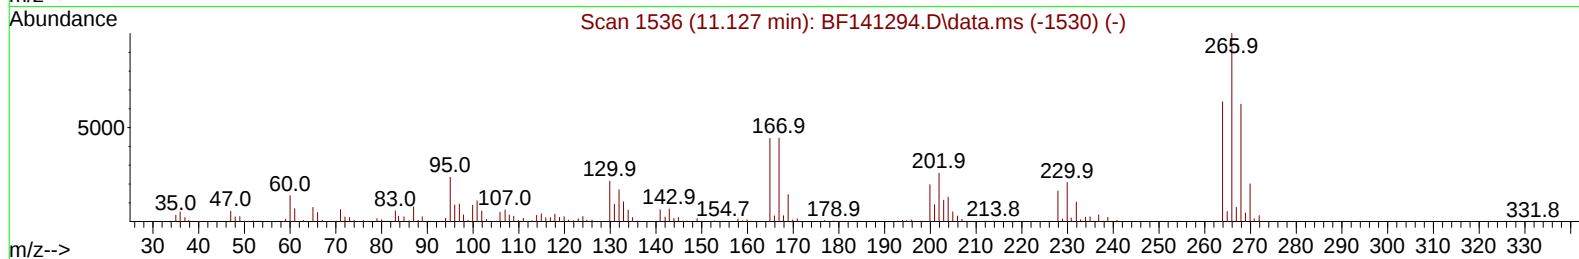



Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013125\
Data File : BF141318.D
Acq On : 31 Jan 2025 08:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 10:52:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration



TIC: BF141318.D\data.ms

(70) Pentachlorophenol (C)**11.128min (-0.006) 13648.97 ng****response 185655**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	62.83
264.00	63.70	62.03
0.00	0.00	0.00



Abundance

Ion 184.00 (183.70 to 184.70): BF141318.D\data.ms
Ion 185.00 (184.70 to 185.70): BF141318.D\data.ms
Ion 183.00 (182.70 to 183.70): BF141318.D\data.ms

800000
600000
400000
200000
0

12.63
12.63
Tail = 1.05
S/E

me--> 11.70 11.80 11.90 12.00 12.10 12.20 12.30 12.40 12.50 12.60 12.70 12.80 12.90 13.00 13.10 13.20 13.30 13.40 13.50 13.60 13.70 13.80



TIC: BF141318.D\data.ms

(77) Benzidine

12.663min (-0.000) 17733.10 ng

response **824318**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.38
183.00	11.90	11.94
0.00	0.00	0.00