
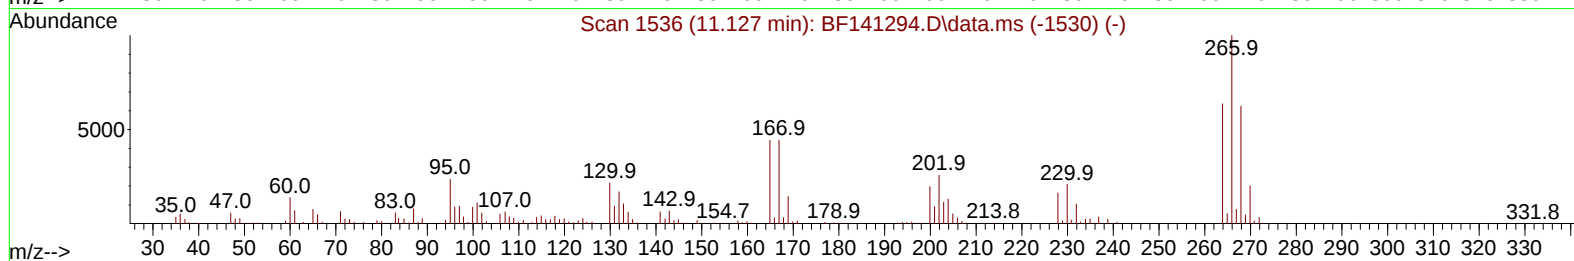
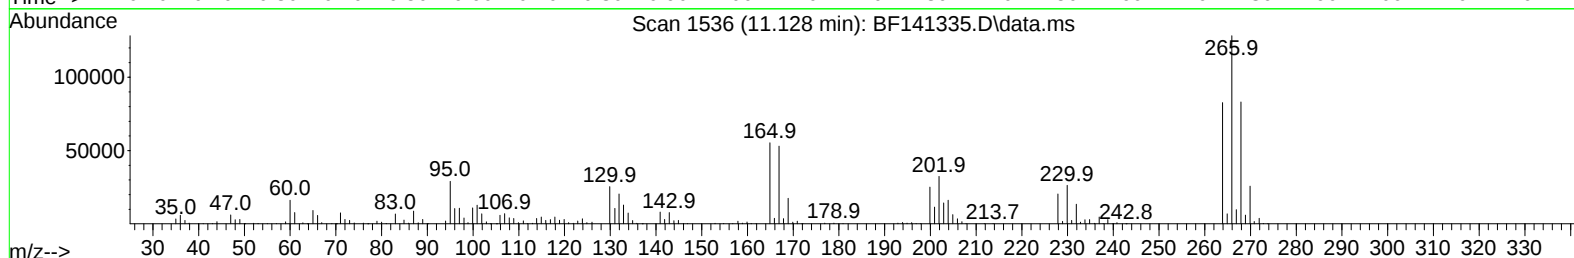


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013125\
Data File : BF141335.D
Acq On : 31 Jan 2025 16:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 17:41:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

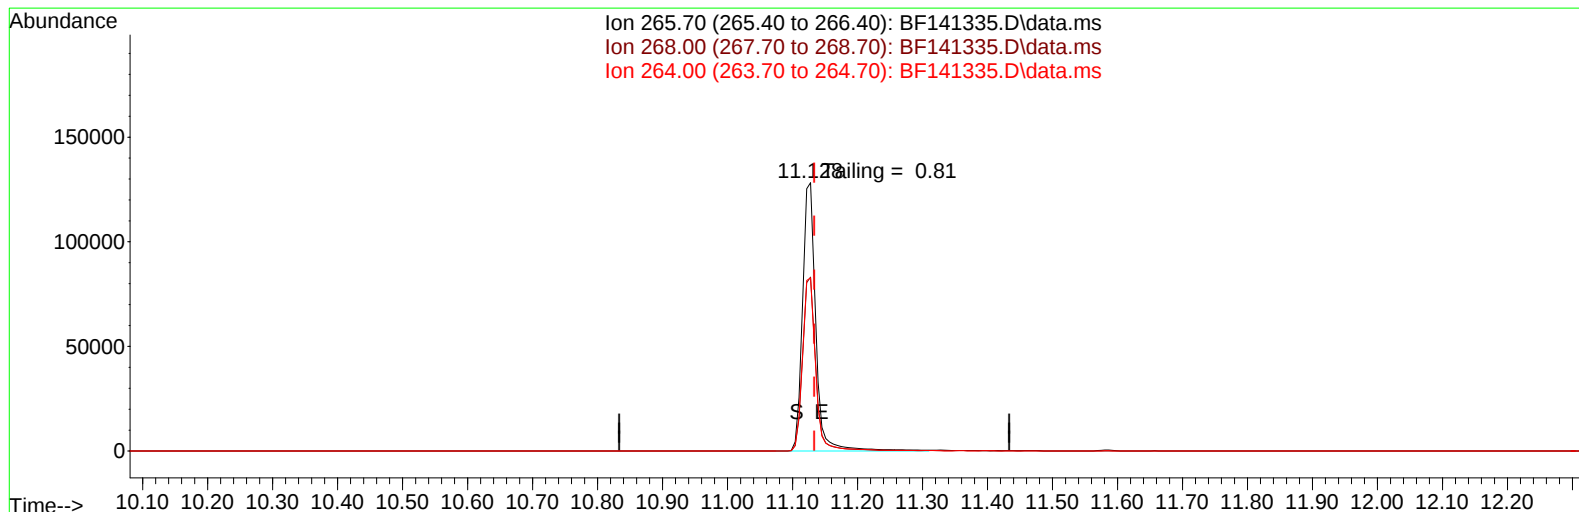

TIC: BF141335.D\data.ms

(70) Pentachlorophenol (C)




11.128min (-0.006) 9273.56 ng

response 183922

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	64.82
264.00	63.70	64.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF013125\
Data File : BF141335.D
Acq On : 31 Jan 2025 16:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 17:41:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 29 17:41:25 2025
Response via : Initial Calibration

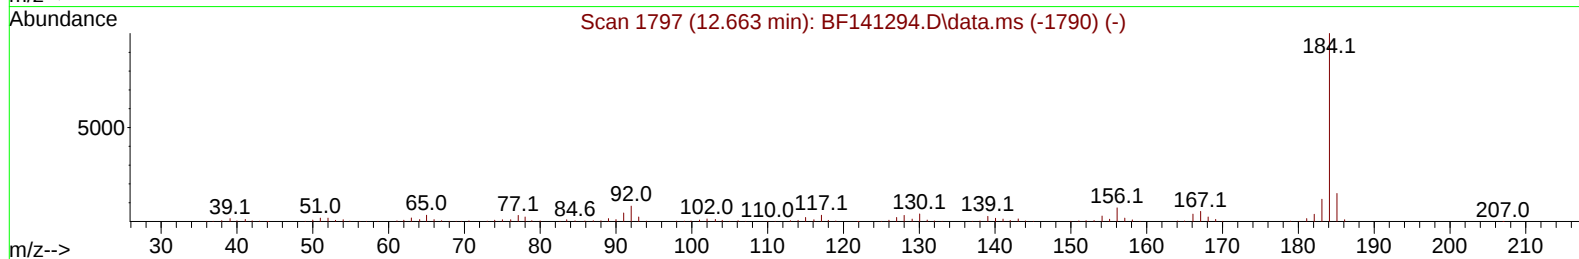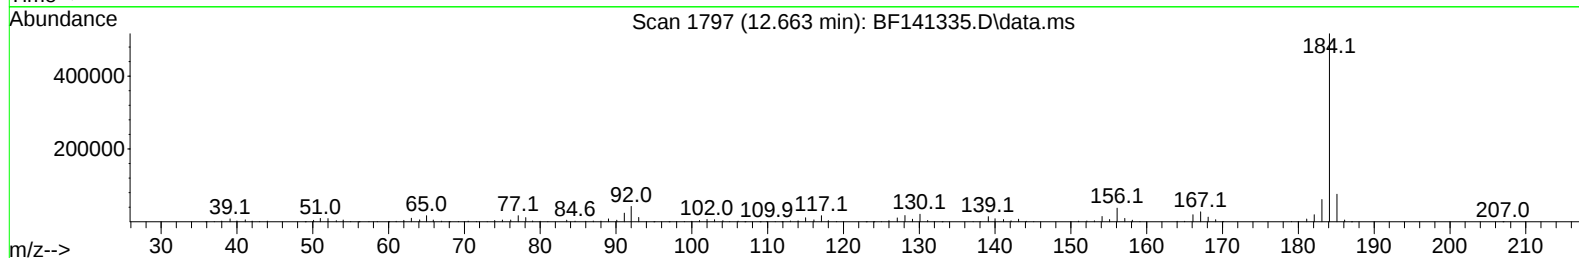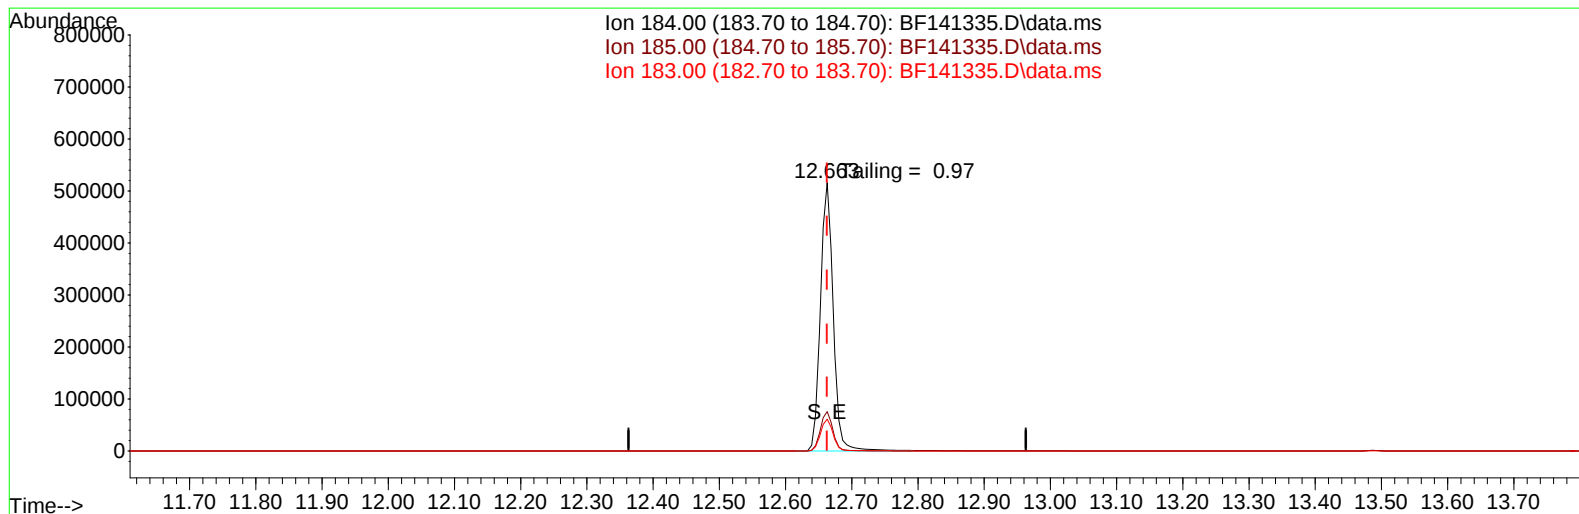

TIC: BF141335.D\data.ms

(77) Benzidine

12.663min (-0.000) 12340.55 ng

response 693915

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.67
183.00	11.90	11.87
0.00	0.00	0.00