

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020122\
 Data File : BF126768.D
 Acq On : 01 Feb 2022 11:52
 Operator : CG/JU
 Sample : PB142400BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB142400BL

Quant Time: Feb 02 04:56:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 27 03:09:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.957	152	136331	20.000	ng	0.00
21) Naphthalene-d8	8.239	136	553146	20.000	ng	0.00
39) Acenaphthene-d10	9.998	164	314528	20.000	ng	0.00
64) Phenanthrene-d10	11.492	188	565855	20.000	ng	0.00
76) Chrysene-d12	14.139	240	426107	20.000	ng	# 0.00
86) Perylene-d12	15.662	264	289118	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.587	112	1216512	117.421	ng	0.02
7) Phenol-d6	6.575	99	1659103	115.260	ng	0.00
23) Nitrobenzene-d5	7.522	82	1212674	85.810	ng	0.00
42) 2,4,6-Tribromophenol	10.792	330	413739	140.560	ng	0.00
45) 2-Fluorobiphenyl	9.316	172	1597633	77.792	ng	0.00
79) Terphenyl-d14	13.086	244	1958532	77.093	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020122\
Data File : BF126768.D
Acq On : 01 Feb 2022 11:52
Operator : CG/JU
Sample : PB142400BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142400BL

Quant Time: Feb 02 04:56:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 27 03:09:40 2022
Response via : Initial Calibration




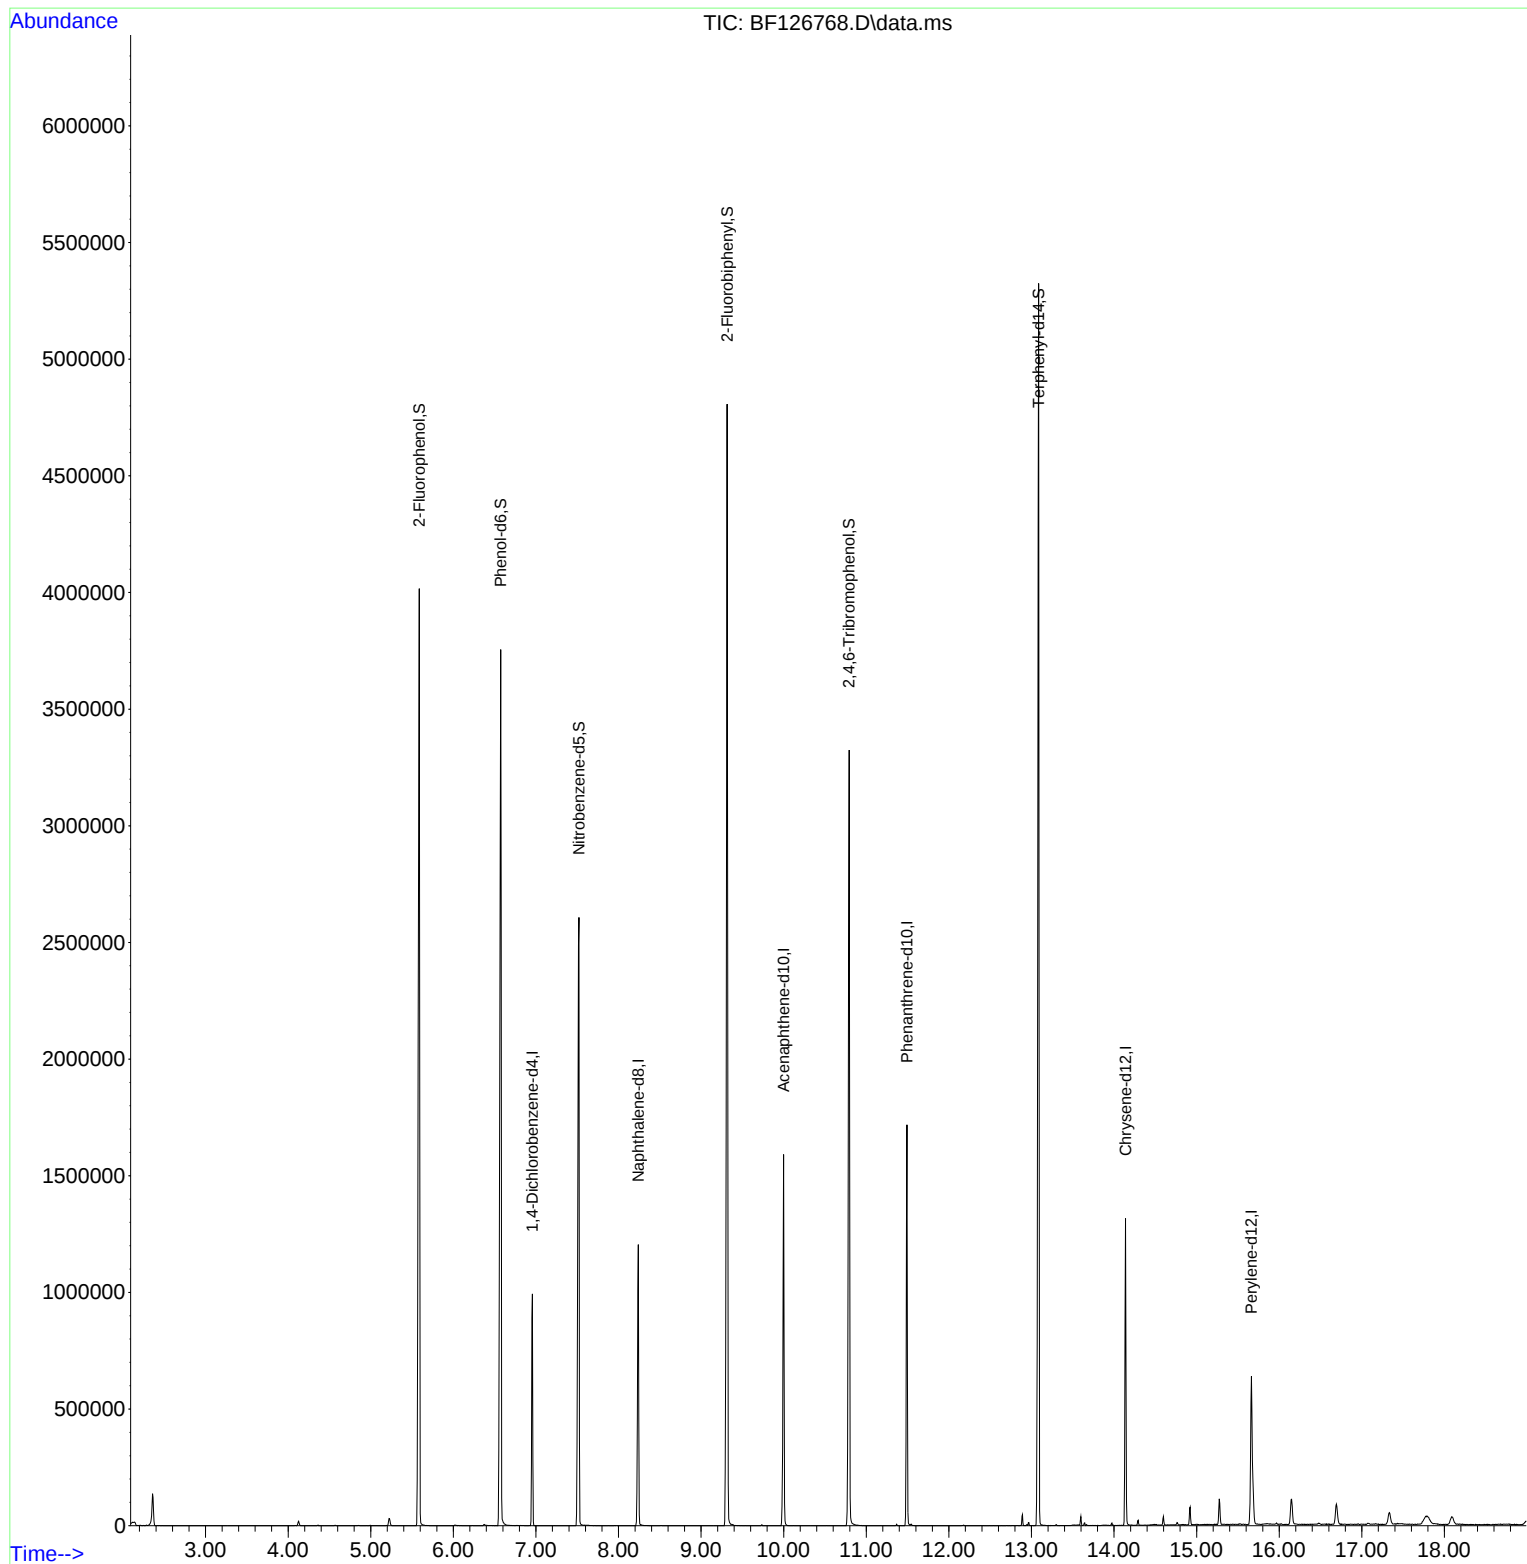




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.957 min Scan# 81
Delta R.T. 0.000 min
Lab File: BF126768.D
Acq: 01 Feb 2022 11:52




Instrument :
BNA_F
ClientSampleId :
PB142400BL


Tgt Ion:152 Resp: 136331
Ion Ratio Lower Upper
152 100
150 155.9 128.1 192.1
115 68.5 56.7 85.1

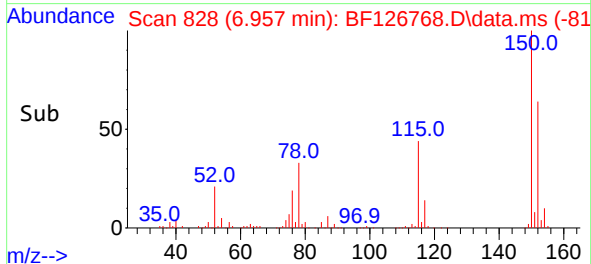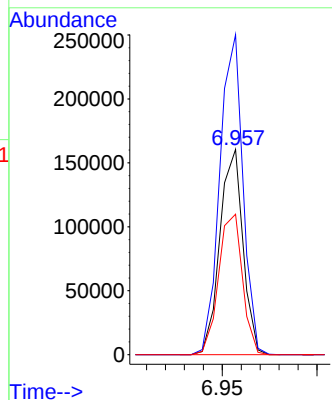

#5
2-Fluorophenol
Concen: 117.421 ng
RT: 5.587 min Scan# 595
Delta R.T. 0.018 min
Lab File: BF126768.D
Acq: 01 Feb 2022 11:52

Tgt Ion:112 Resp: 1216512
Ion Ratio Lower Upper
112 100
64 64.0 49.5 74.3
63 33.0 23.9 35.9


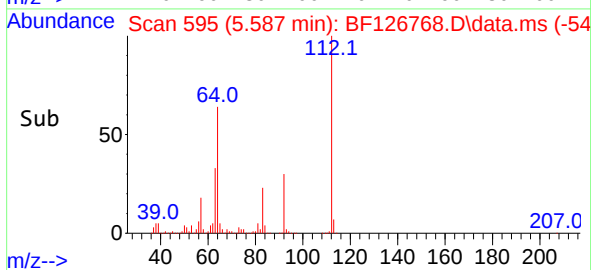
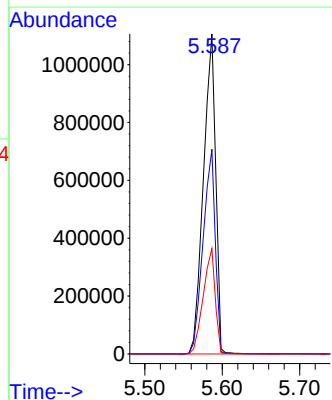
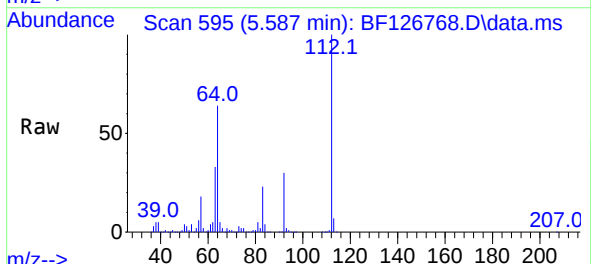




#7
Phenol-d6
Concen: 115.260 ng
RT: 6.575 min Scan# 71
Delta R.T. -0.000 min
Lab File: BF126768.D
Acq: 01 Feb 2022 11:52




Instrument :
BNA_F
ClientSampleId :
PB142400BL

Tgt Ion: 99 Resp: 1659103
Ion Ratio Lower Upper
99 100
42 15.6 14.2 21.4
71 40.1 24.3 36.5#

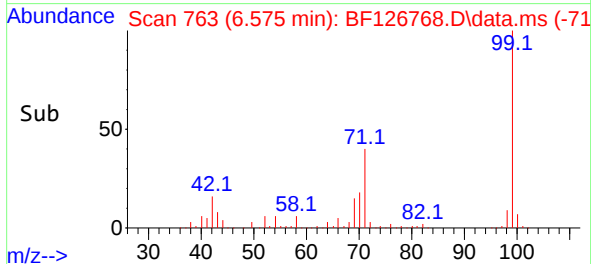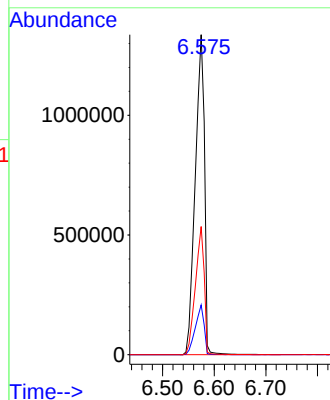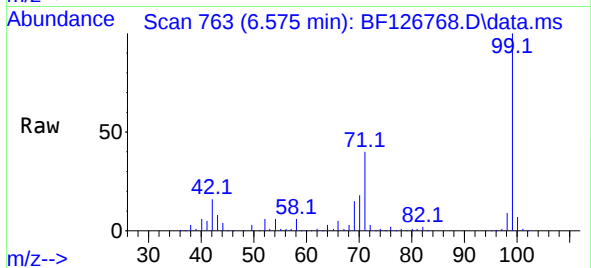

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.239 min Scan# 1046
Delta R.T. -0.000 min
Lab File: BF126768.D
Acq: 01 Feb 2022 11:52

Tgt Ion:136 Resp: 553146
Ion Ratio Lower Upper
136 100
137 10.5 8.6 13.0
54 8.1 7.8 11.6
68 7.7 6.3 9.5


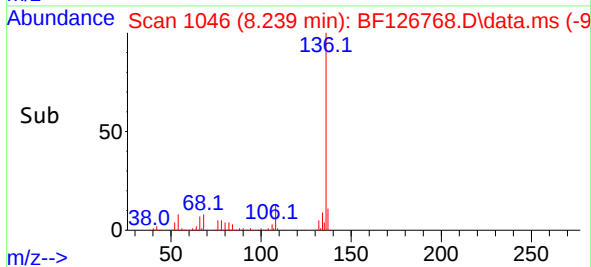
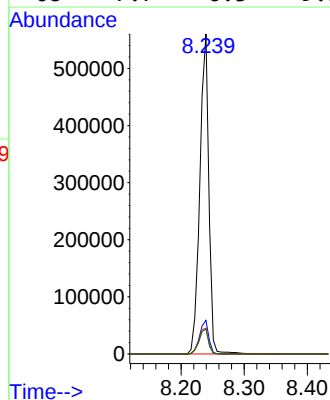
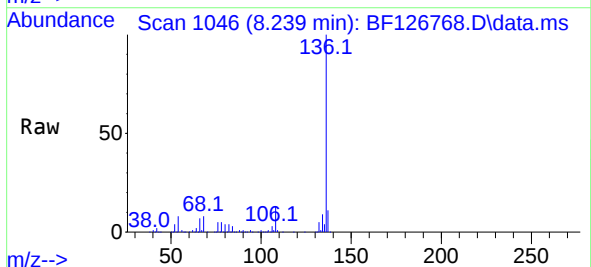




#23
Nitrobenzene-d5
Concen: 85.810 ng
RT: 7.522 min Scan# 91
Delta R.T. -0.000 min
Lab File: BF126768.D
Acq: 01 Feb 2022 11:52




Instrument :
BNA_F
ClientSampleId :
PB142400BL


Tgt Ion: 82 Resp: 1212674
Ion Ratio Lower Upper
82 100
128 33.8 32.7 49.1
54 38.4 41.7 62.5#

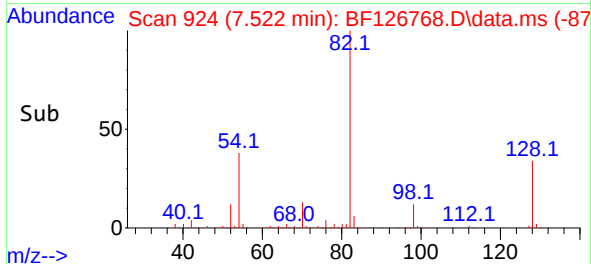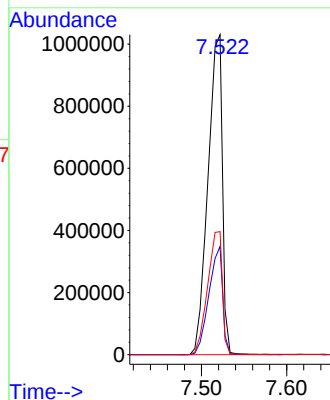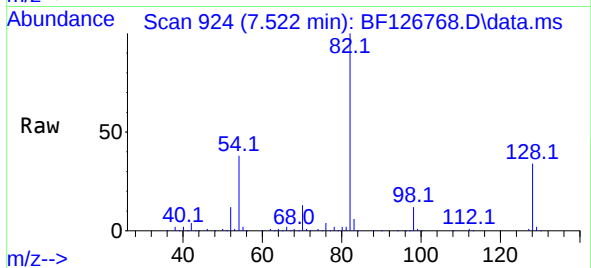

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.998 min Scan# 1345
Delta R.T. -0.000 min
Lab File: BF126768.D
Acq: 01 Feb 2022 11:52


Tgt Ion:164 Resp: 314528
Ion Ratio Lower Upper
164 100
162 102.2 81.4 122.0
160 43.3 36.6 54.8

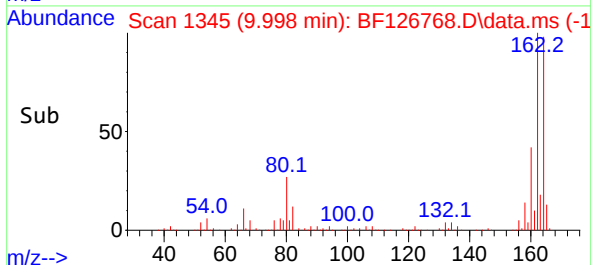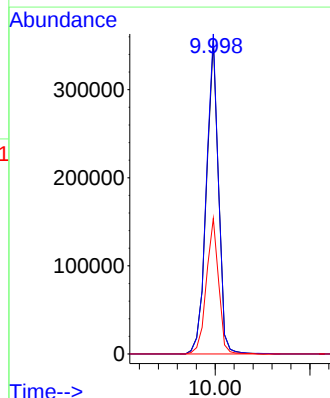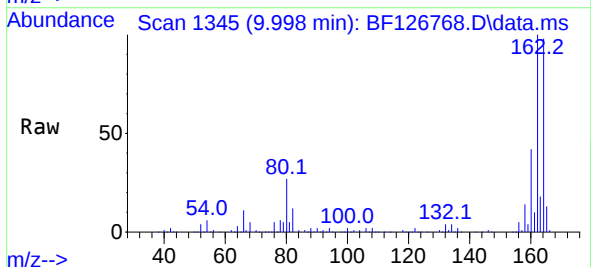



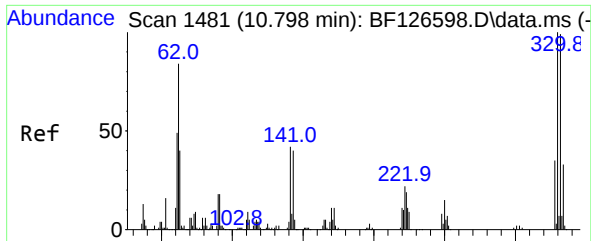


#42
2,4,6-Tribromophenol
Concen: 140.560 ng
RT: 10.792 min Scan# 1481
Delta R.T. -0.000 min
Lab File: BF126768.D
Acq: 01 Feb 2022 11:52

Instrument :
BNA_F
ClientSampleId :
PB142400BL



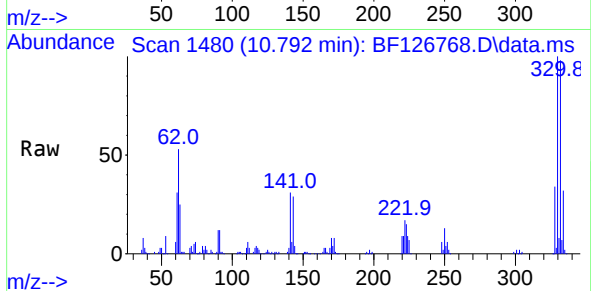



Tgt Ion:330 Resp: 413739
Ion Ratio Lower Upper
330 100
332 97.1 76.0 114.0
141 31.8 30.1 45.1

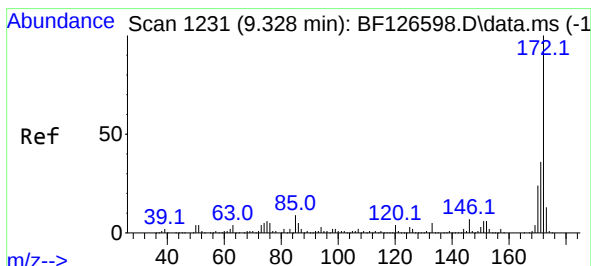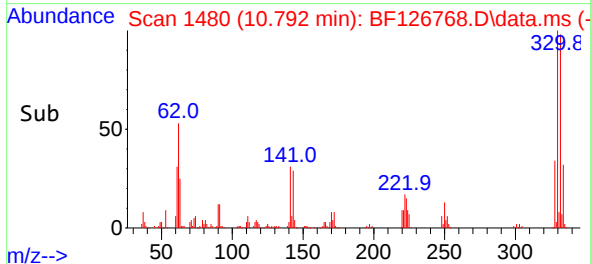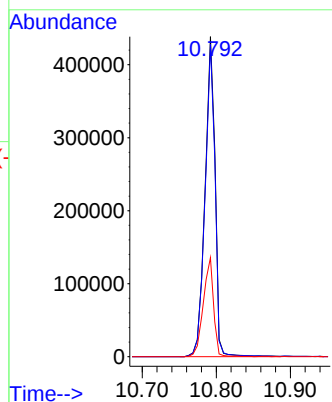

#45
2-Fluorobiphenyl
Concen: 77.792 ng
RT: 9.316 min Scan# 1229
Delta R.T. -0.000 min
Lab File: BF126768.D
Acq: 01 Feb 2022 11:52

Tgt Ion:172 Resp: 1597633
Ion Ratio Lower Upper
172 100
171 36.0 28.3 42.5
170 24.0 19.0 28.6


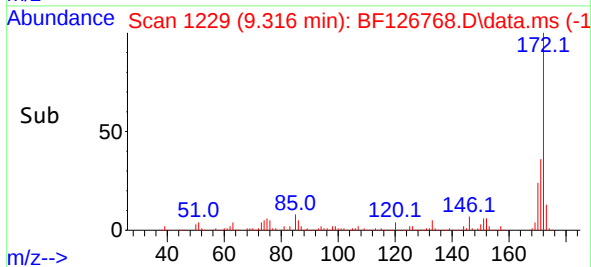
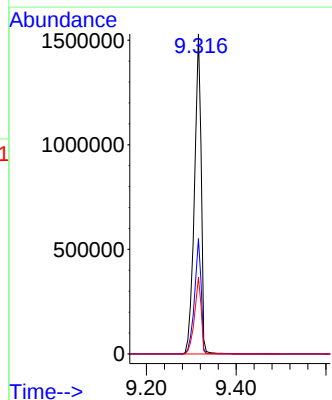
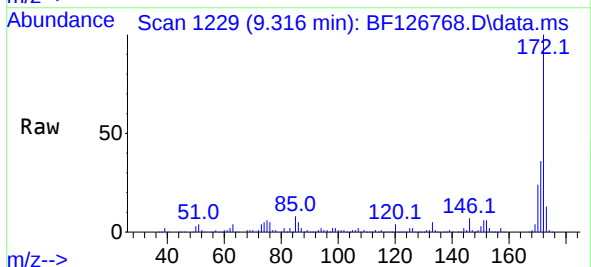


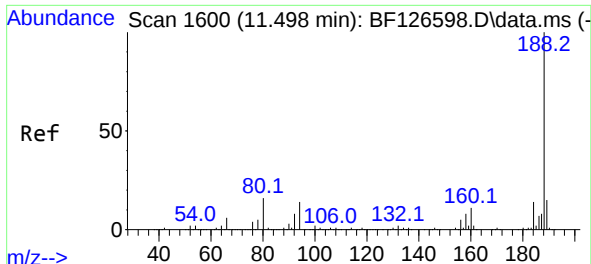

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.492 min Scan# 11
Delta R.T. -0.000 min
Lab File: BF126768.D
Acq: 01 Feb 2022 11:52




Instrument :
BNA_F
ClientSampleId :
PB142400BL


Tgt Ion:188 Resp: 565855
Ion Ratio Lower Upper
188 100
94 12.2 10.1 15.1
80 14.1 11.8 17.6

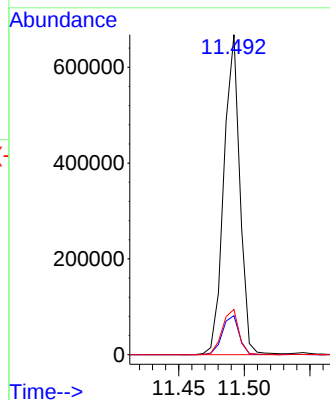

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.139 min Scan# 2049
Delta R.T. -0.006 min
Lab File: BF126768.D
Acq: 01 Feb 2022 11:52


Tgt Ion:240 Resp: 426107
Ion Ratio Lower Upper
240 100
120 10.7 14.4 21.6#
236 24.6 20.5 30.7

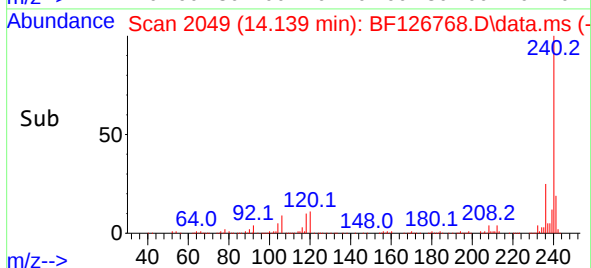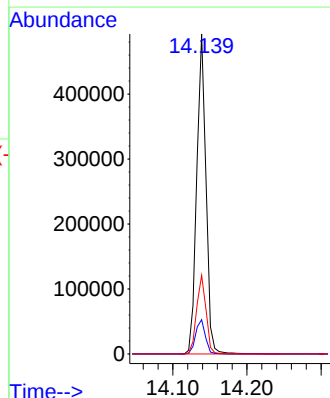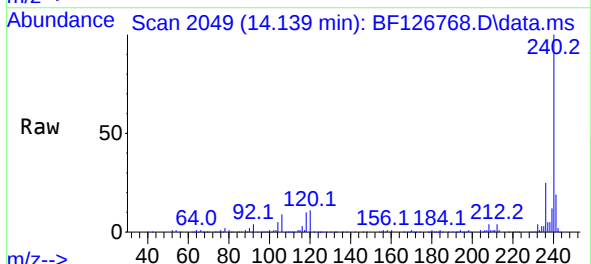






#79
 Terphenyl-d14
 Concen: 77.093 ng
 RT: 13.086 min Scan# 11
 Delta R.T. 0.006 min
 Lab File: BF126768.D
 Acq: 01 Feb 2022 11:52

Instrument :
 BNA_F
 ClientSampleId :
 PB142400BL

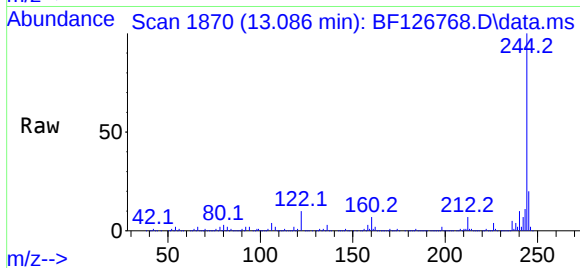

Tgt Ion:244 Resp: 1958532
 Ion Ratio Lower Upper
 244 100
 212 6.9 5.0 7.4
 122 9.6 13.3 19.9#

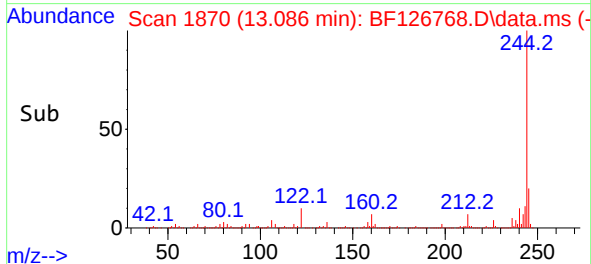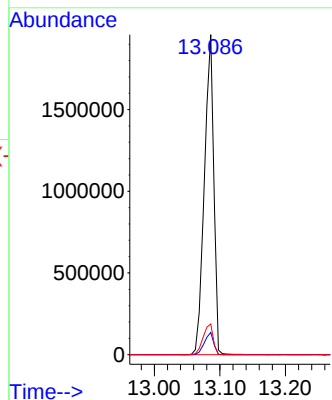

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.662 min Scan# 2308
 Delta R.T. -0.000 min
 Lab File: BF126768.D
 Acq: 01 Feb 2022 11:52

Tgt Ion:264 Resp: 289118
 Ion Ratio Lower Upper
 264 100
 260 24.3 19.2 28.8
 265 21.4 17.4 26.2

