

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020122\
 Data File : BF126774.D
 Acq On : 01 Feb 2022 15:17
 Operator : CG/JU
 Sample : N1340-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-7(1.5-2)

Quant Time: Feb 02 04:58:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 27 03:09:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.957	152	122851	20.000	ng	0.00
21) Naphthalene-d8	8.239	136	472298	20.000	ng	# 0.00
39) Acenaphthene-d10	9.998	164	268399	20.000	ng	0.00
64) Phenanthrene-d10	11.486	188	466208	20.000	ng	0.00
76) Chrysene-d12	14.139	240	277596	20.000	ng	# 0.00
86) Perylene-d12	15.656	264	228918	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.581	112	921900	98.748	ng	0.01
7) Phenol-d6	6.575	99	1250164	96.381	ng	0.00
23) Nitrobenzene-d5	7.516	82	900665	74.641	ng	0.00
42) 2,4,6-Tribromophenol	10.786	330	289551	115.276	ng	0.00
45) 2-Fluorobiphenyl	9.316	172	1189017	67.846	ng	0.00
79) Terphenyl-d14	13.080	244	1287307	77.780	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020122\
Data File : BF126774.D
Acq On : 01 Feb 2022 15:17
Operator : CG/JU
Sample : N1340-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-7(1.5-2)

Quant Time: Feb 02 04:58:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 27 03:09:40 2022
Response via : Initial Calibration




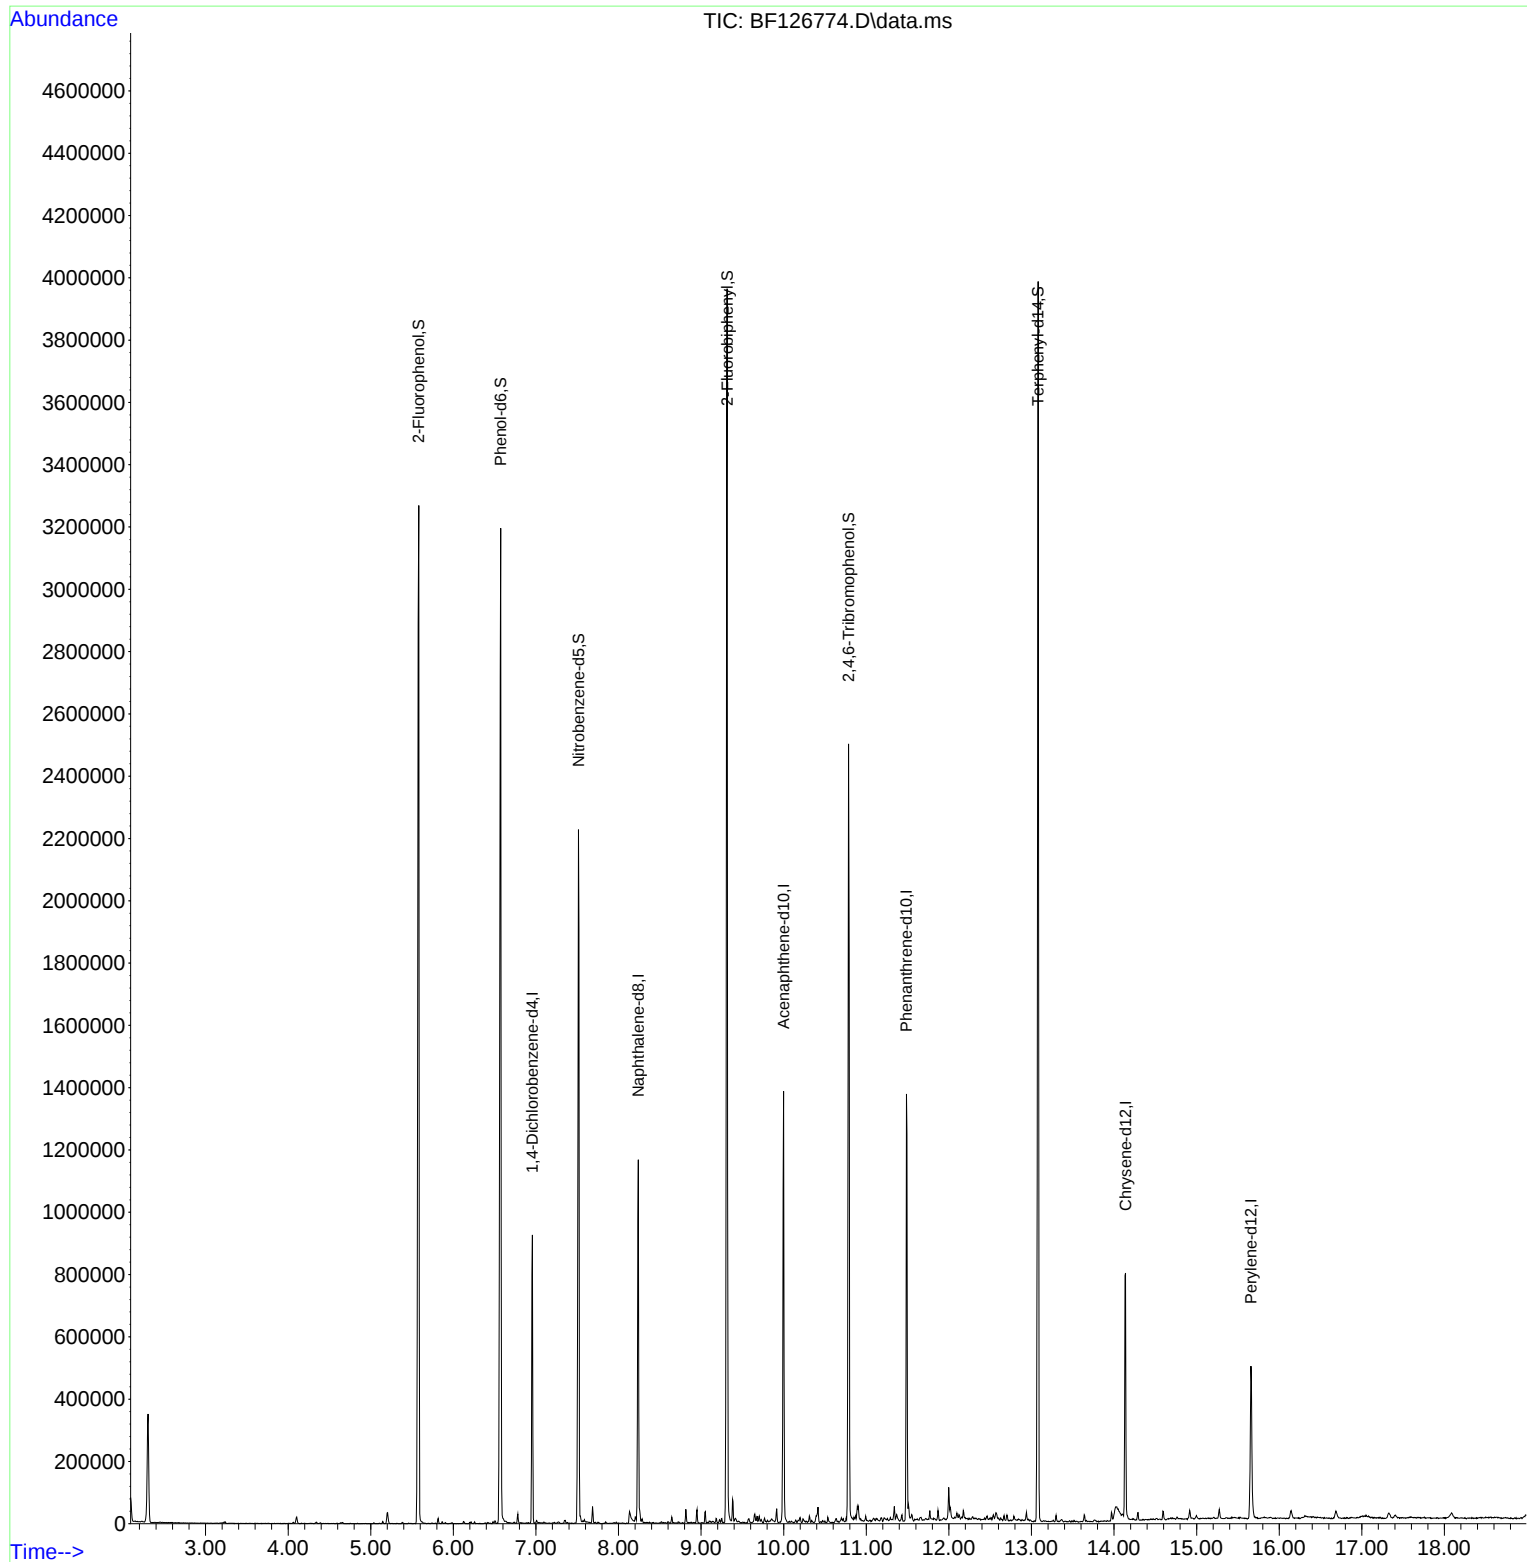




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.957 min Scan# 81
Delta R.T. 0.000 min
Lab File: BF126774.D
Acq: 01 Feb 2022 15:17




Instrument :
BNA_F
ClientSampleId :
SB-7(1.5-2)


Tgt Ion:152 Resp: 122851
Ion Ratio Lower Upper
152 100
150 157.2 128.1 192.1
115 69.1 56.7 85.1

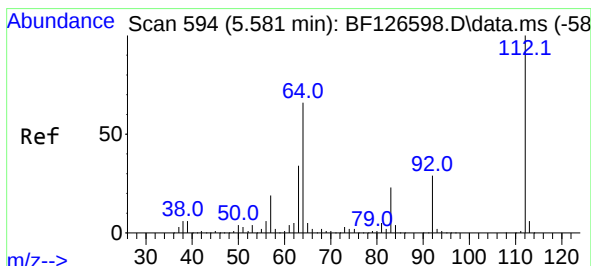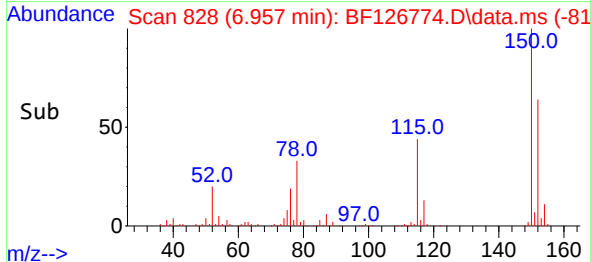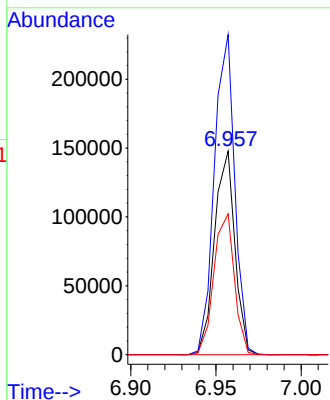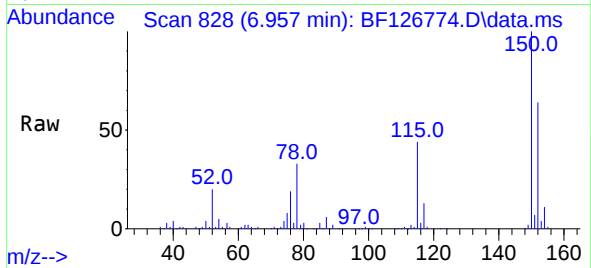

#5
2-Fluorophenol
Concen: 98.748 ng
RT: 5.581 min Scan# 594
Delta R.T. 0.012 min
Lab File: BF126774.D
Acq: 01 Feb 2022 15:17

Tgt Ion:112 Resp: 921900
Ion Ratio Lower Upper
112 100
64 62.8 49.5 74.3
63 31.8 23.9 35.9


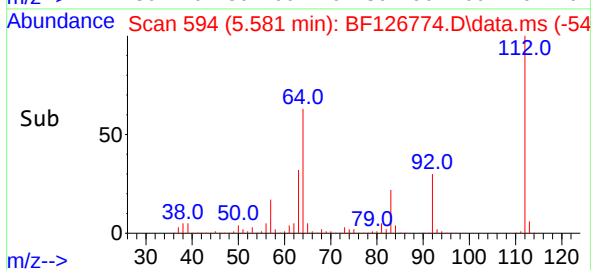
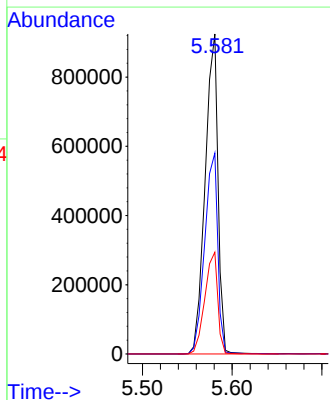
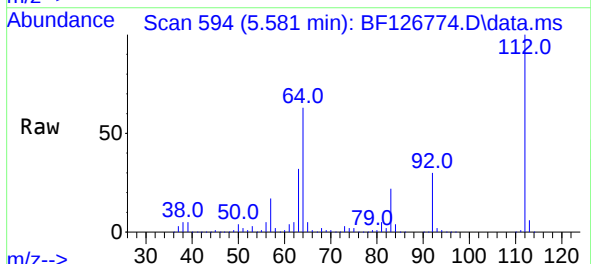


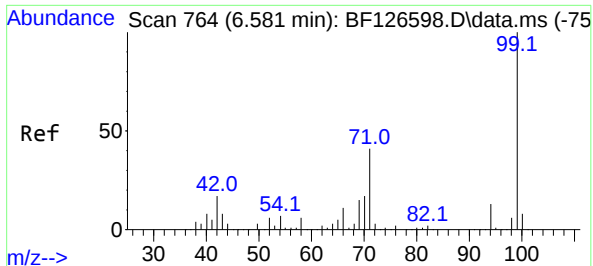

#7
Phenol-d6
Concen: 96.381 ng
RT: 6.575 min Scan# 71
Delta R.T. -0.000 min
Lab File: BF126774.D
Acq: 01 Feb 2022 15:17




Instrument :
BNA_F
ClientSampleId :
SB-7(1.5-2)


Tgt Ion: 99 Resp: 1250164
Ion Ratio Lower Upper
99 100
42 14.5 14.2 21.4
71 37.4 24.3 36.5#

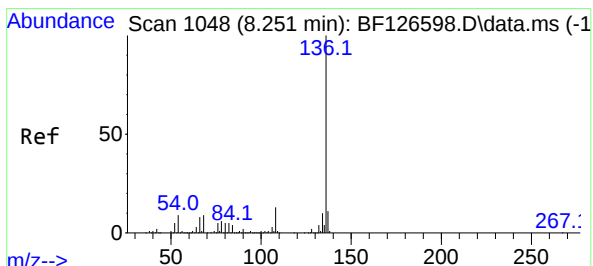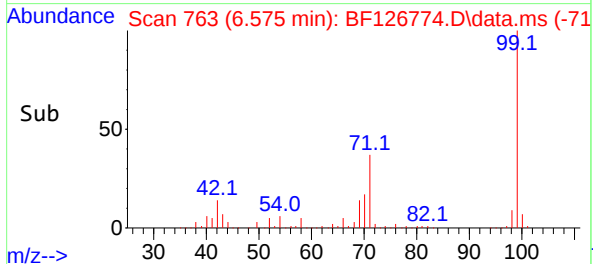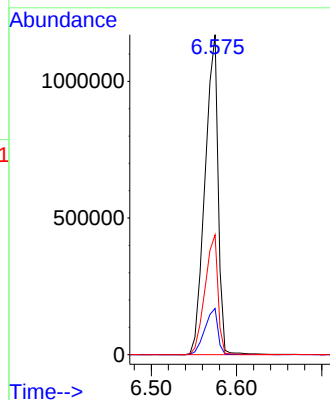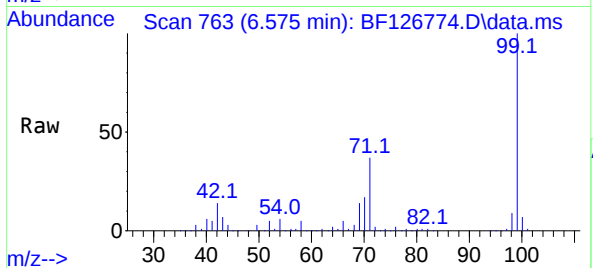

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.239 min Scan# 1046
Delta R.T. -0.000 min
Lab File: BF126774.D
Acq: 01 Feb 2022 15:17

Tgt Ion:136 Resp: 472298
Ion Ratio Lower Upper
136 100
137 10.6 8.6 13.0
54 7.6 7.8 11.6#
68 8.0 6.3 9.5


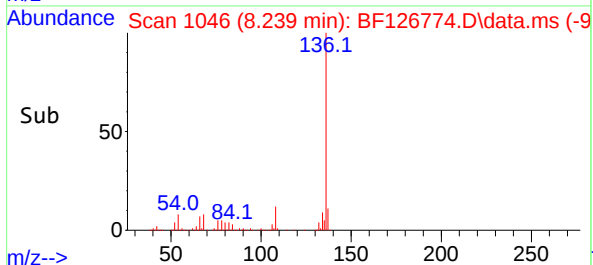
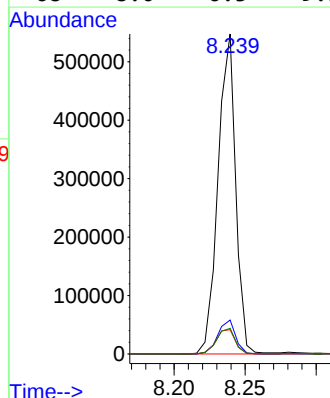
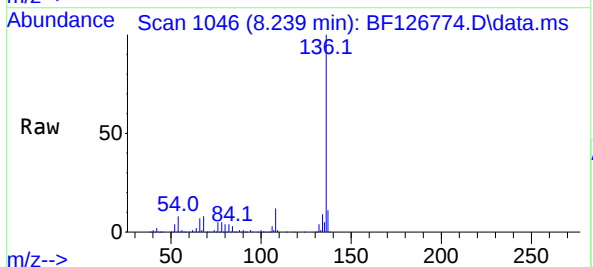


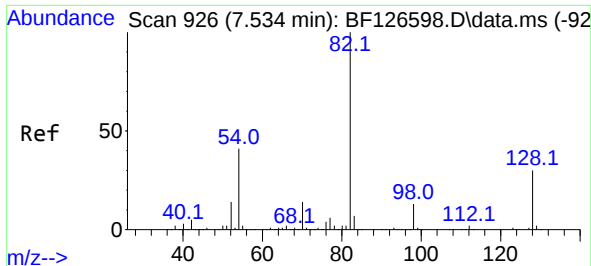

#23
Nitrobenzene-d5
Concen: 74.641 ng
RT: 7.516 min Scan# 91
Delta R.T. -0.006 min
Lab File: BF126774.D
Acq: 01 Feb 2022 15:17




Instrument :
BNA_F
ClientSampleId :
SB-7(1.5-2)


Tgt Ion: 82 Resp: 900665
Ion Ratio Lower Upper
82 100
128 31.7 32.7 49.1#
54 40.5 41.7 62.5#

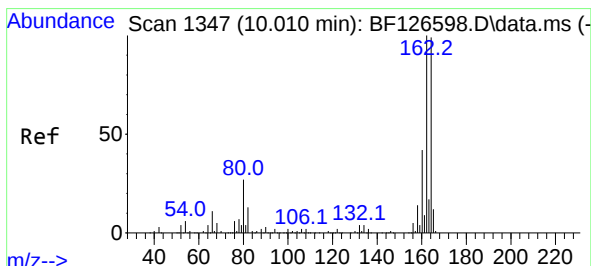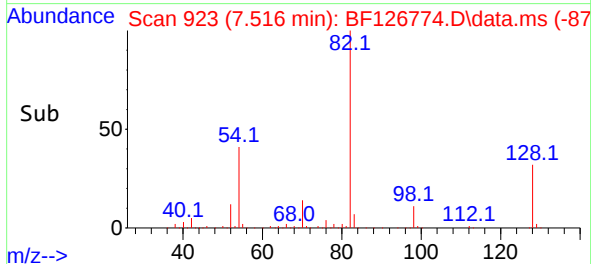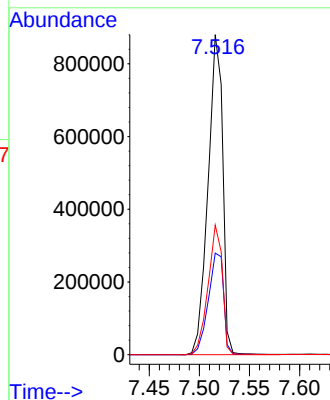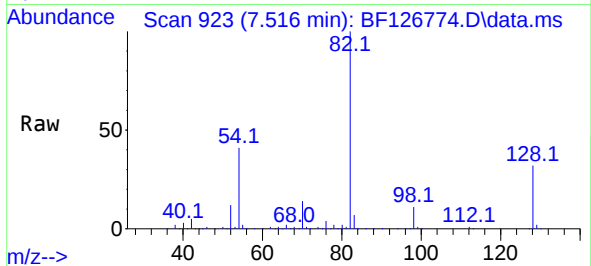

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.998 min Scan# 1345
Delta R.T. -0.000 min
Lab File: BF126774.D
Acq: 01 Feb 2022 15:17


Tgt Ion:164 Resp: 268399
Ion Ratio Lower Upper
164 100
162 100.1 81.4 122.0
160 42.5 36.6 54.8

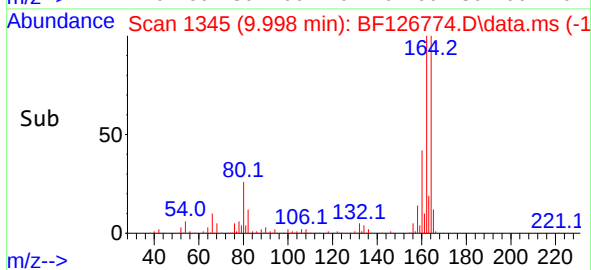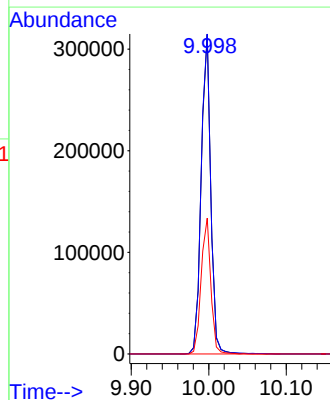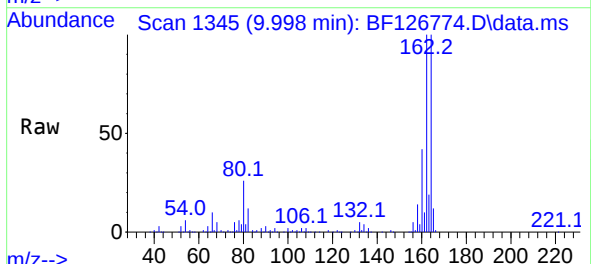



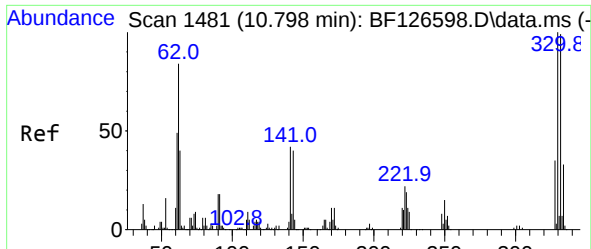


#42
2,4,6-Tribromophenol
Concen: 115.276 ng
RT: 10.786 min Scan# 1481
Delta R.T. -0.006 min
Lab File: BF126774.D
Acq: 01 Feb 2022 15:17

Instrument :
BNA_F
ClientSampleId :
SB-7(1.5-2)



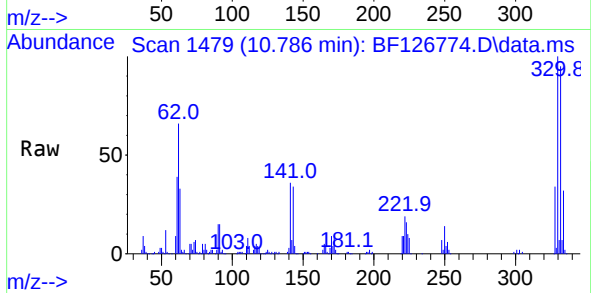



Tgt Ion:330 Resp: 289551
Ion Ratio Lower Upper
330 100
332 96.2 76.0 114.0
141 32.2 30.1 45.1

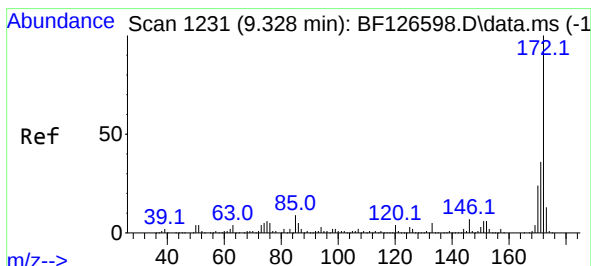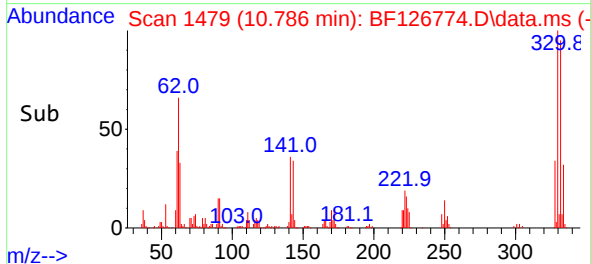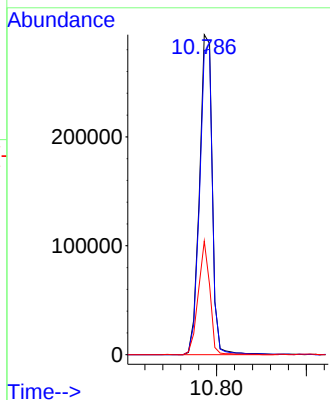

#45
2-Fluorobiphenyl
Concen: 67.846 ng
RT: 9.316 min Scan# 1229
Delta R.T. -0.000 min
Lab File: BF126774.D
Acq: 01 Feb 2022 15:17

Tgt Ion:172 Resp: 1189017
Ion Ratio Lower Upper
172 100
171 34.9 28.3 42.5
170 24.2 19.0 28.6


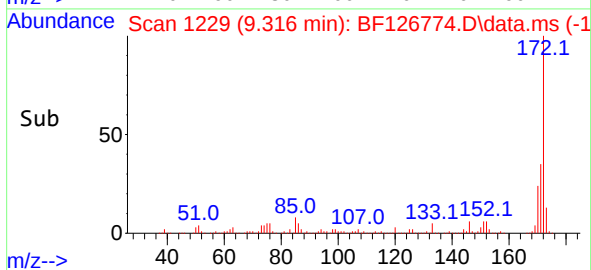
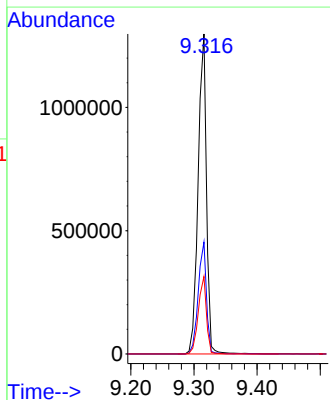
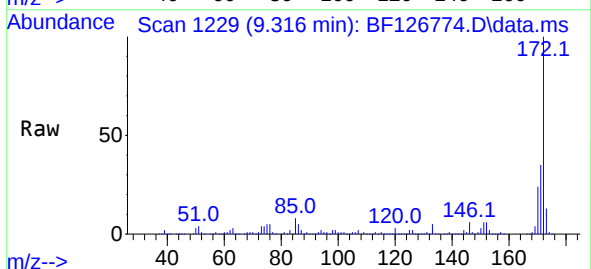


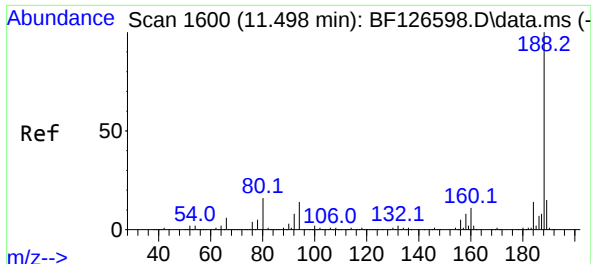

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.486 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF126774.D
Acq: 01 Feb 2022 15:17




Instrument :
BNA_F
ClientSampleId :
SB-7(1.5-2)

Tgt Ion:188 Resp: 466208
Ion Ratio Lower Upper
188 100
94 13.8 10.1 15.1
80 16.4 11.8 17.6

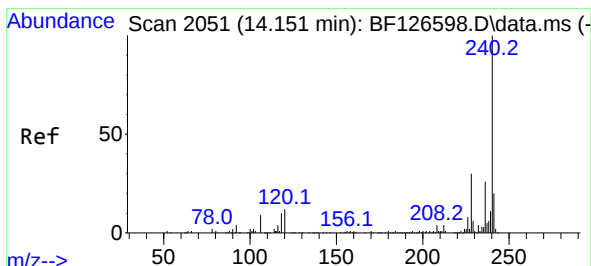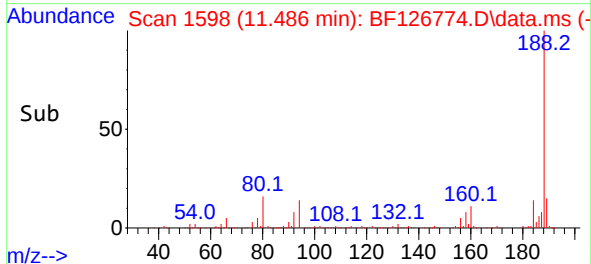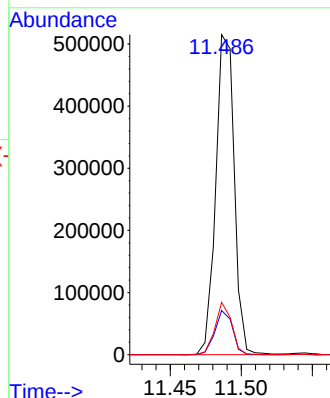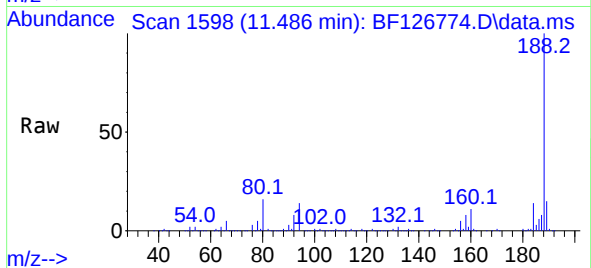

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.139 min Scan# 2049
Delta R.T. -0.006 min
Lab File: BF126774.D
Acq: 01 Feb 2022 15:17


Tgt Ion:240 Resp: 277596
Ion Ratio Lower Upper
240 100
120 10.9 14.4 21.6#
236 24.8 20.5 30.7

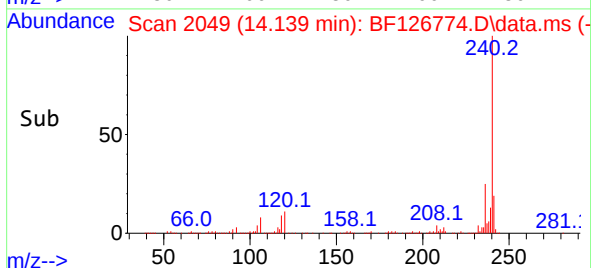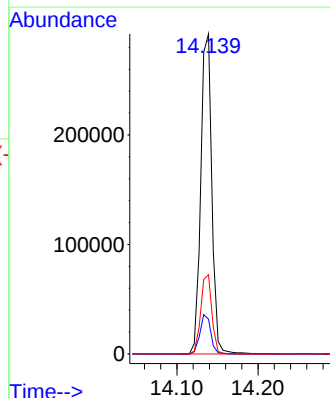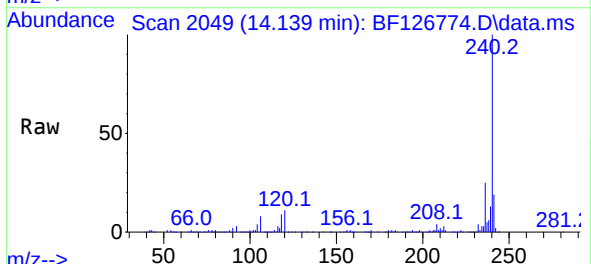






#79
 Terphenyl-d14
 Concen: 77.780 ng
 RT: 13.080 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: BF126774.D
 Acq: 01 Feb 2022 15:17

Instrument :
 BNA_F
 ClientSampleId :
 SB-7(1.5-2)

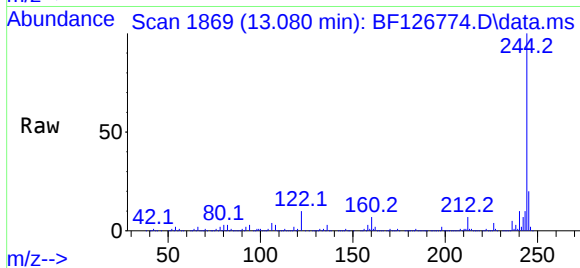

Tgt Ion:244 Resp: 1287307
 Ion Ratio Lower Upper
 244 100
 212 7.1 5.0 7.4
 122 10.5 13.3 19.9#

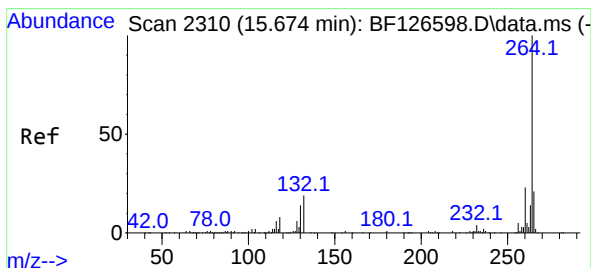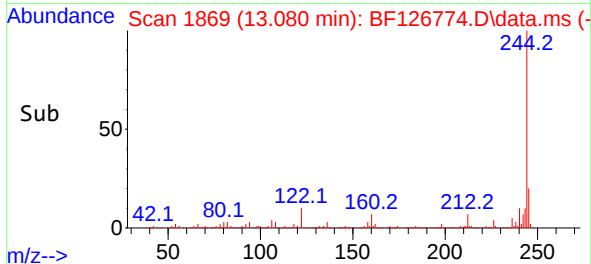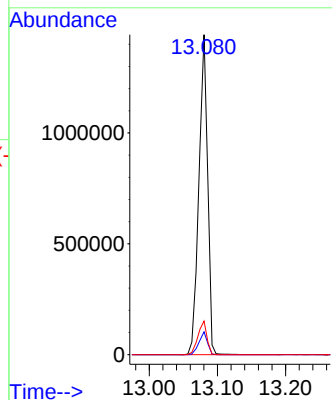

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.656 min Scan# 2307
 Delta R.T. -0.006 min
 Lab File: BF126774.D
 Acq: 01 Feb 2022 15:17

Tgt Ion:264 Resp: 228918
 Ion Ratio Lower Upper
 264 100
 260 23.1 19.2 28.8
 265 20.6 17.4 26.2

