
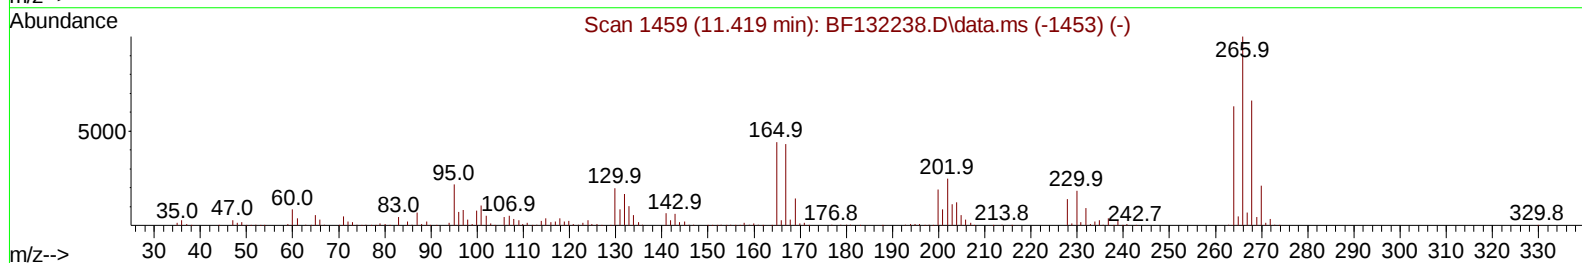
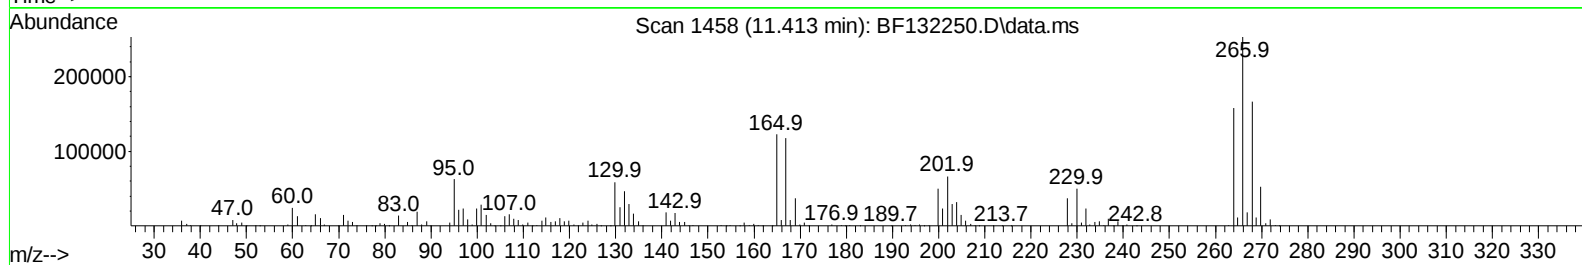


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020123\
Data File : BF132250.D
Acq On : 01 Feb 2023 09:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 02 05:27:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 02 01:30:34 2023
Response via : Initial Calibration

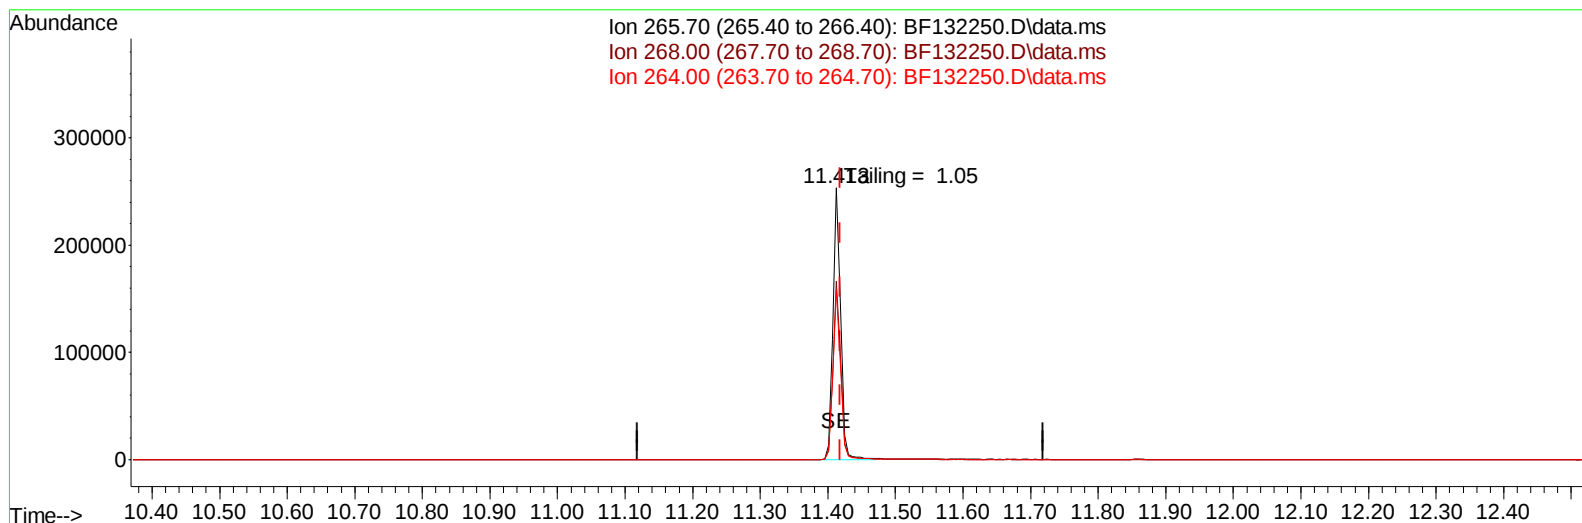

TIC: BF132250.D\data.ms

(70) Pentachlorophenol (C)




11.413min (-0.006) 34115.88 ng

response 202678

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	65.73
264.00	63.10	62.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020123\
Data File : BF132250.D
Acq On : 01 Feb 2023 09:37
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 02 05:27:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 02 01:30:34 2023
Response via : Initial Calibration

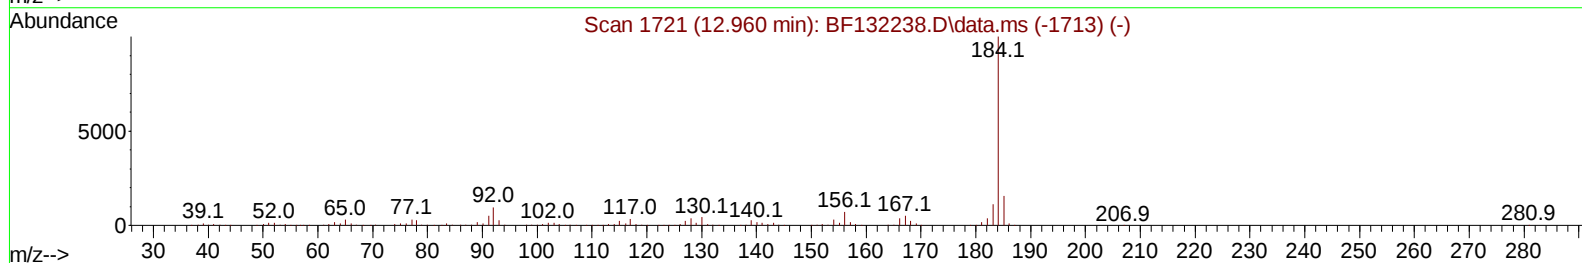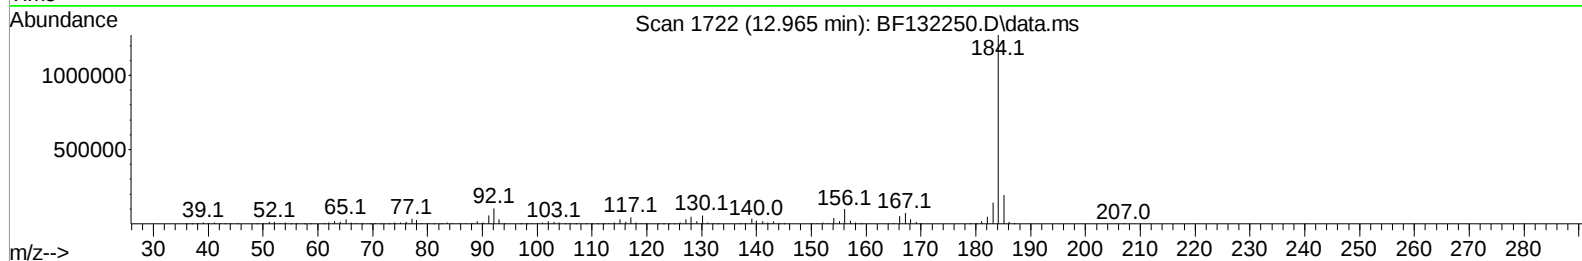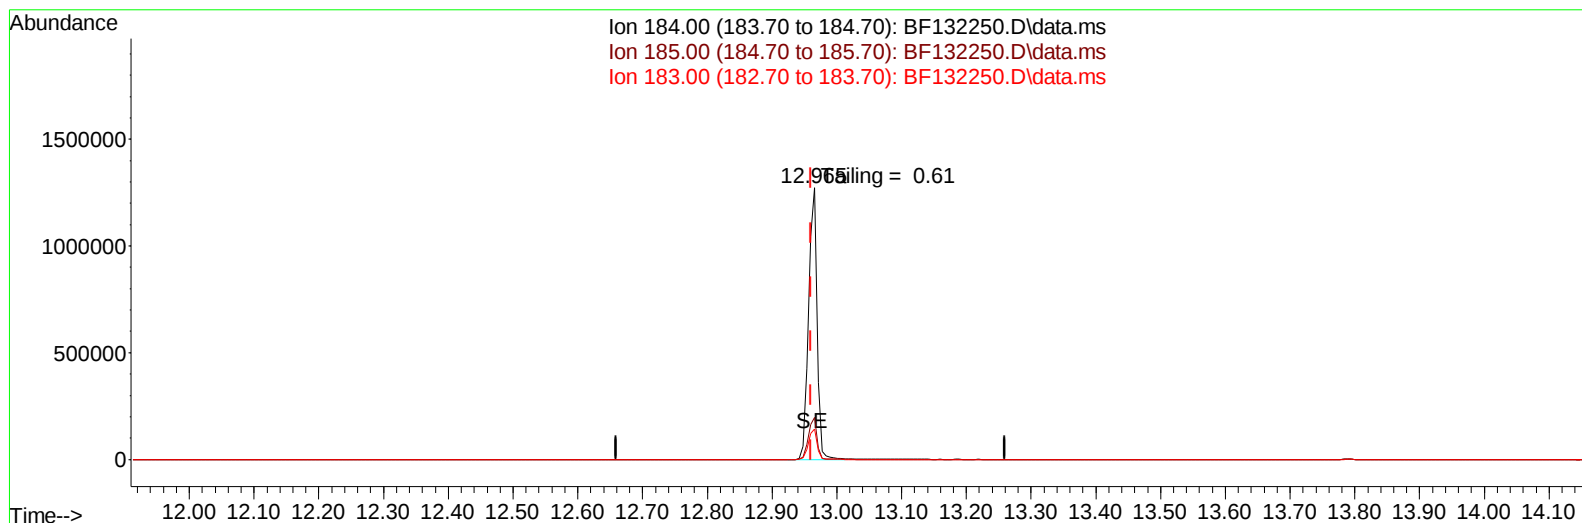

TIC: BF132250.D\data.ms

(77) Benzidine**12.965min (+ 0.005) 0.00 ng****response 1158820**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	15.38
183.00	11.10	11.32
0.00	0.00	0.00