


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020123\
Data File : BF132250.D
Acq On : 01 Feb 2023 09:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 02 01:30:34 2023

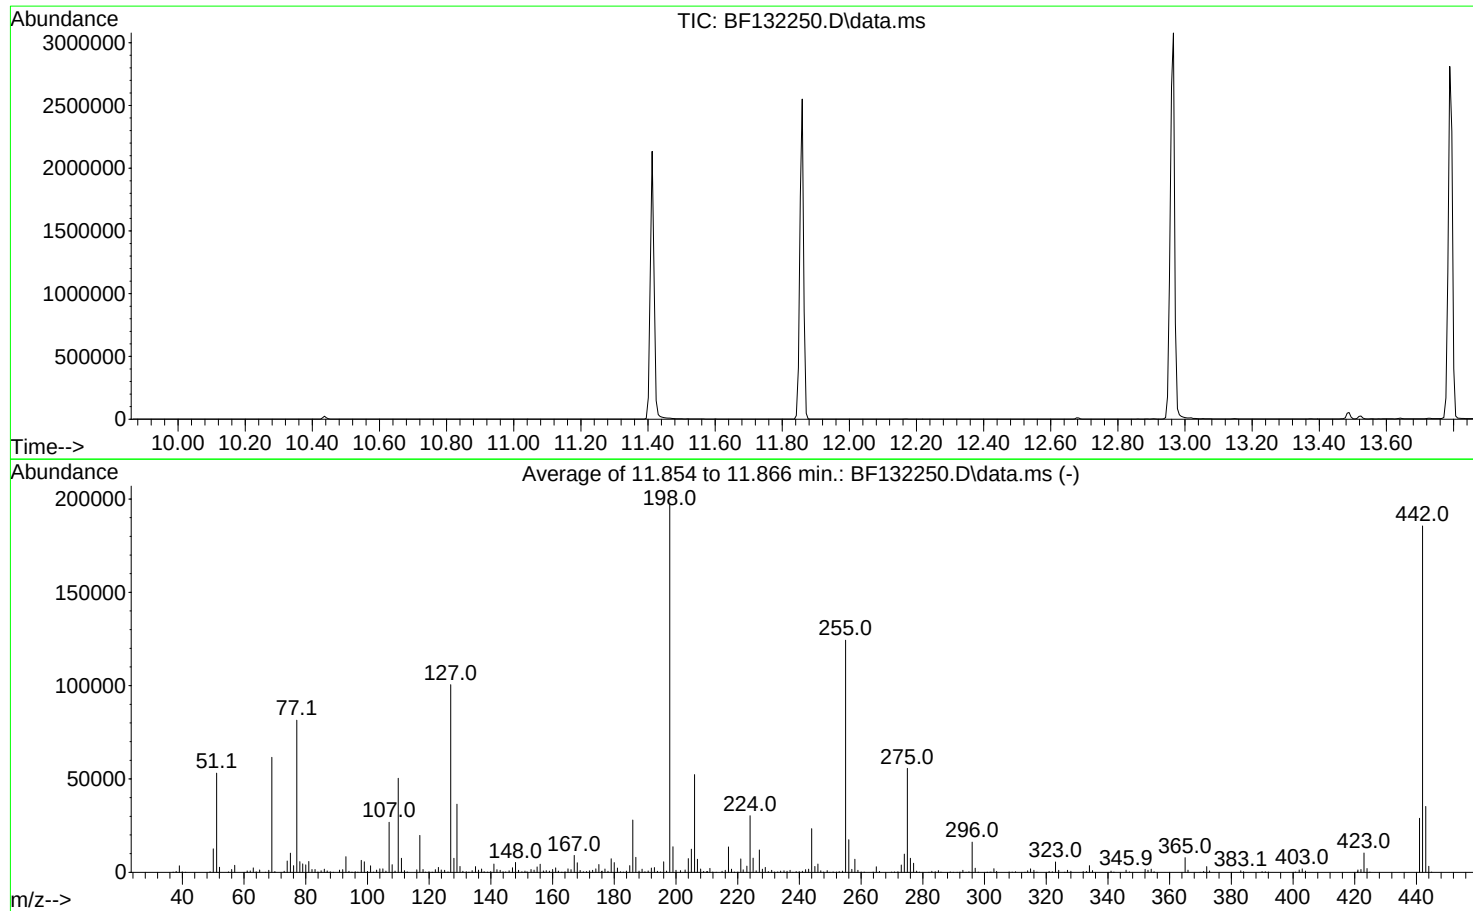




AutoFind: Scans 1533, 1534, 1535; Background Corrected with Scan 1528

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.0	53136	PASS
68	69	0.00	2	1.7	1046	PASS
69	198	0.00	100	31.3	61640	PASS
70	69	0.00	2	0.7	401	PASS
127	198	10	80	51.0	100493	PASS
197	198	0.00	2	0.3	653	PASS
198	198	100	100	100.0	197104	PASS
199	198	5	9	7.0	13701	PASS
275	198	10	60	28.2	55656	PASS
365	198	1	100	4.0	7814	PASS
441	198	0.01	100	14.7	28912	PASS
442	442	50	100	100.0	185589	PASS
443	442	15	24	19.0	35320	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020123\
Data File : BF132250.D
Acq On : 01 Feb 2023 09:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 02 05:27:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 02 01:30:34 2023
Response via : Initial Calibration

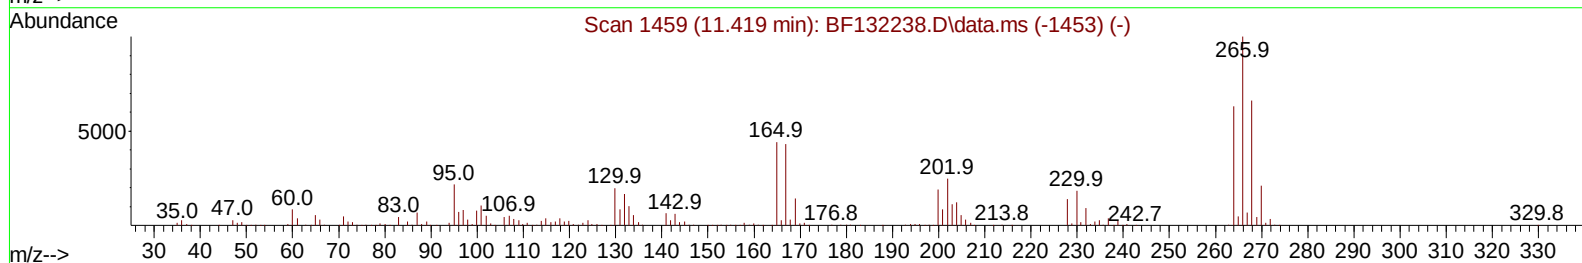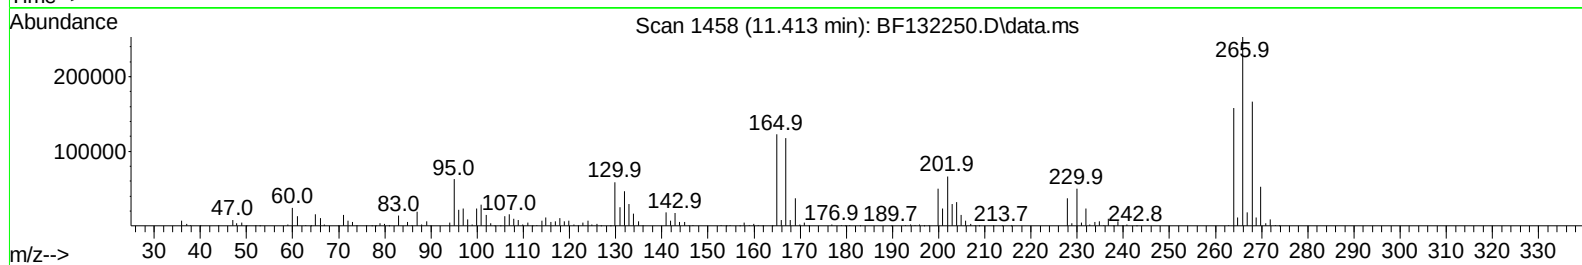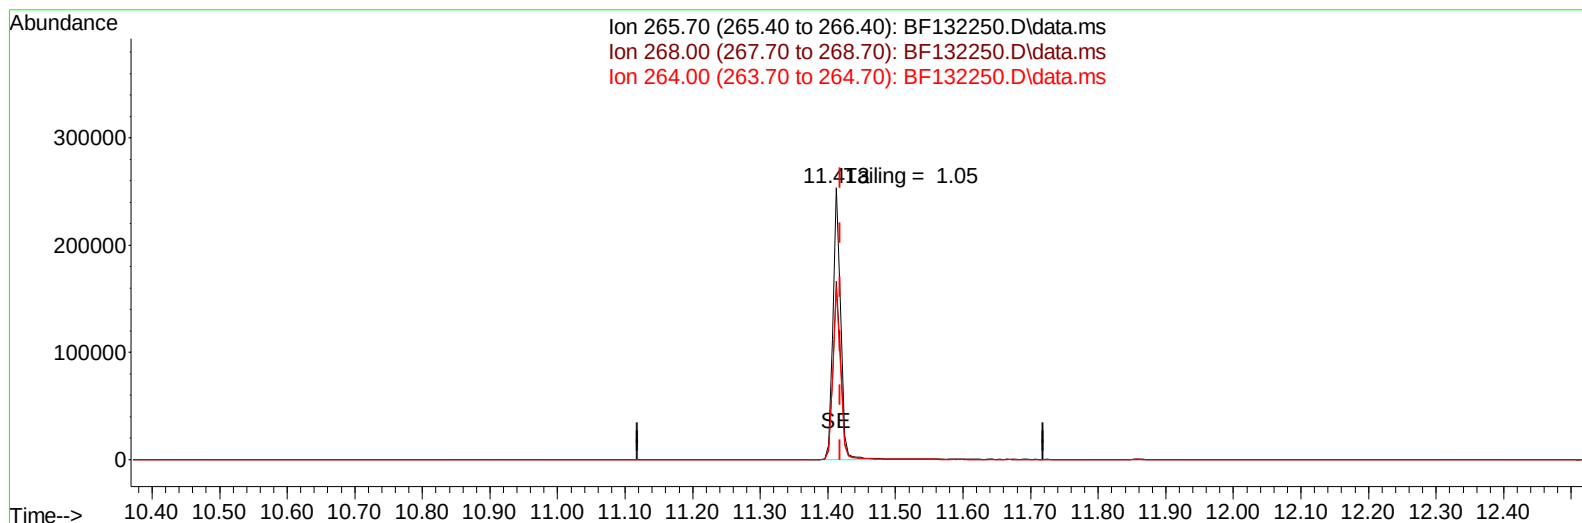

TIC: BF132250.D\data.ms

(70) Pentachlorophenol (C)

11.413min (-0.006) 34115.88 ng




response 202678

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	65.73
264.00	63.10	62.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020123\
Data File : BF132250.D
Acq On : 01 Feb 2023 09:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 02 05:27:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 02 01:30:34 2023
Response via : Initial Calibration

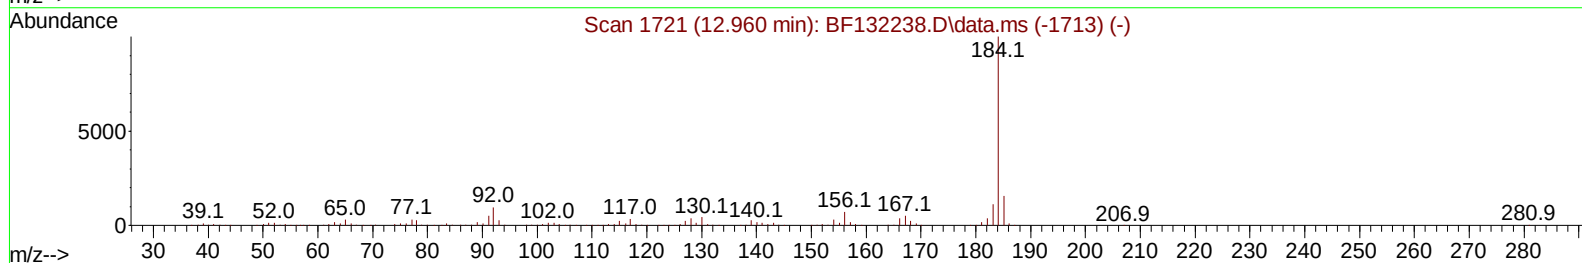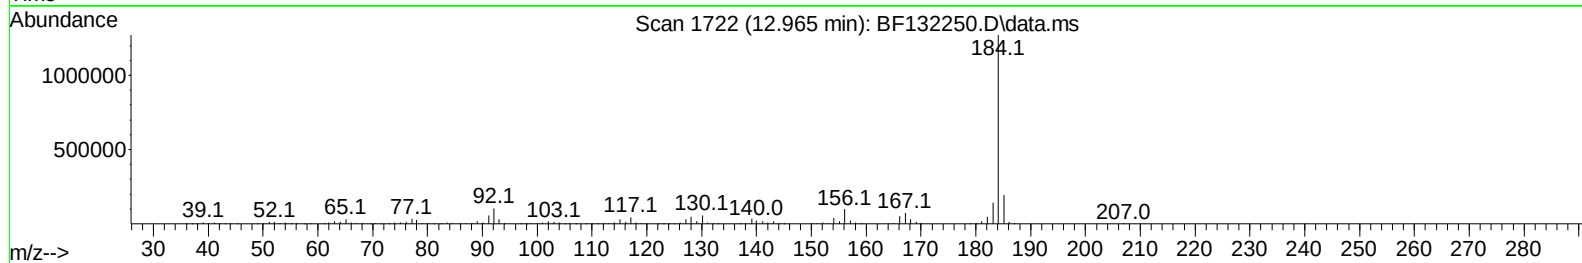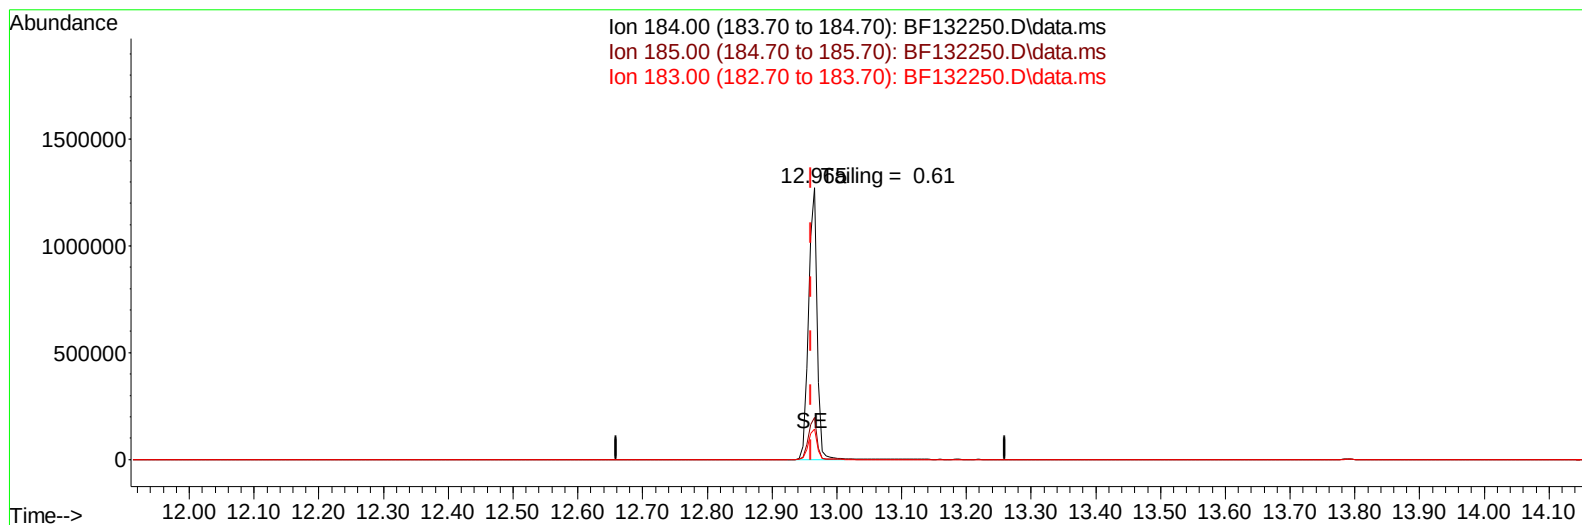

TIC: BF132250.D\data.ms

(77) Benzidine

12.965min (+ 0.005) 0.00 ng

response 1158820

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	15.38
183.00	11.10	11.32
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/1/2023	BNA_F	<u>BF132250.D</u>
Compound Name	Response	Retention Time
DDT	475773	13.789
DDD	13426	13.489
DDE	472	13.148
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13898	489671	2.84

Instrument :
BNA_F
ClientSampleId :
DFTPP